

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033952.D
 Acq On : 15 Sep 2024 15:15
 Operator : JU/RC
 Sample : P3922-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AT3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 01:26:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	4461	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	12562	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.124	164	6699	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.881	188	14272m	0.400	ng/ul	0.00
17) Chrysene-d12	21.098	240	12300m	0.400	ng/ul	0.00
23) Perylene-d12	23.240	264	12165m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	25276	5.511	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	5605	0.311	ng/ul	0.00
18) Fluoranthene-d10	18.920	212	15160	0.413	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.131	88	248	0.049	ng/ul#	49

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033952.D
Acq On : 15 Sep 2024 15:15
Operator : JU/RC
Sample : P3922-09
Misc :
ALS Vial : 43 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AT3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 16 01:26:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

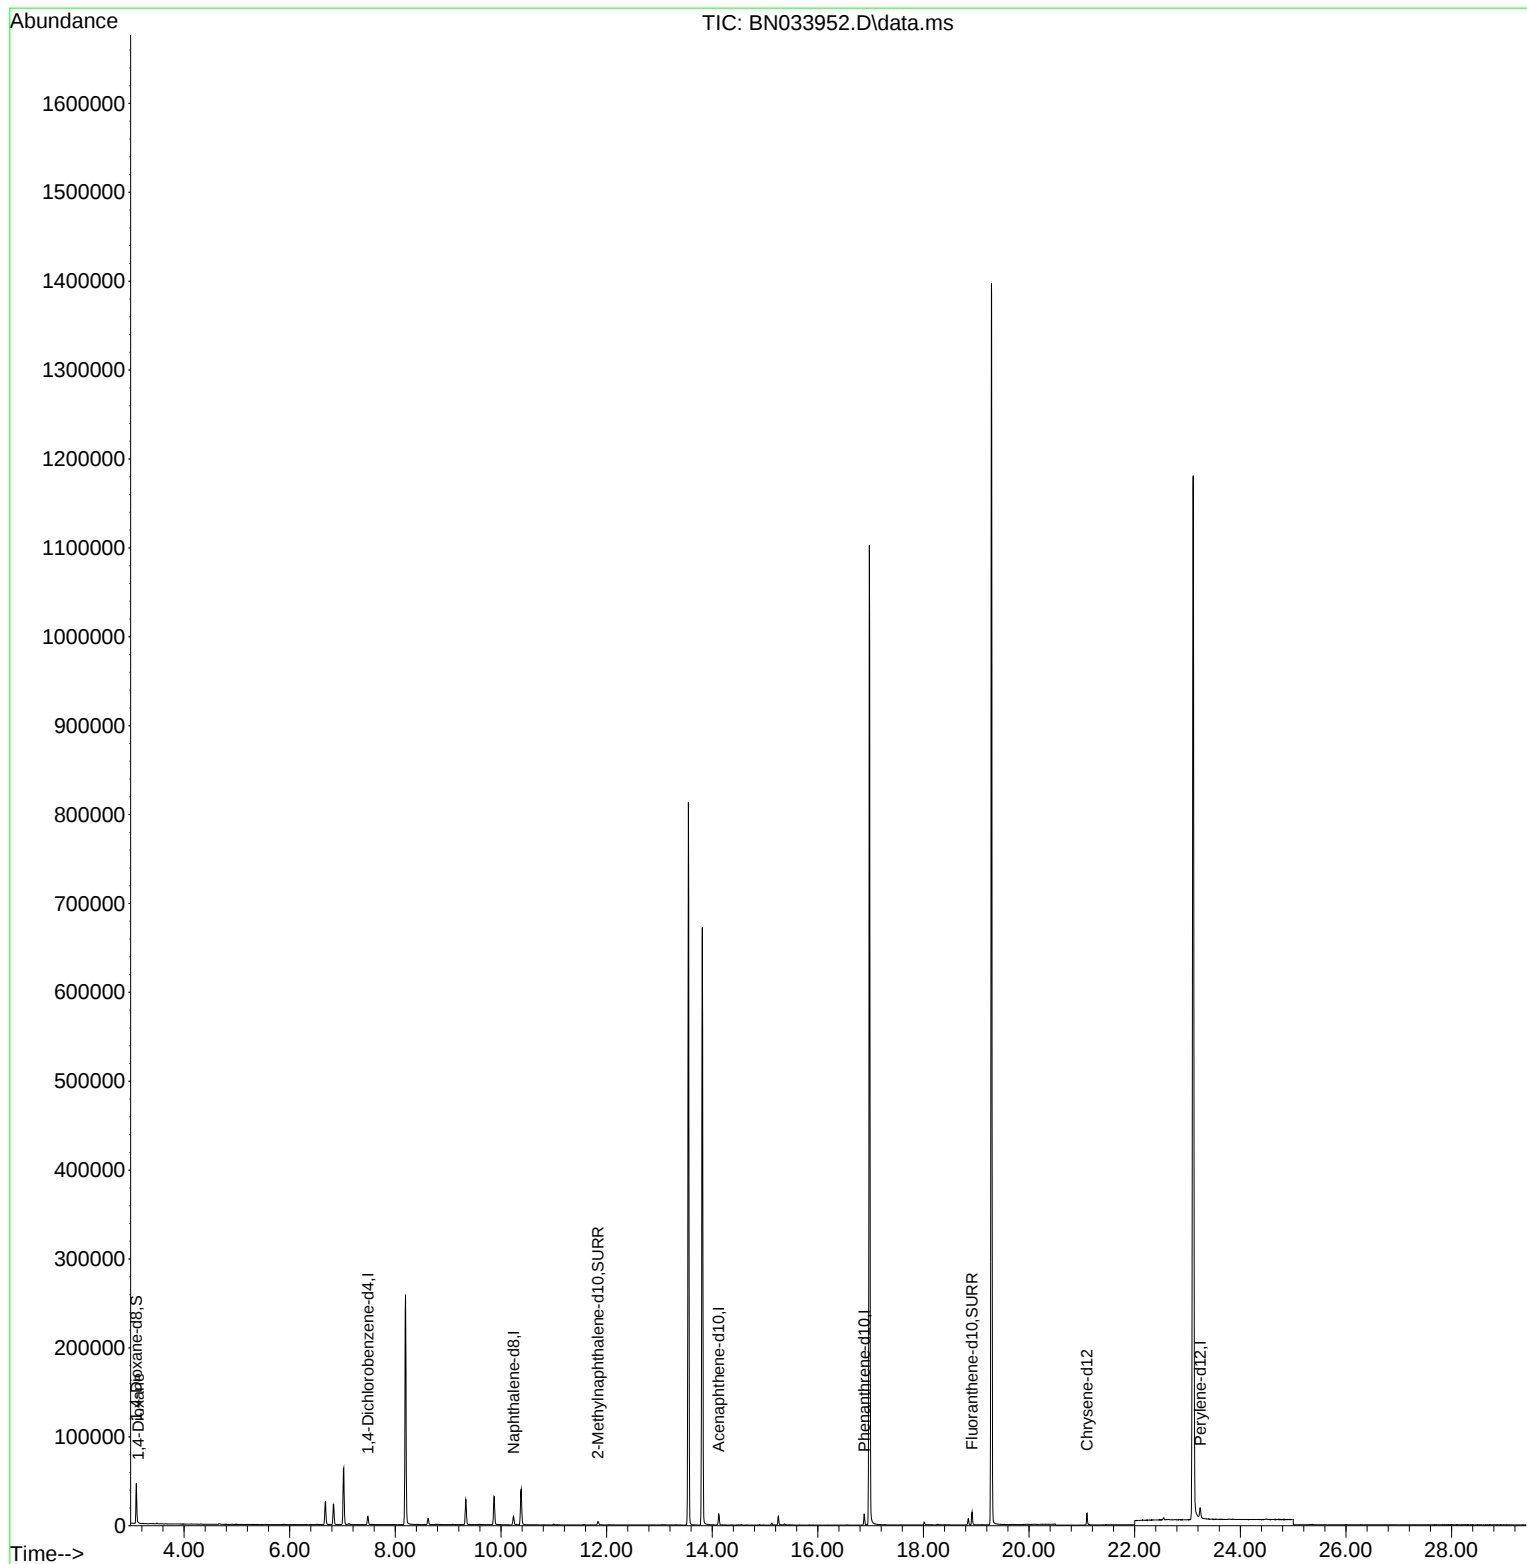

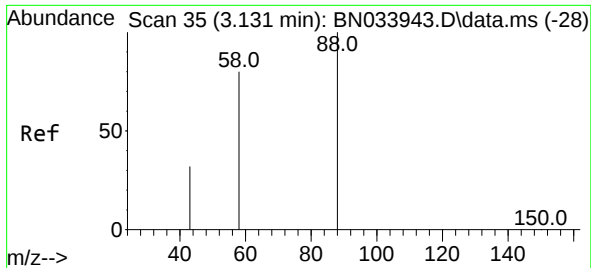

#2
 1,4-Dioxane
 Concen: 0.049 ng/ul
 RT: 3.131 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BN033952.D
 Acq: 15 Sep 2024 15:15

Instrument :
 BNA_N
 ClientSampleId :
 C0AT3

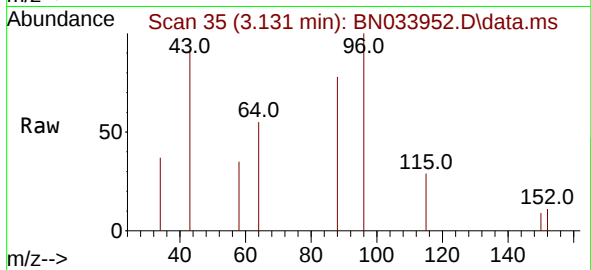

Tgt Ion: 88 Resp: 248

Ion	Ratio	Lower	Upper
88	100		
43	117.7	47.0	70.4
58	45.7	53.0	79.4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

