

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033965.D
 Acq On : 15 Sep 2024 23:39
 Operator : JU/RC
 Sample : P3997-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 00:15:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	5214	0.400	ng/ul	0.00
4) Naphthalene-d8	10.238	136	14828	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.122	164	7960	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.880	188	16562m	0.400	ng/ul	0.00
17) Chrysene-d12	21.096	240	14322m	0.400	ng/ul	0.00
23) Perylene-d12	23.235	264	14386m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	31251	5.830	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.838	152	6706	0.315	ng/ul	0.00
18) Fluoranthene-d10	18.919	212	17040	0.399	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.131	88	2290	0.385	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033965.D
Acq On : 15 Sep 2024 23:39
Operator : JU/RC
Sample : P3997-08
Misc :
ALS Vial : 57 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AQ7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 16 00:15:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

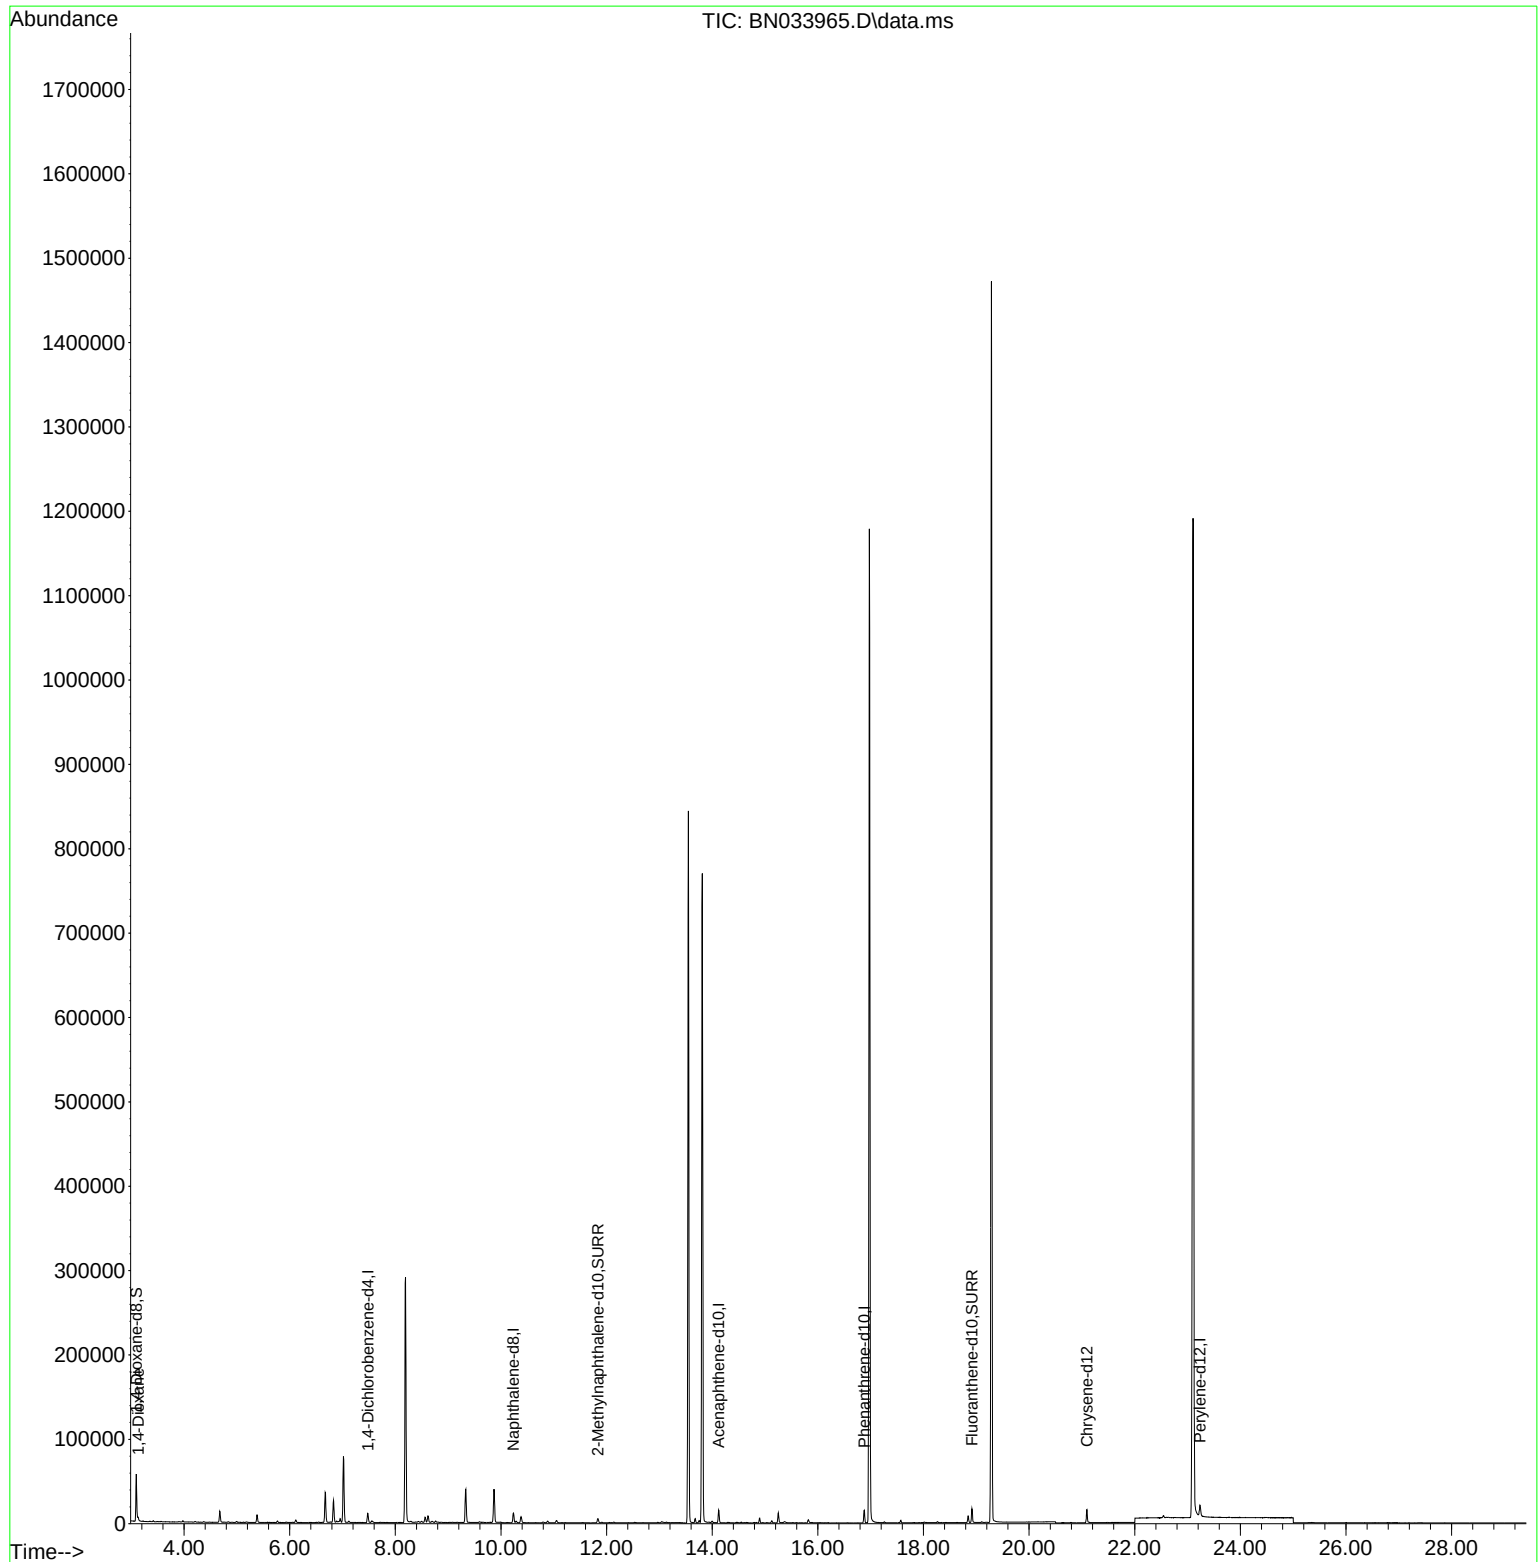

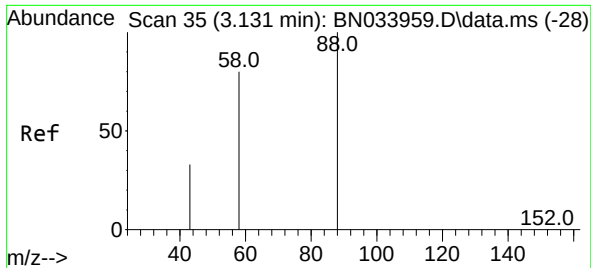

#2
 1,4-Dioxane
 Concen: 0.385 ng/ul
 RT: 3.131 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN033965.D
 Acq: 15 Sep 2024 23:39

Instrument :
 BNA_N
 ClientSampleId :
 C0AQ7

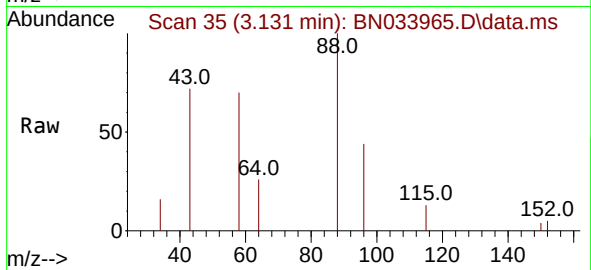

Tgt Ion: 88	Resp: 2290
Ion Ratio	Lower Upper
88 100	
43 72.1	47.0 70.4
58 69.8	53.0 79.4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

