

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
 Data File : BN033968.D
 Acq On : 16 Sep 2024 01:27
 Operator : JU/RC
 Sample : P3952-16
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B20

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 04:11:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.481	152	5541	0.400	ng/ul	0.00
4) Naphthalene-d8	10.239	136	16017	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.124	164	8747	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.877	188	18743m	0.400	ng/ul	0.00
17) Chrysene-d12	21.092	240	15920m	0.400	ng/ul	0.00
23) Perylene-d12	23.234	264	16511m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	21973	3.857	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	7365	0.320	ng/ul	0.00
18) Fluoranthene-d10	18.920	212	20234	0.426	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.131	88	12694	2.008	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091424\
Data File : BN033968.D
Acq On : 16 Sep 2024 01:27
Operator : JU/RC
Sample : P3952-16
Misc :
ALS Vial : 60 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0B20

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 16 04:11:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

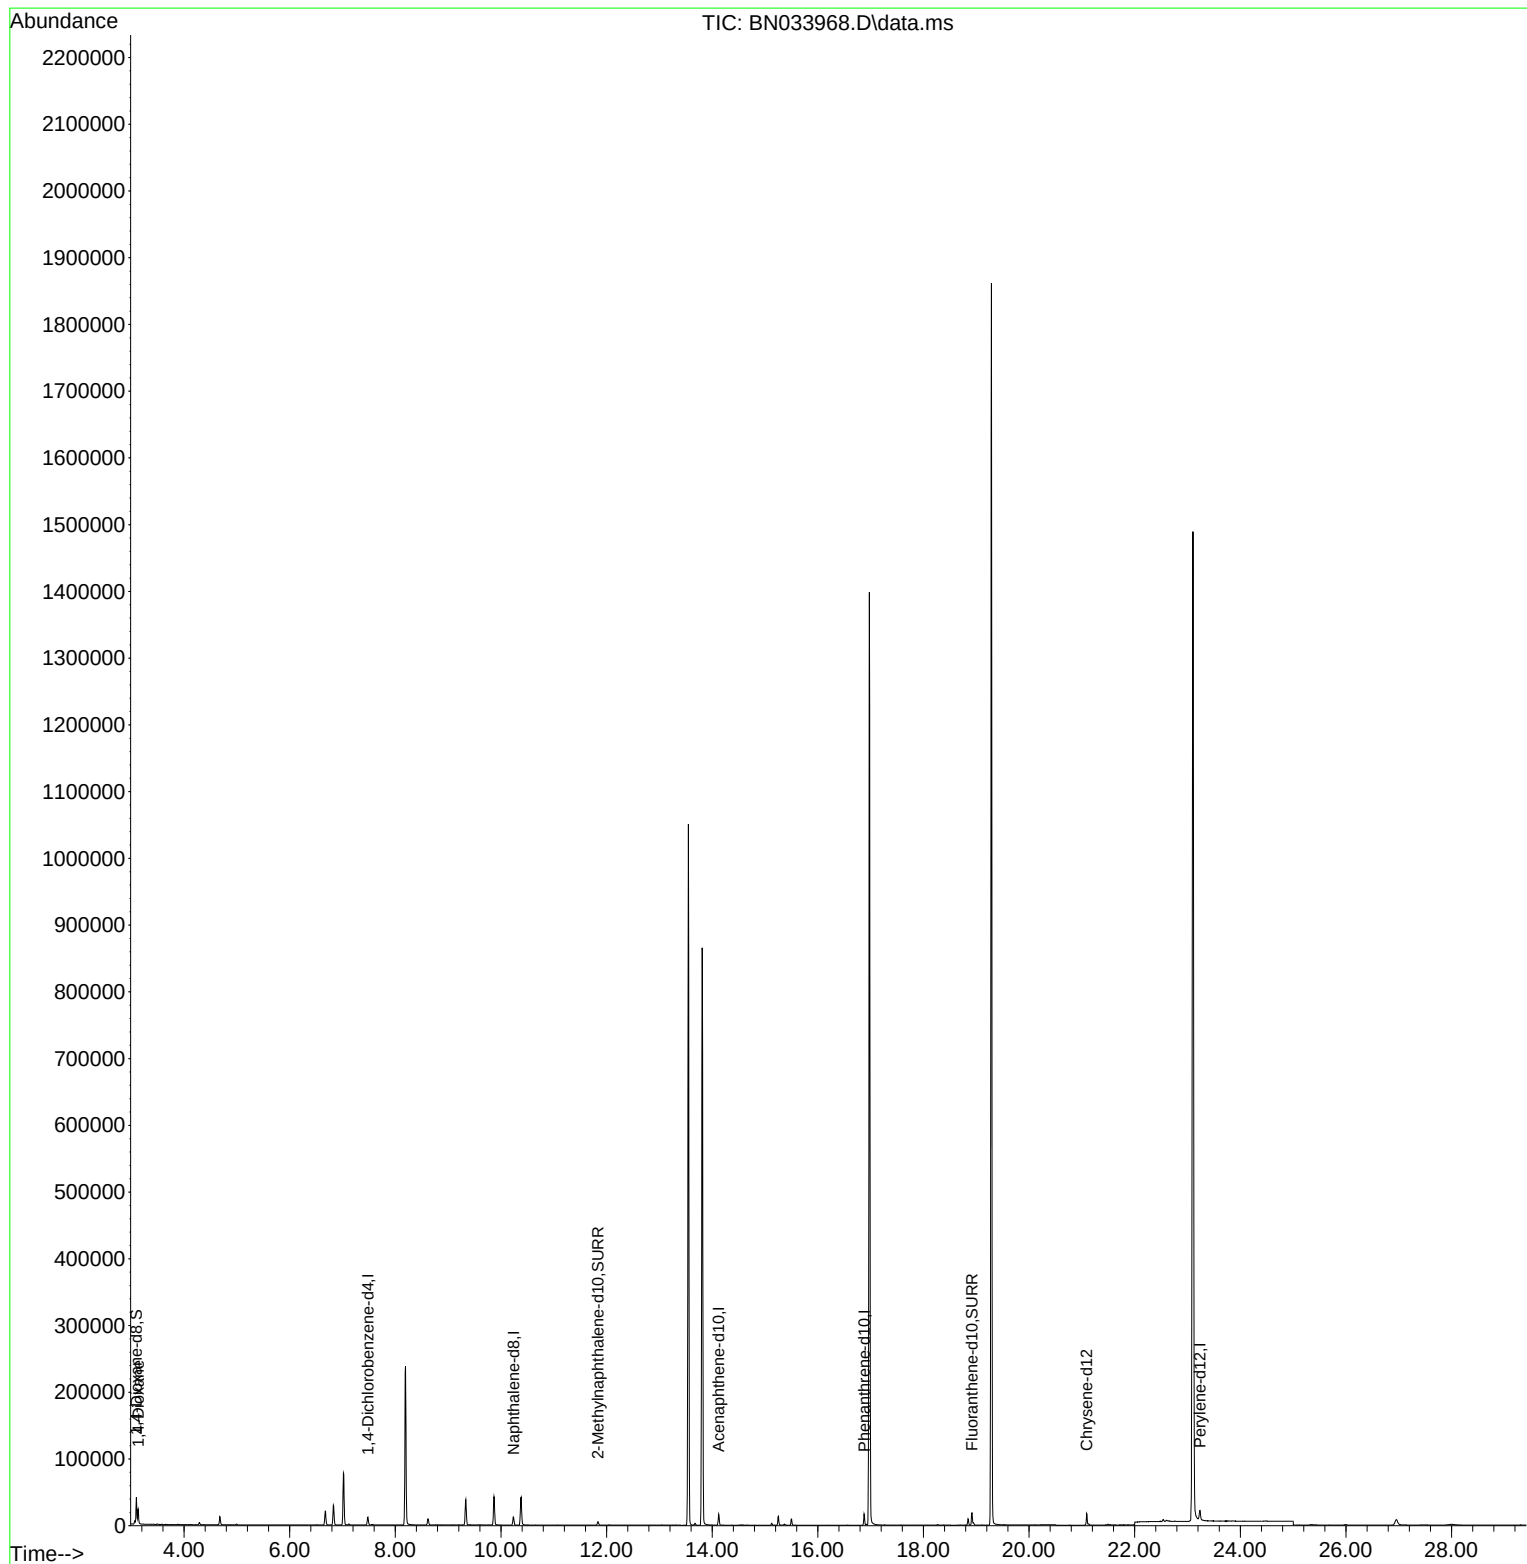

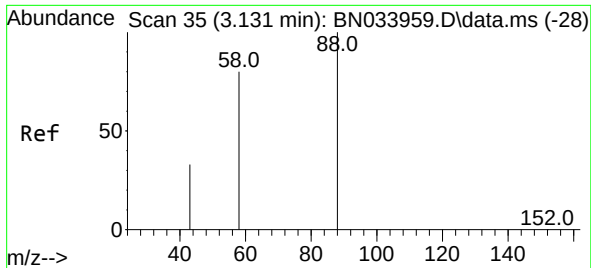

#2
 1,4-Dioxane
 Concen: 2.008 ng/ul
 RT: 3.131 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN033968.D
 Acq: 16 Sep 2024 01:27

Instrument :
 BNA_N
 ClientSampleId :
 C0B20

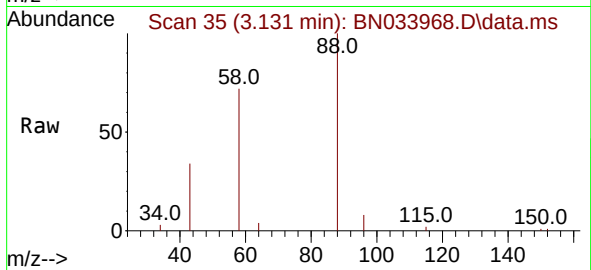

Tgt Ion: 88 Resp: 12694
 Ion Ratio Lower Upper
 88 100
 43 33.5 47.0 70.4
 58 72.5 53.0 79.4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/16/2024
 Supervised By :mohammad ahmed 09/17/2024

