

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027700.D
 Acq On : 15 Sep 2023 18:22
 Operator : MA/JU
 Sample : PB155434BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK434

Quant Time: Sep 16 01:31:40 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.017	152	4746	0.400	ng/ul	0.00
4) Naphthalene-d8	10.839	136	15720	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.652	164	9561	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.401	188	21373	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	16769	0.400	ng/ul	0.00
23) Perylene-d12	24.076	264	17814	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	36896	6.172	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.418	152	7641	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	19198	0.375	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.642	166	3049	0.072	ng/ul#	15
20) Pyrene	19.794	202	3106	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.916	252	7140	0.112	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027700.D
Acq On : 15 Sep 2023 18:22
Operator : MA/JU
Sample : PB155434BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK434

Quant Time: Sep 16 01:31:40 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration




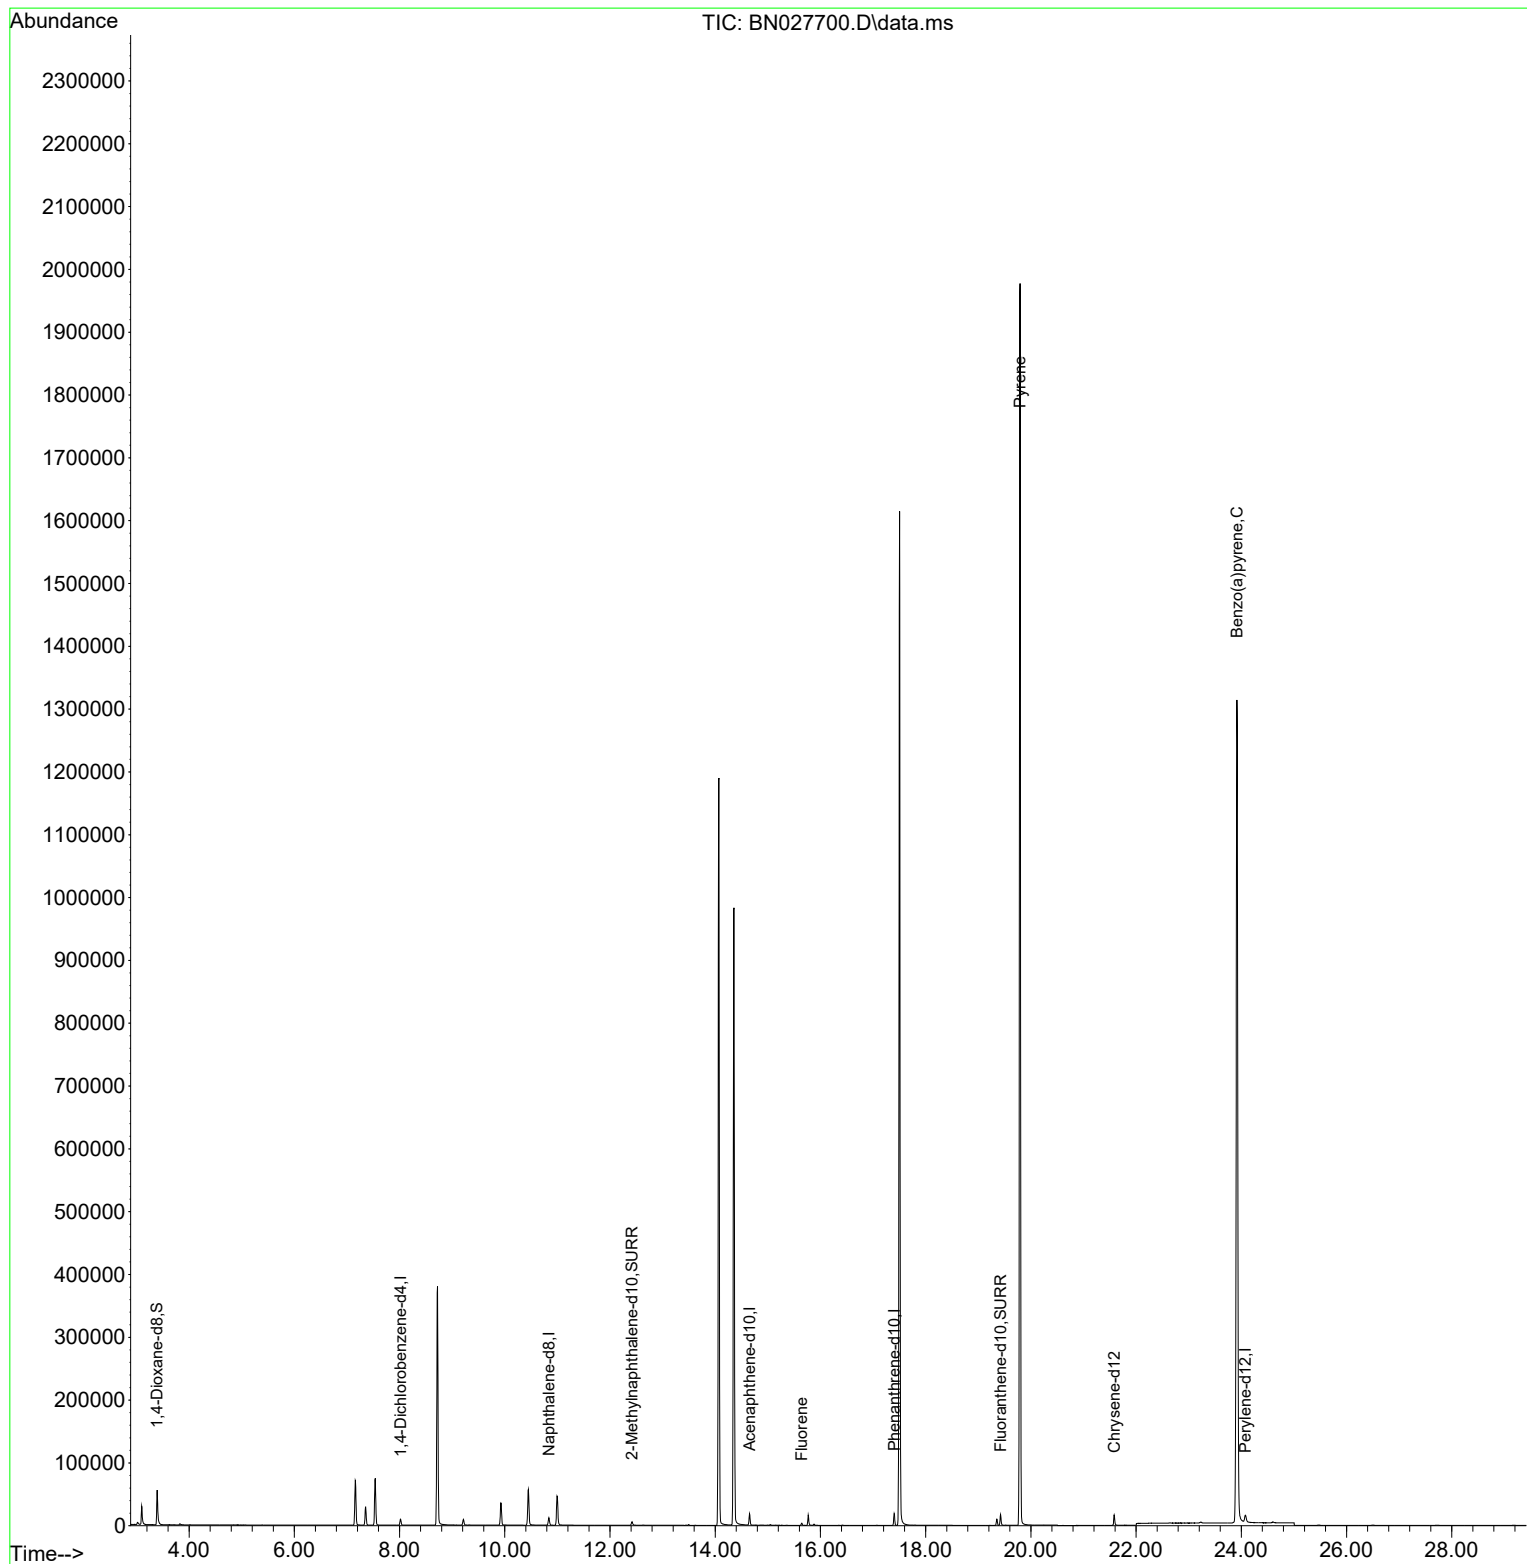


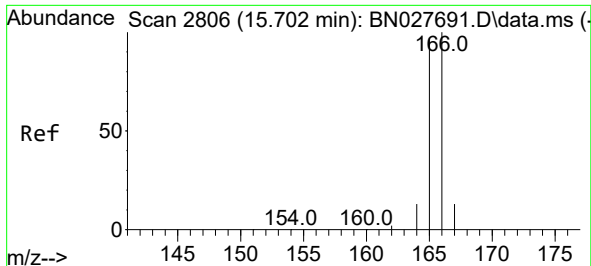

#12
Fluorene
Concen: 0.072 ng/ul
RT: 15.642 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN027700.D
Acq: 15 Sep 2023 18:22




Instrument :
BNA_N
ClientSampleId :
SBLK434


Tgt Ion:166 Resp: 3049
Ion Ratio Lower Upper
166 100
165 7.0 78.0 117.0#
167 31.7 11.4 17.2#

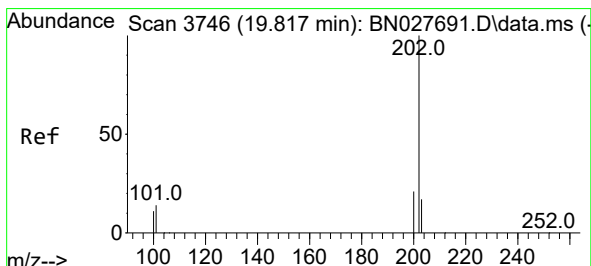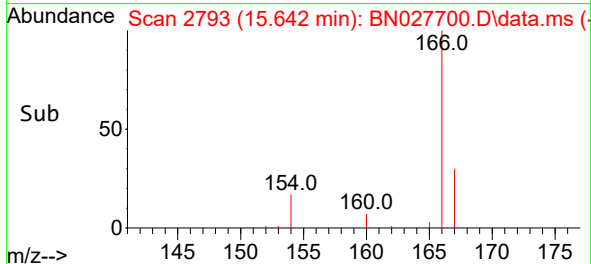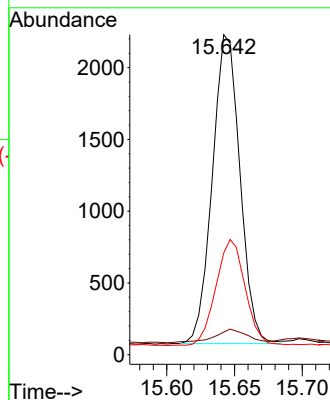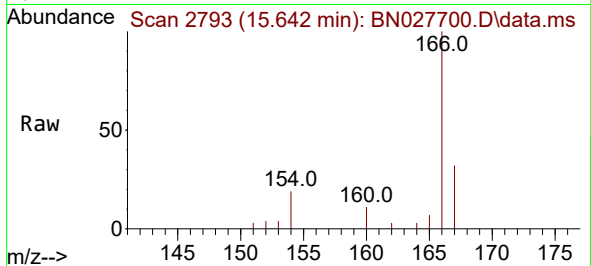

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.794 min Scan# 3741
Delta R.T. -0.023 min
Lab File: BN027700.D
Acq: 15 Sep 2023 18:22


Tgt Ion:202 Resp: 3106
Ion Ratio Lower Upper
202 100
101 163.9 11.4 17.0#
100 1186.1 9.1 13.7#

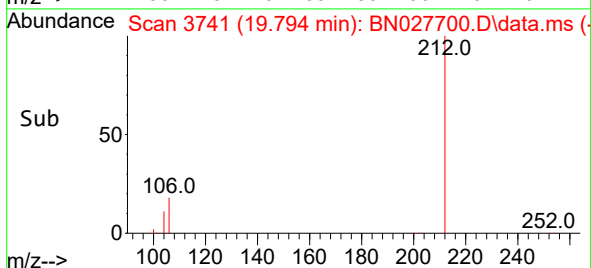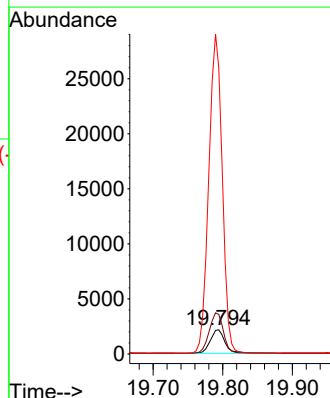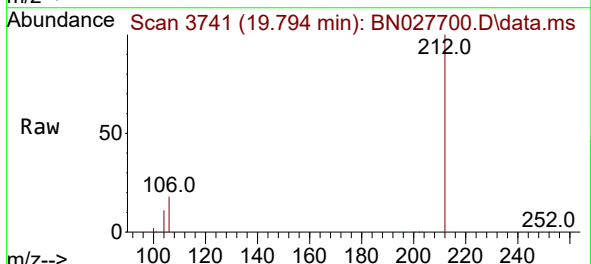

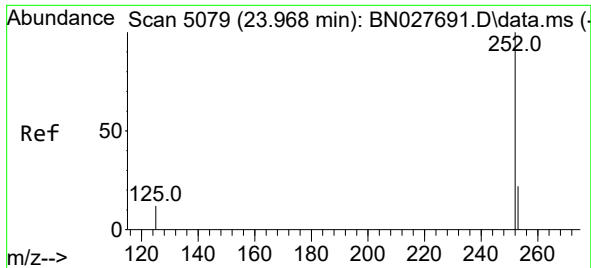

#26
Benzo(a)pyrene
Concen: 0.112 ng/ul
RT: 23.916 min Scan# 50
Delta R.T. -0.053 min
Lab File: BN027700.D
Acq: 15 Sep 2023 18:22

Instrument :
BNA_N
ClientSampleId :
SBLK434

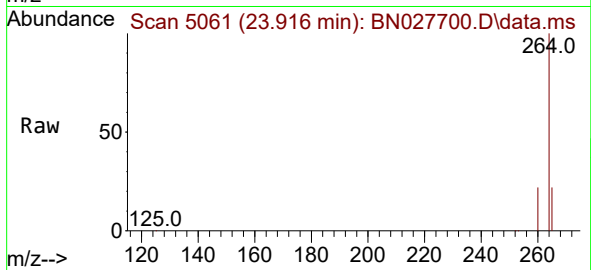

Tgt Ion:252 Resp: 7140
Ion Ratio Lower Upper
252 100
253 42.8 21.9 32.9#
125 38.7 15.5 23.3#

