

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027702.D
 Acq On : 15 Sep 2023 19:36
 Operator : MA/JU
 Sample : 04324-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJA8

Quant Time: Sep 16 01:31:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.017	152	4842	0.400	ng/ul	0.00
4) Naphthalene-d8	10.839	136	16402	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.652	164	10038	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.400	188	22290	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	18414	0.400	ng/ul	0.00
23) Perylene-d12	24.076	264	19218	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	26674	4.373	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.418	152	8889	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	23779	0.423	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.431	88	187	0.029	ng/ul#	45
20) Pyrene	19.794	202	3926	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.918	252	8347	0.121	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027702.D
Acq On : 15 Sep 2023 19:36
Operator : MA/JU
Sample : 04324-20
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJA8

Quant Time: Sep 16 01:31:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration




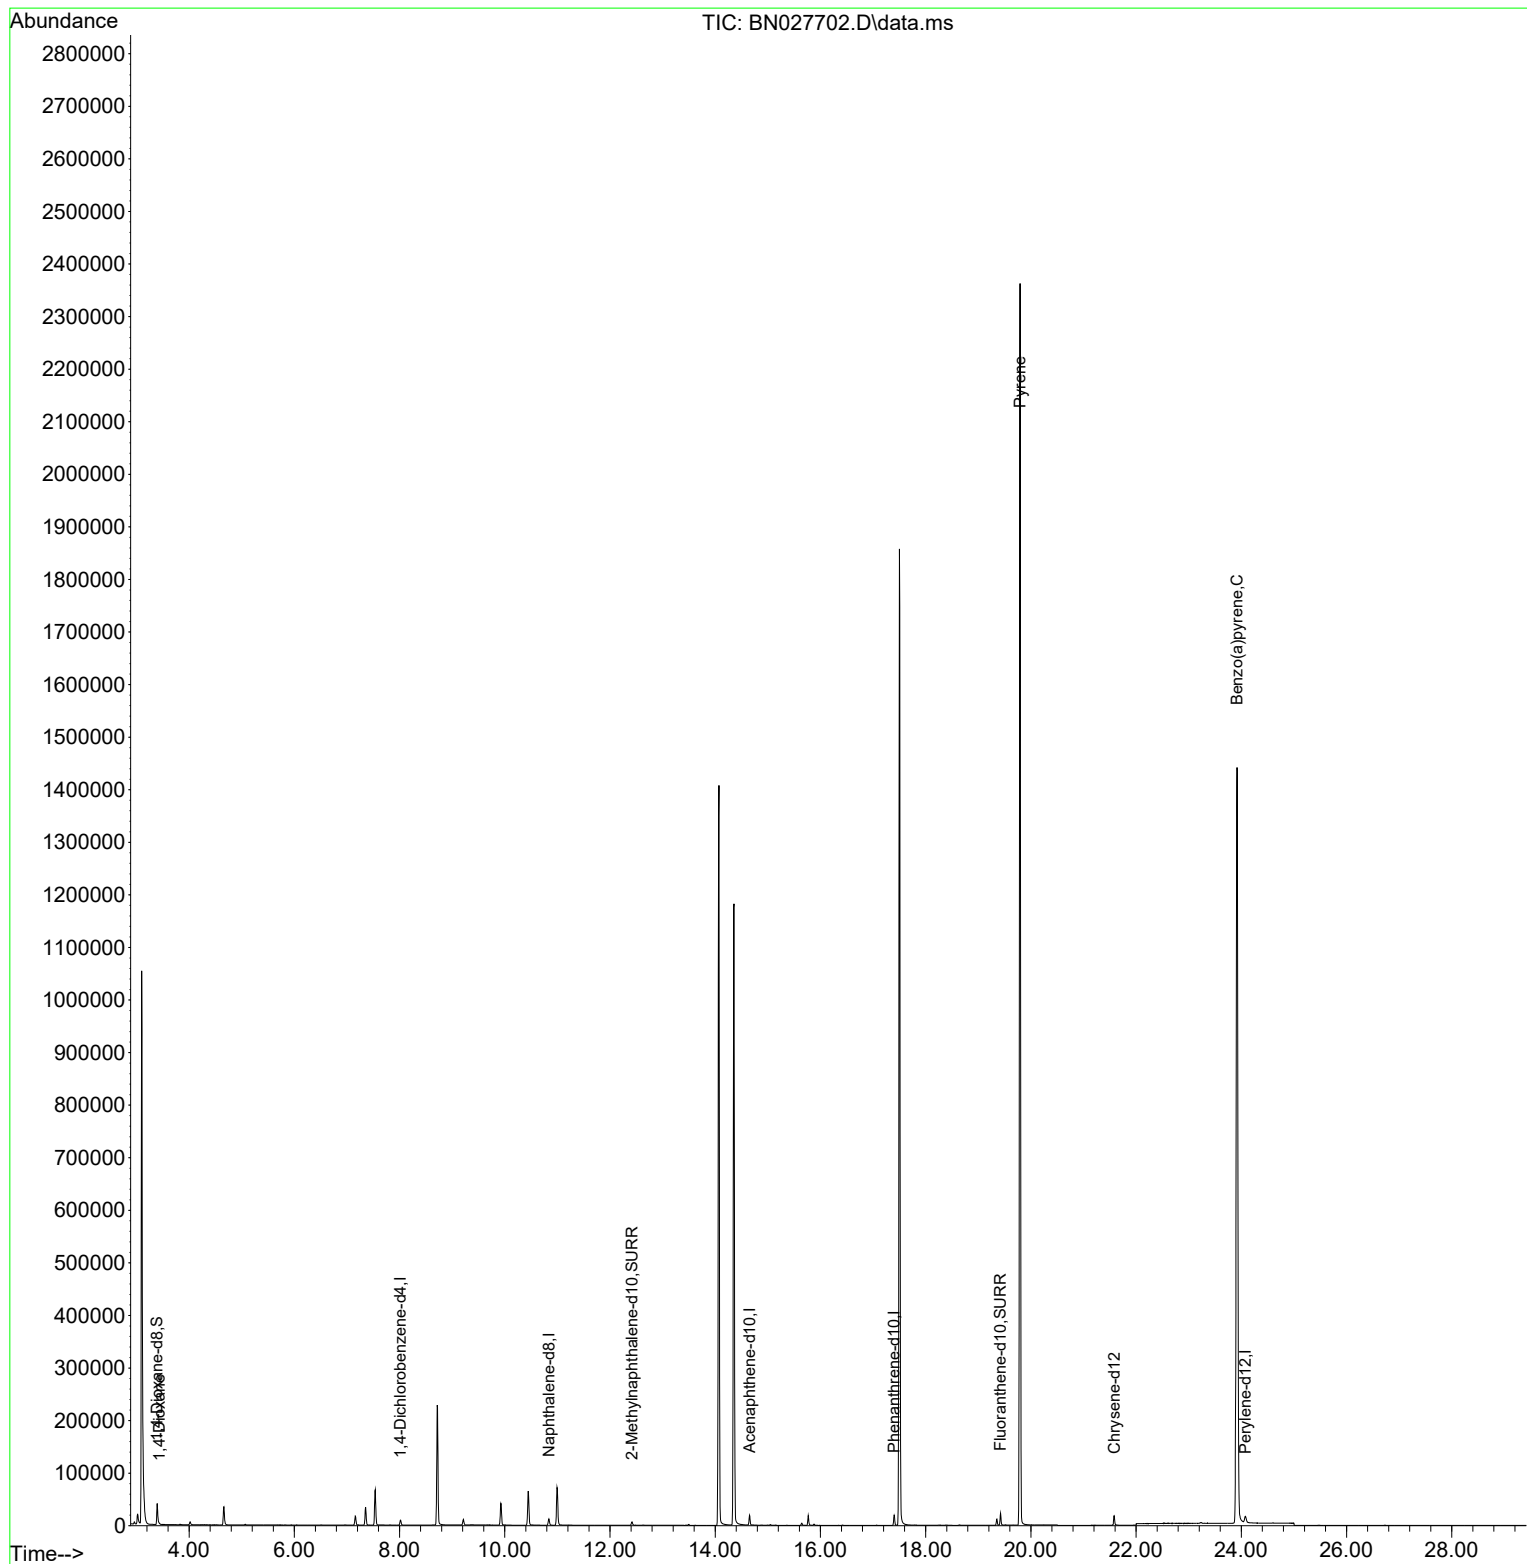


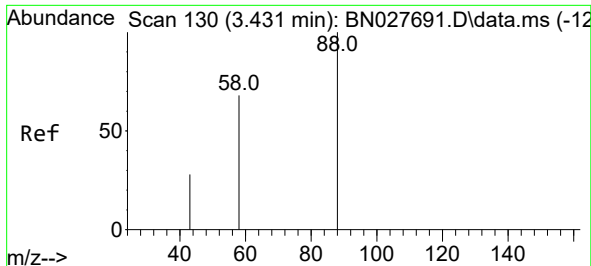

#2
1,4-Dioxane
Concen: 0.029 ng/ul
RT: 3.431 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN027702.D
Acq: 15 Sep 2023 19:36




Instrument :
BNA_N
ClientSampleId :
BBJA8


Tgt Ion: 88 Resp: 187
Ion Ratio Lower Upper
88 100
43 85.1 39.6 59.4#
58 16.7 48.3 72.5#

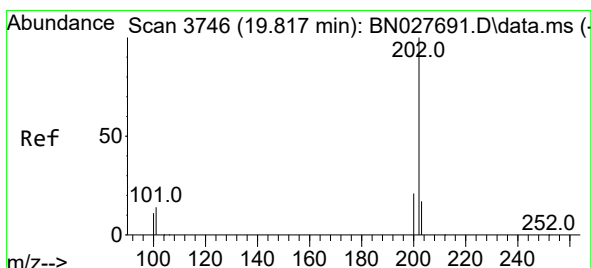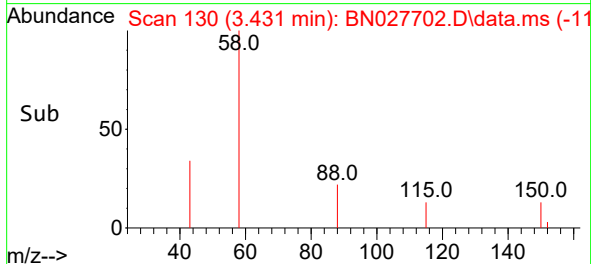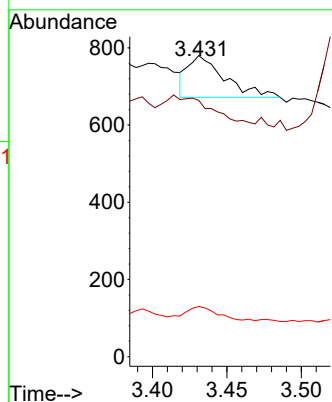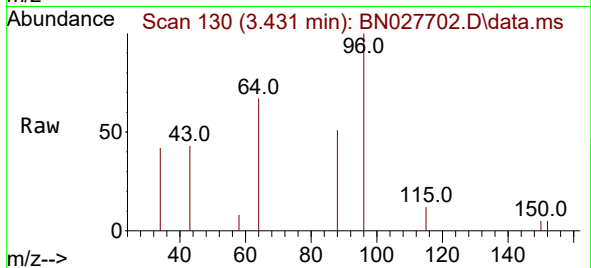

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.794 min Scan# 3741
Delta R.T. -0.024 min
Lab File: BN027702.D
Acq: 15 Sep 2023 19:36


Tgt Ion: 202 Resp: 3926
Ion Ratio Lower Upper
202 100
101 166.7 11.4 17.0#
100 1231.0 9.1 13.7#

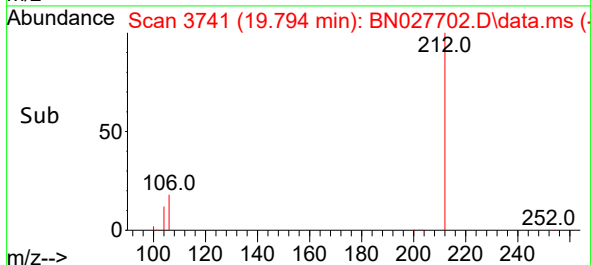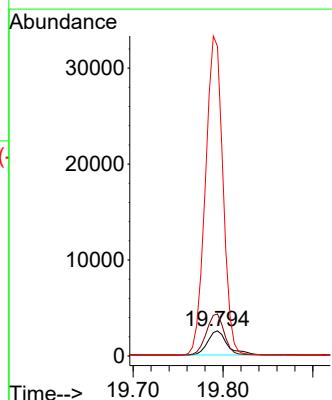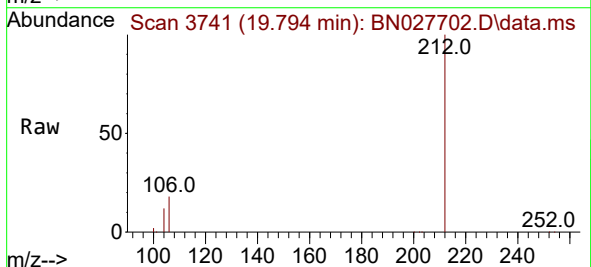

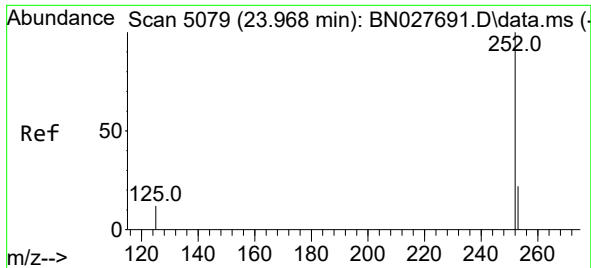

#26
Benzo(a)pyrene
Concen: 0.121 ng/ul
RT: 23.918 min Scan# 50
Delta R.T. -0.050 min
Lab File: BN027702.D
Acq: 15 Sep 2023 19:36

Instrument :
BNA_N
ClientSampleId :
BBJA8

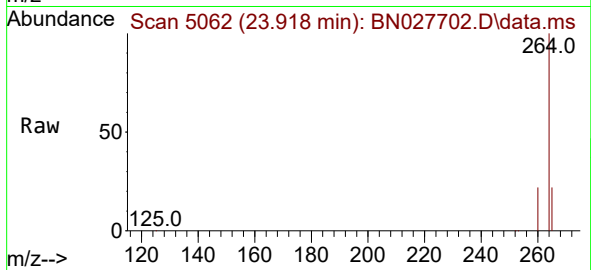

Tgt Ion:252 Resp: 8347
Ion Ratio Lower Upper
252 100
253 42.6 21.9 32.9#
125 37.7 15.5 23.3#

