

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027707.D
 Acq On : 15 Sep 2023 22:40
 Operator : MA/JU
 Sample : 04324-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHR6

Quant Time: Sep 16 01:32:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.017	152	5275	0.400	ng/ul	0.00
4) Naphthalene-d8	10.839	136	17933	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.652	164	11332	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.401	188	26126	0.400	ng/ul	0.00
17) Chrysene-d12	21.580	240	21548	0.400	ng/ul	0.00
23) Perylene-d12	24.074	264	22663	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	33723	5.075	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.418	152	7933	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	28315	0.430	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.431	88	2138	0.309	ng/ul	100
20) Pyrene	19.794	202	4607	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.913	252	8999	0.111	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027707.D
Acq On : 15 Sep 2023 22:40
Operator : MA/JU
Sample : 04324-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHR6

Quant Time: Sep 16 01:32:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration




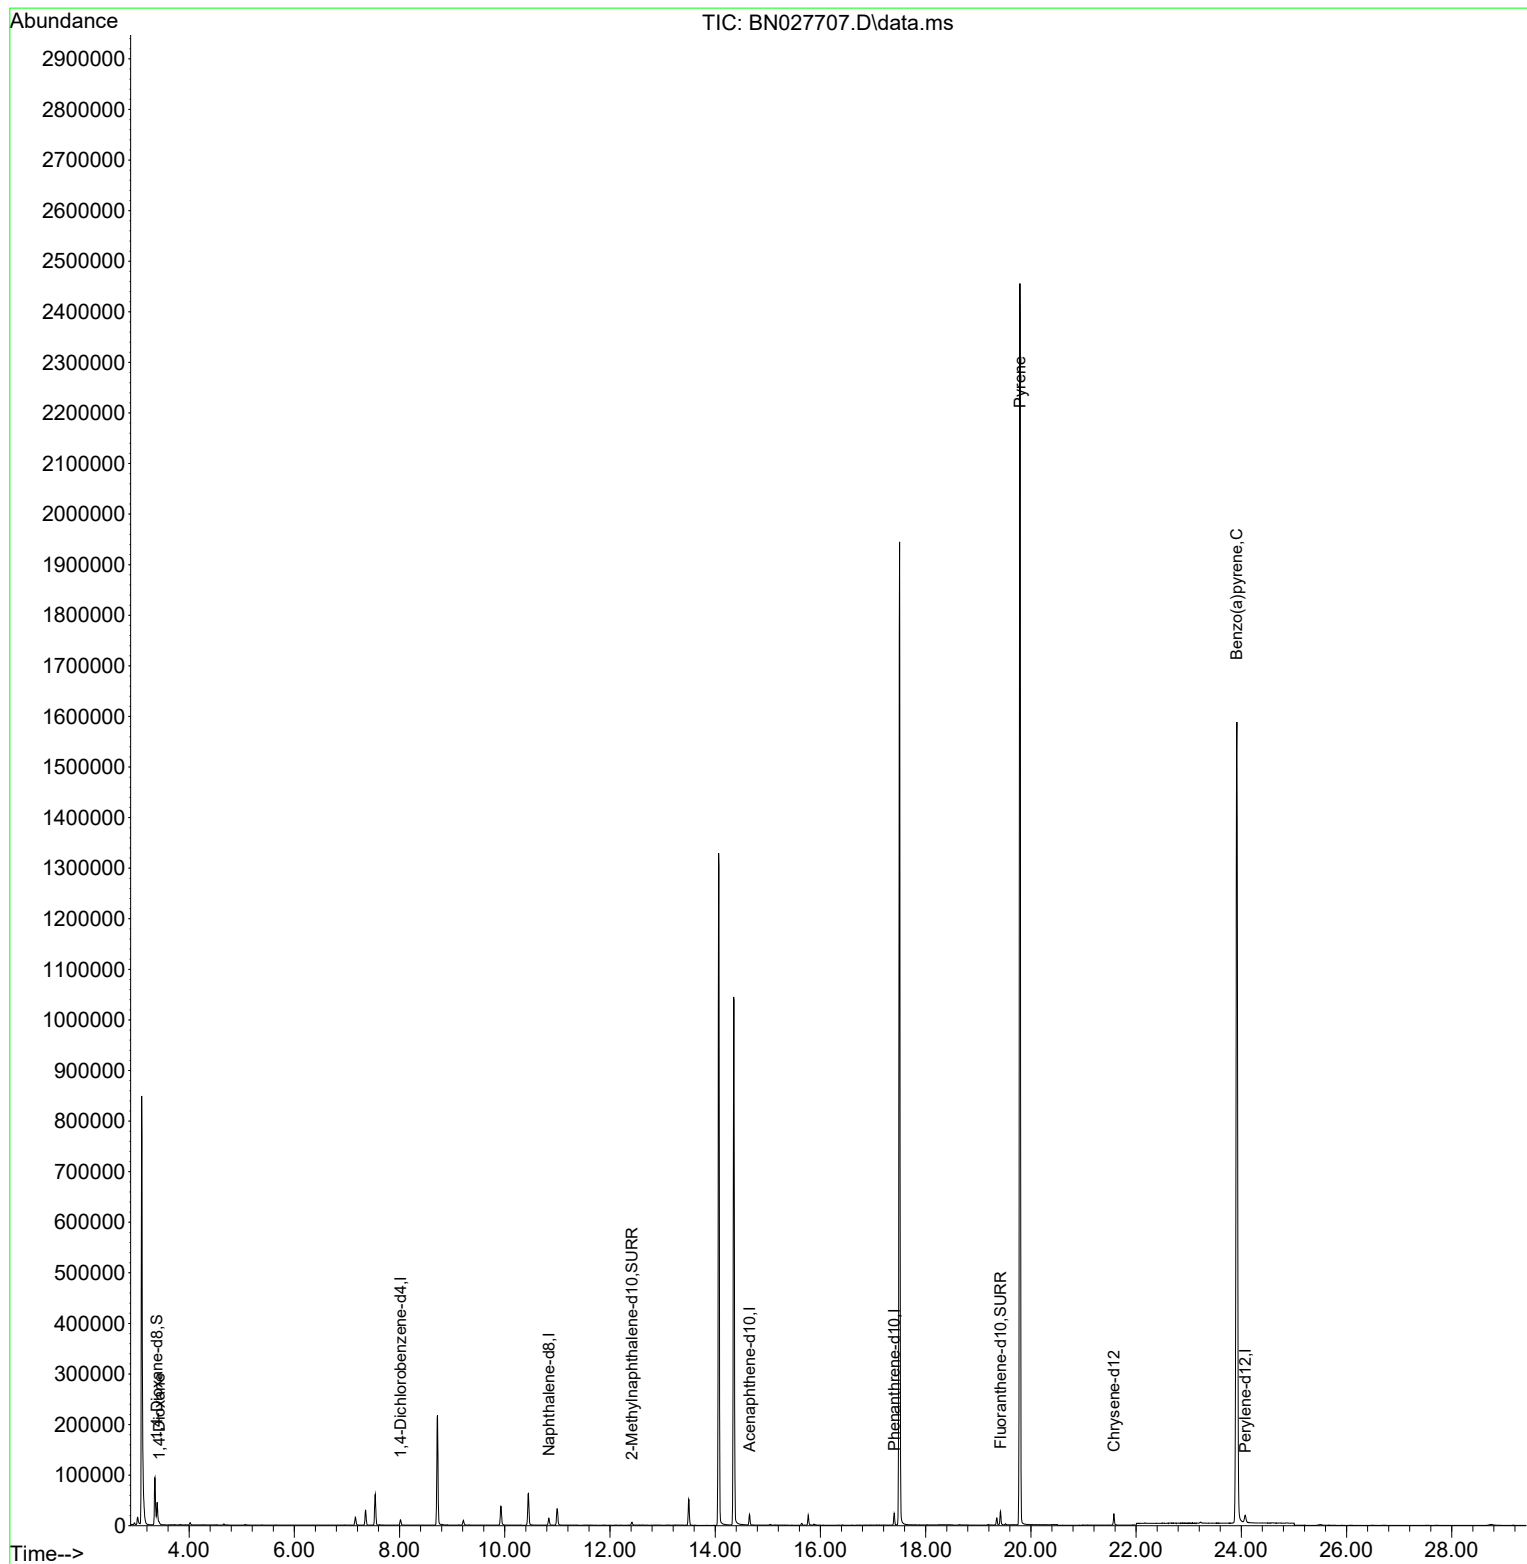


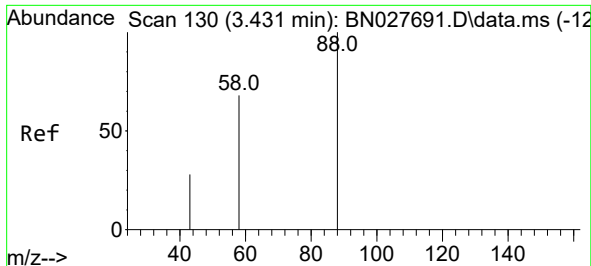

#2
1,4-Dioxane
Concen: 0.309 ng/ul
RT: 3.431 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN027707.D
Acq: 15 Sep 2023 22:40




Instrument :
BNA_N
ClientSampleId :
BBHR6


Tgt Ion: 88 Resp: 2138
Ion Ratio Lower Upper
88 100
43 49.6 39.6 59.4
58 60.5 48.3 72.5

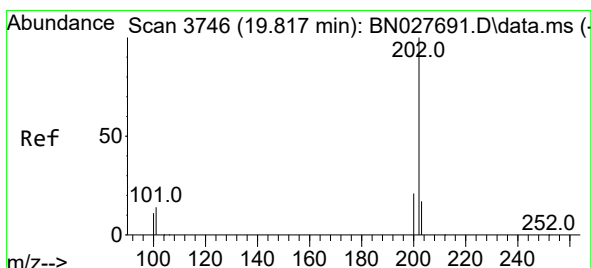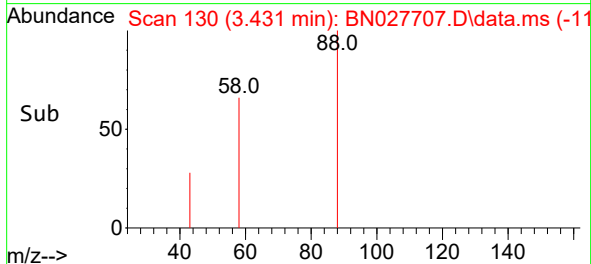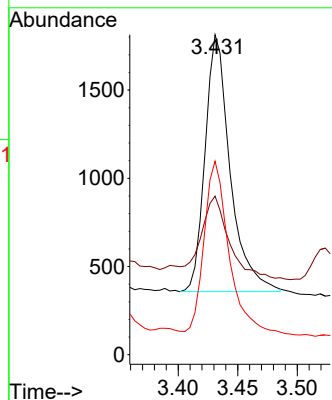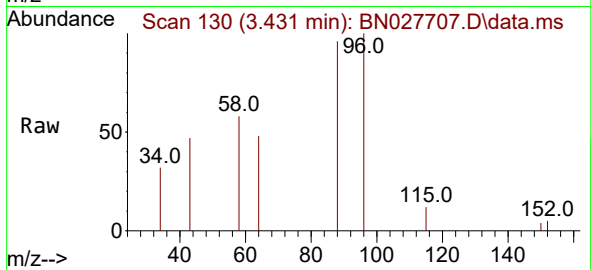

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.794 min Scan# 3741
Delta R.T. -0.023 min
Lab File: BN027707.D
Acq: 15 Sep 2023 22:40


Tgt Ion: 202 Resp: 4607
Ion Ratio Lower Upper
202 100
101 155.3 11.4 17.0#
100 1097.3 9.1 13.7#

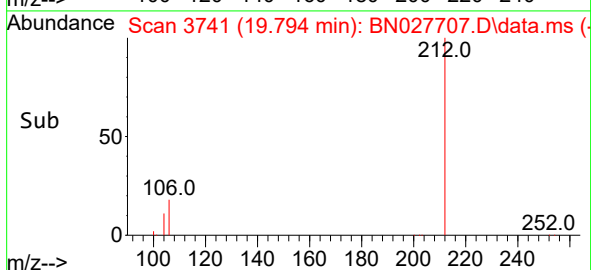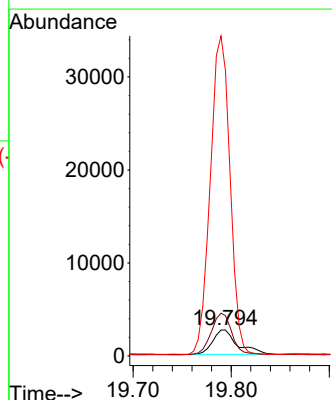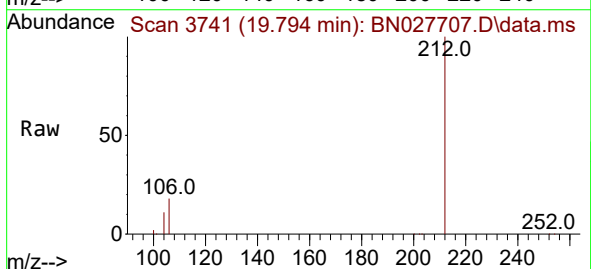

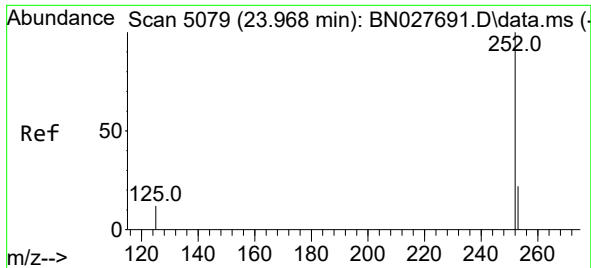

#26
Benzo(a)pyrene
Concen: 0.111 ng/ul
RT: 23.913 min Scan# 50
Delta R.T. -0.056 min
Lab File: BN027707.D
Acq: 15 Sep 2023 22:40

Instrument :
BNA_N
ClientSampleId :
BBHR6

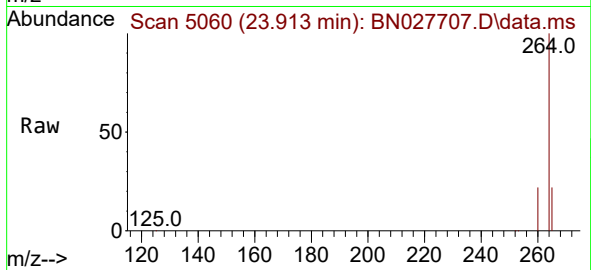

Tgt Ion:252 Resp: 8999
Ion Ratio Lower Upper
252 100
253 43.9 21.9 32.9#
125 38.1 15.5 23.3#

