

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027697.D
 Acq On : 15 Sep 2023 16:32
 Operator : MA/JU
 Sample : 04324-19
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJA4

Quant Time: Sep 16 01:31:18 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.009	152	5942	0.400	ng/ul	0.00
4) Naphthalene-d8	10.828	136	20183	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.647	164	11876	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.401	188	26955	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	22629	0.400	ng/ul	0.00
23) Perylene-d12	24.079	264	24002	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	18183	2.429	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.412	152	10465	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	29796	0.431	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.427	88	558	0.072	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027697.D
Acq On : 15 Sep 2023 16:32
Operator : MA/JU
Sample : 04324-19
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJA4

Quant Time: Sep 16 01:31:18 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration

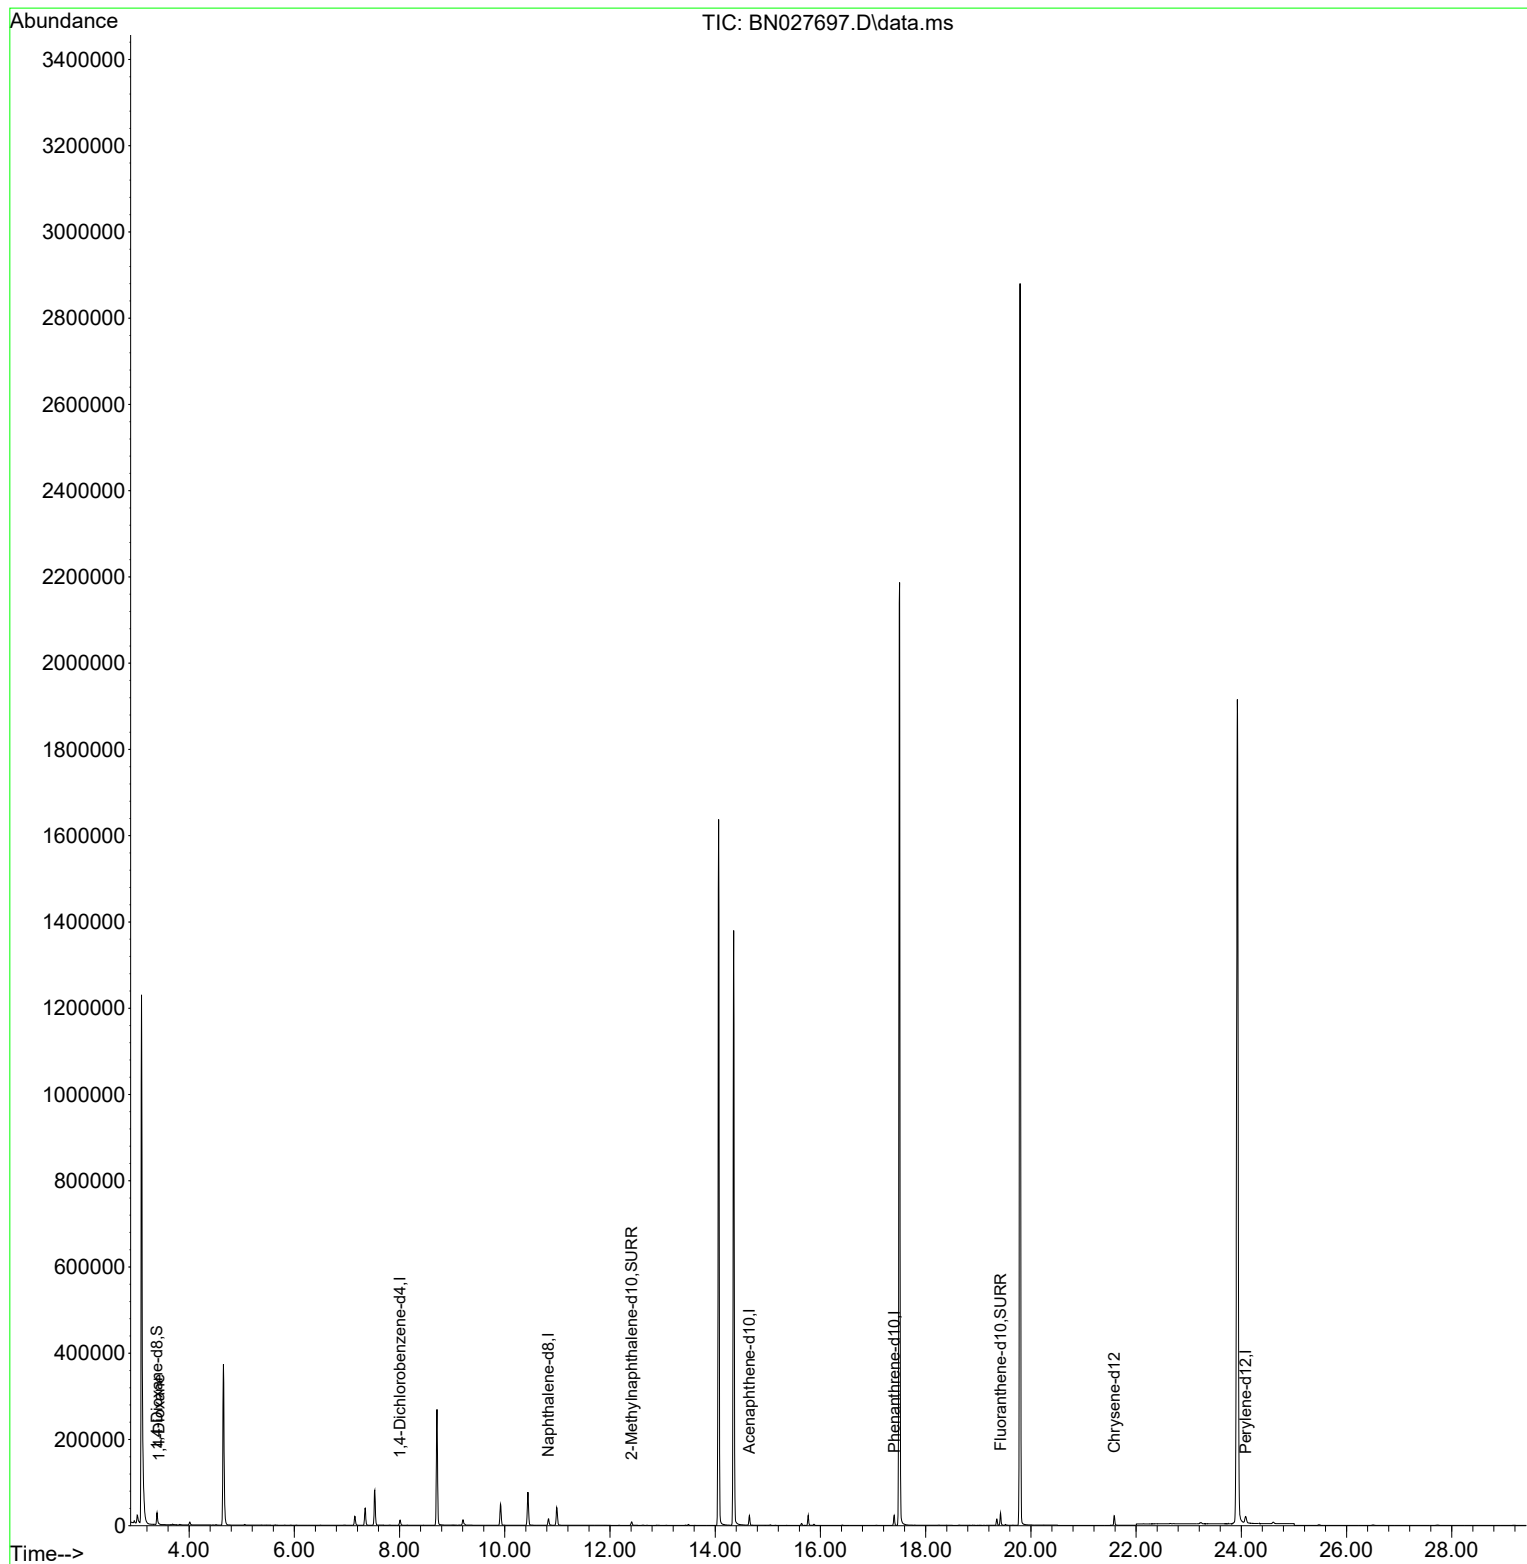

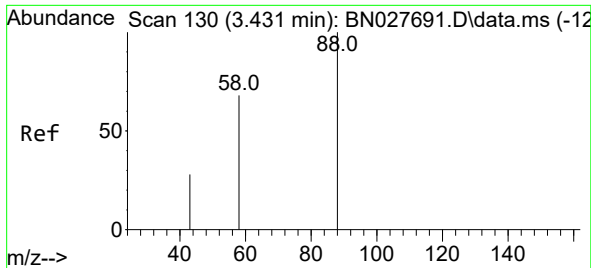

1,4-Dioxane

Concen: 0.072 ng/ul

RT: 3.427 min Scan# 11

Delta R.T. -0.004 min

Lab File: BN027697.D

Acq: 15 Sep 2023 16:32

Instrument :

BNA_N

ClientSampleId :

BBJA4

Tgt Ion: 88 Resp: 558

Ion Ratio Lower Upper

88 100

43 40.6 39.6 59.4

58 17.0 48.3 72.5#

