

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027698.D
 Acq On : 15 Sep 2023 17:08
 Operator : MA/JU
 Sample : 04306-17
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH4L8

Quant Time: Sep 16 01:31:24 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.017	152	4779	0.400	ng/ul	0.00
4) Naphthalene-d8	10.834	136	15824	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.652	164	9363	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.401	188	21918	0.400	ng/ul	0.00
17) Chrysene-d12	21.583	240	19419	0.400	ng/ul	0.00
23) Perylene-d12	24.079	264	19579	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	39397	6.545	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.418	152	18217	0.760	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	48318	0.815	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.431	88	1359	0.217	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027698.D
Acq On : 15 Sep 2023 17:08
Operator : MA/JU
Sample : 04306-17
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH4L8

Quant Time: Sep 16 01:31:24 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration

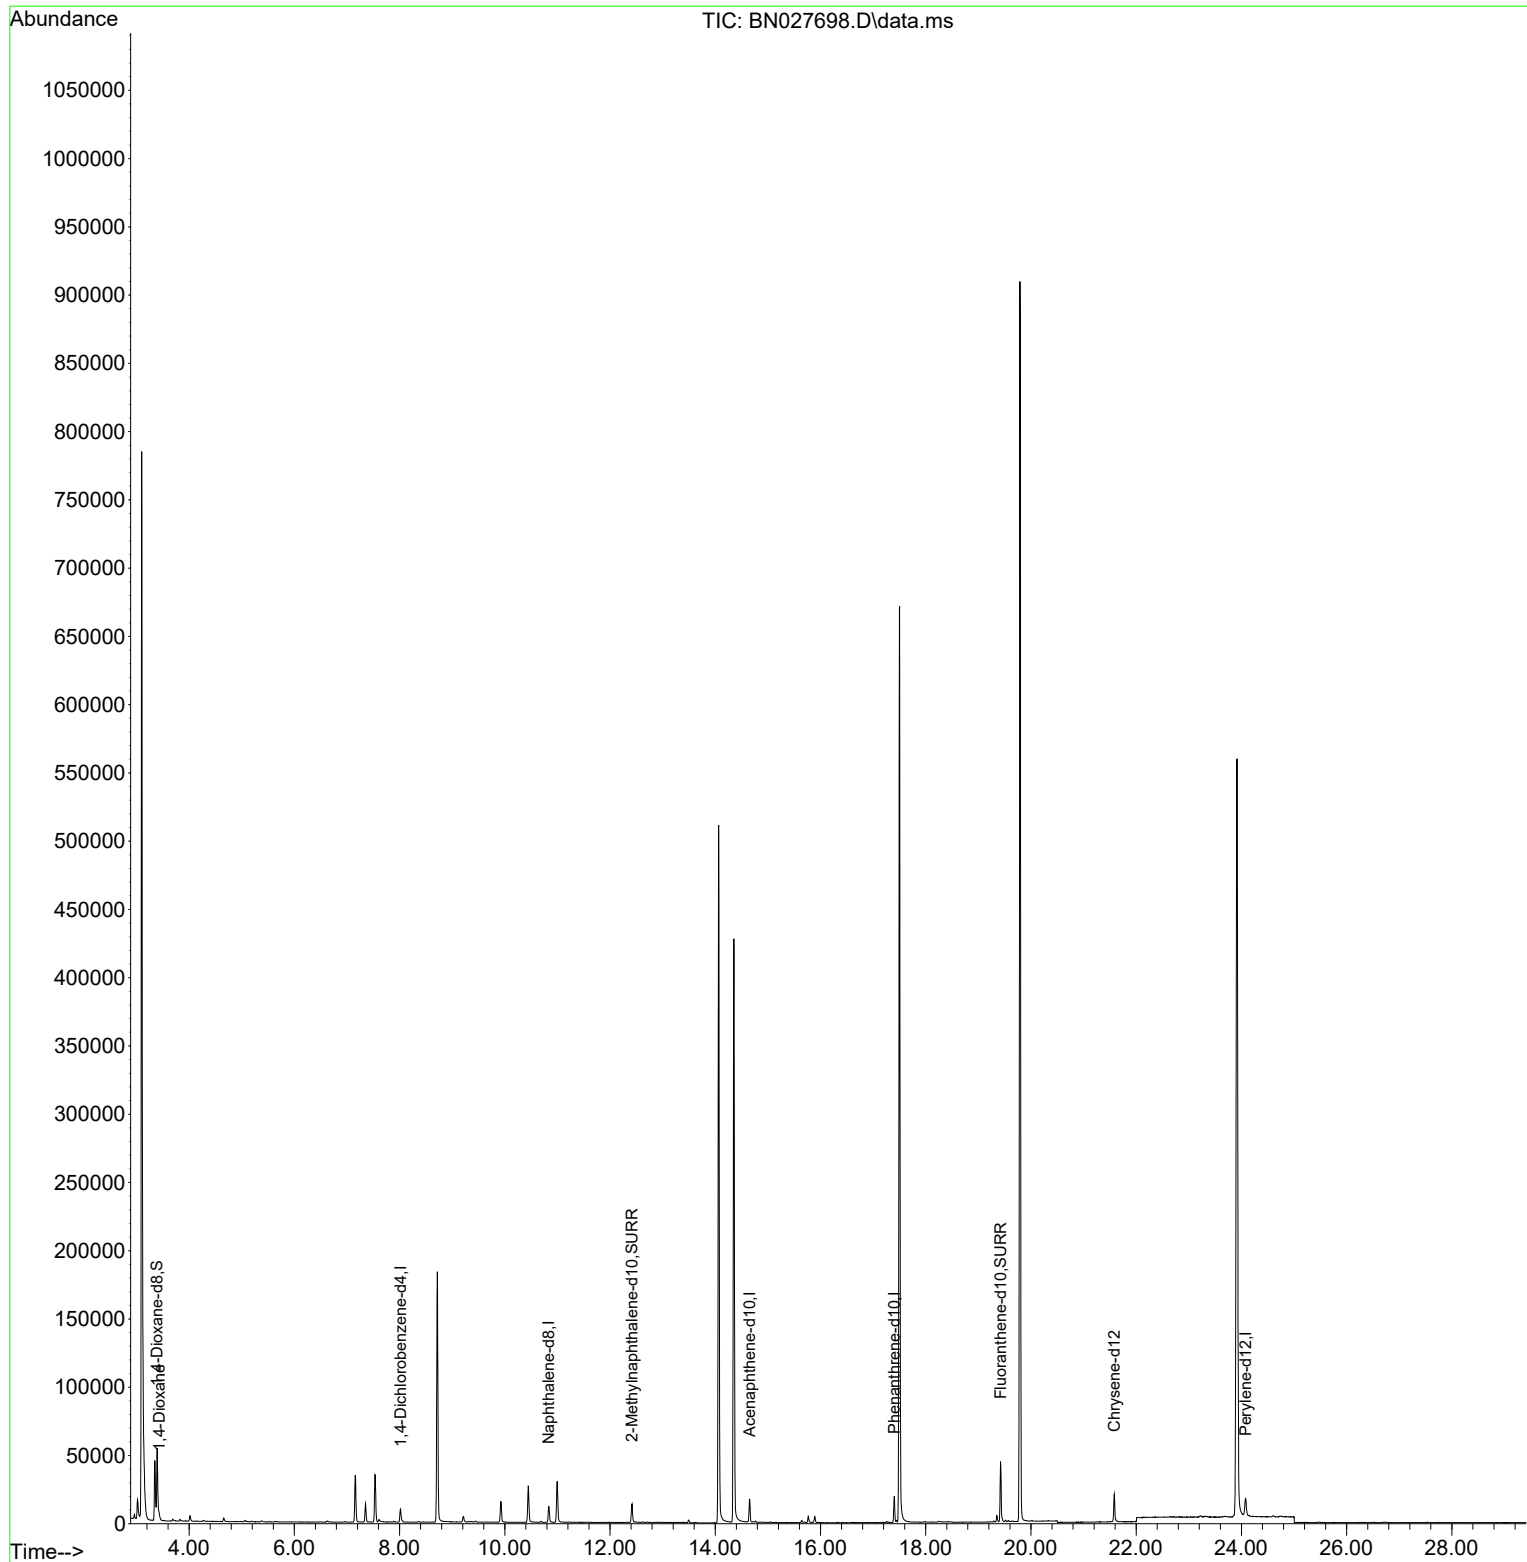

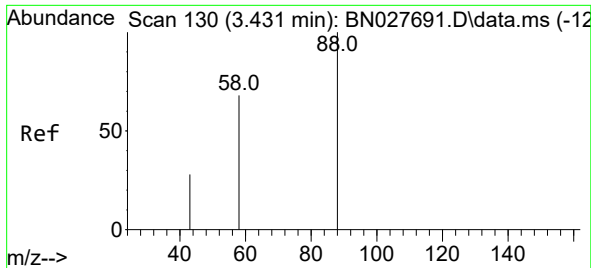

1,4-Dioxane

Concen: 0.217 ng/ul

RT: 3.431 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN027698.D


Acq: 15 Sep 2023 17:08

Instrument :

BNA_N

ClientSampleId :

BH4L8

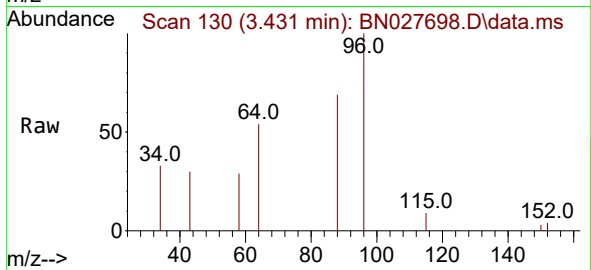

Tgt Ion: 88 Resp: 1359

Ion Ratio Lower Upper

88 100

43 43.3 39.6 59.4

58 42.2 48.3 72.5#

