

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027711.D
 Acq On : 16 Sep 2023 01:09
 Operator : MA/JU
 Sample : 04324-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBKA8

Quant Time: Sep 16 02:46:52 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.017	152	4390	0.400	ng/ul	0.00
4) Naphthalene-d8	10.839	136	16460	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.652	164	9473	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.401	188	20969	0.400	ng/ul	0.00
17) Chrysene-d12	21.577	240	17479	0.400	ng/ul	0.00
23) Perylene-d12	24.070	264	18695	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	24706	4.468	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.418	152	8206	0.329	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	24476	0.458	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.889	128	1801	0.038	ng/ul#	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027711.D
Acq On : 16 Sep 2023 01:09
Operator : MA/JU
Sample : 04324-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBKA8


Quant Time: Sep 16 02:46:52 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration

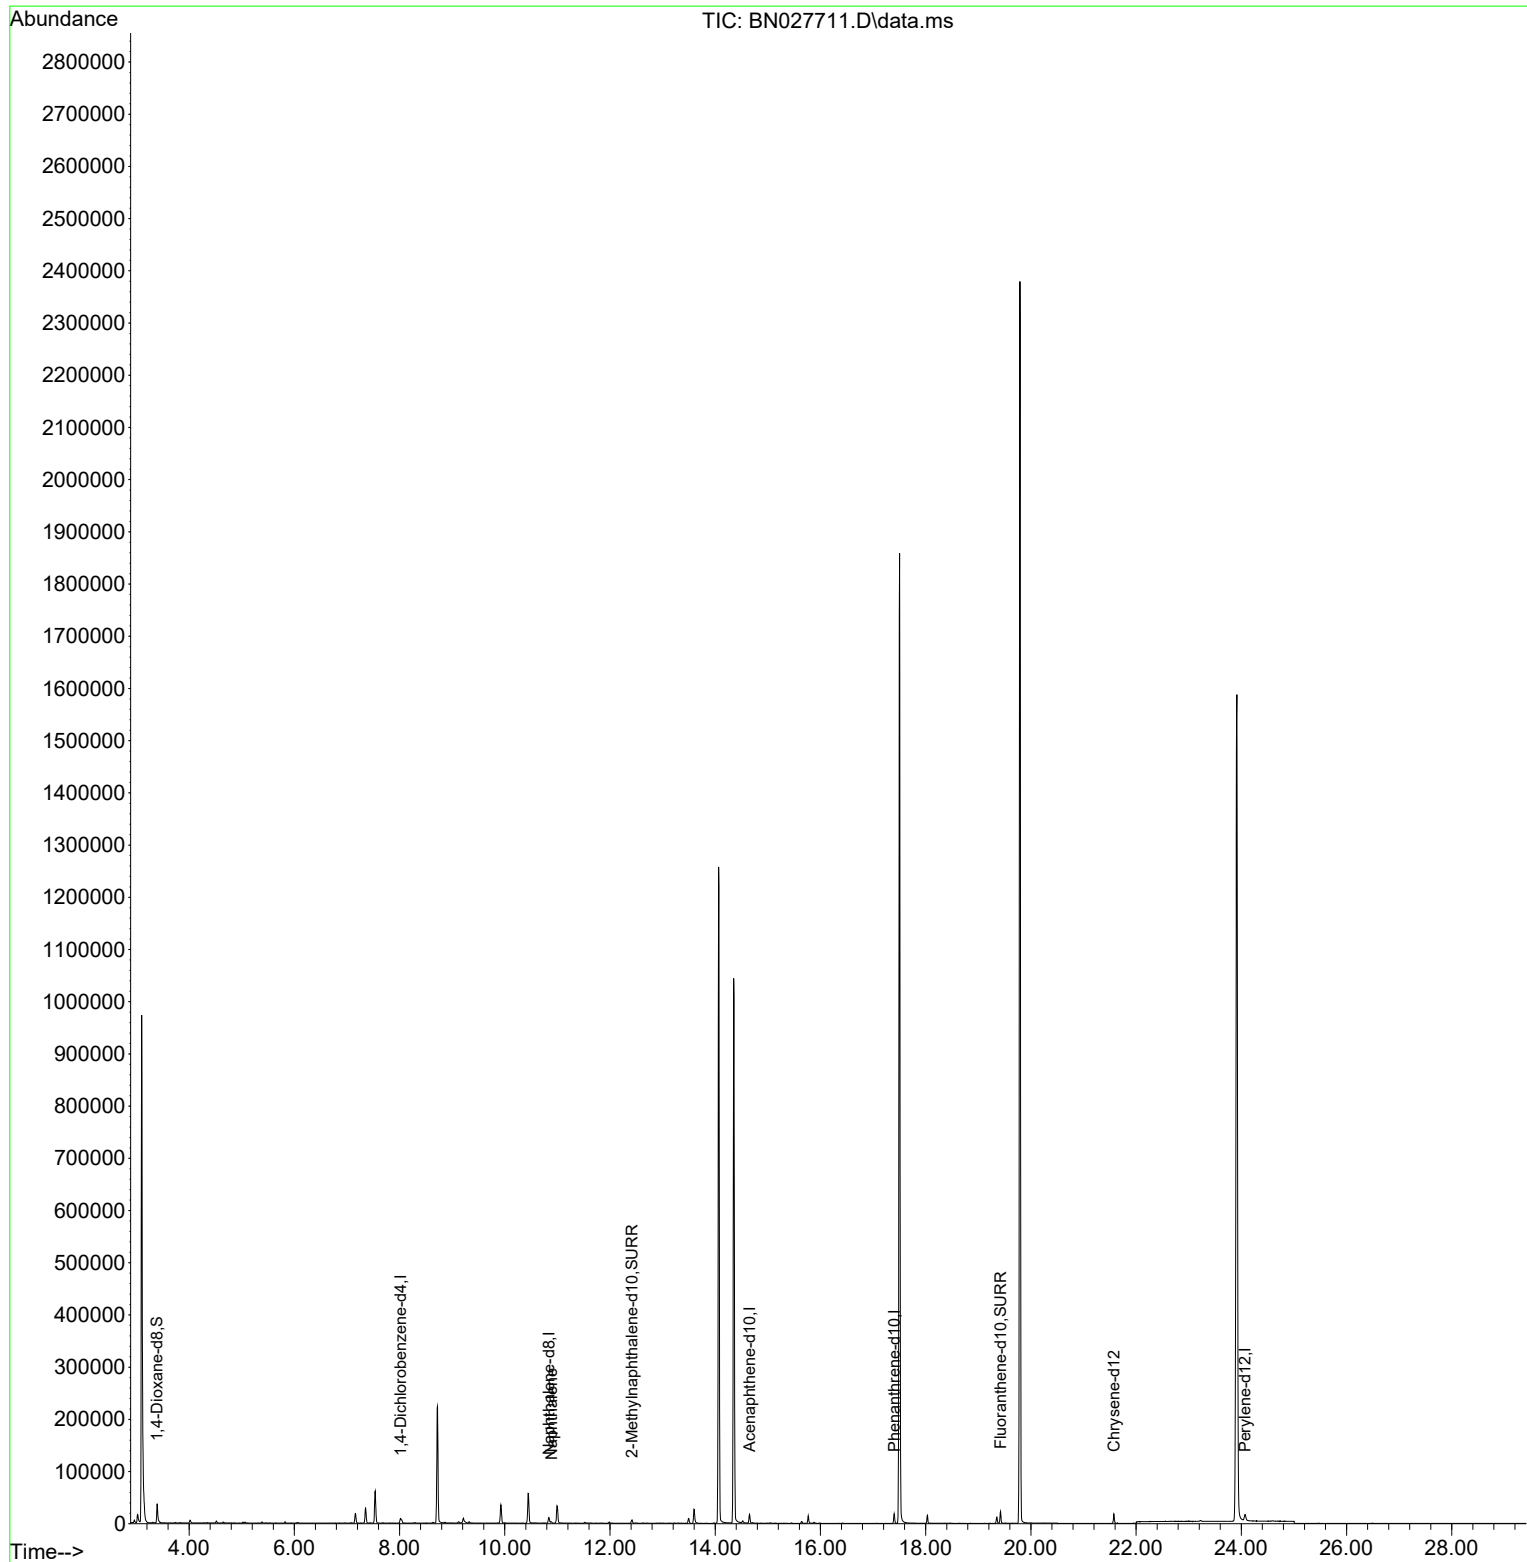

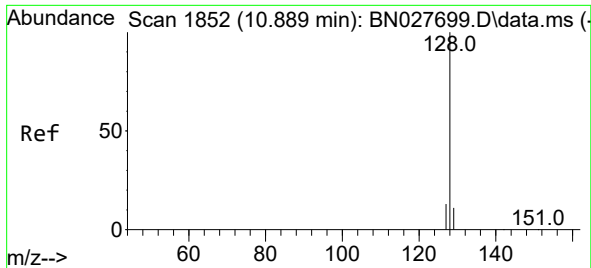

#5
Naphthalene
Concen: 0.038 ng/ul
RT: 10.889 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN027711.D
Acq: 16 Sep 2023 01:09

Instrument :
BNA_N
ClientSampleId :
BBKA8

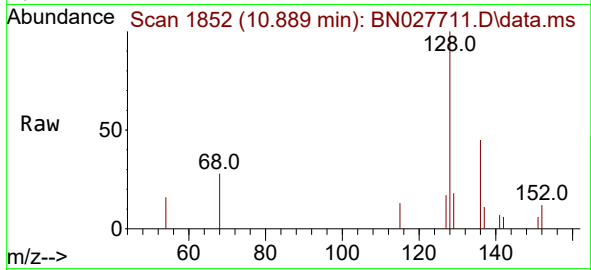

Tgt Ion:128 Resp: 1801
Ion Ratio Lower Upper
128 100
129 18.4 9.3 13.9#
127 17.4 10.7 16.1#

