

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027712.D
 Acq On : 16 Sep 2023 01:46
 Operator : MA/JU
 Sample : 04330-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EZYP2

Quant Time: Sep 16 02:47:27 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.017	152	5177	0.400	ng/ul	0.00
4) Naphthalene-d8	10.839	136	18187	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.652	164	11252	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.401	188	24239	0.400	ng/ul	0.00
17) Chrysene-d12	21.577	240	19678	0.400	ng/ul	0.00
23) Perylene-d12	24.071	264	21195	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	33711	5.170	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.412	152	10503	0.381	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	29544	0.492	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.431	88	538	0.079	ng/ul#	66
5) Naphthalene	10.889	128	2196	0.042	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027712.D
Acq On : 16 Sep 2023 01:46
Operator : MA/JU
Sample : 04330-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EZYP2

Quant Time: Sep 16 02:47:27 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration




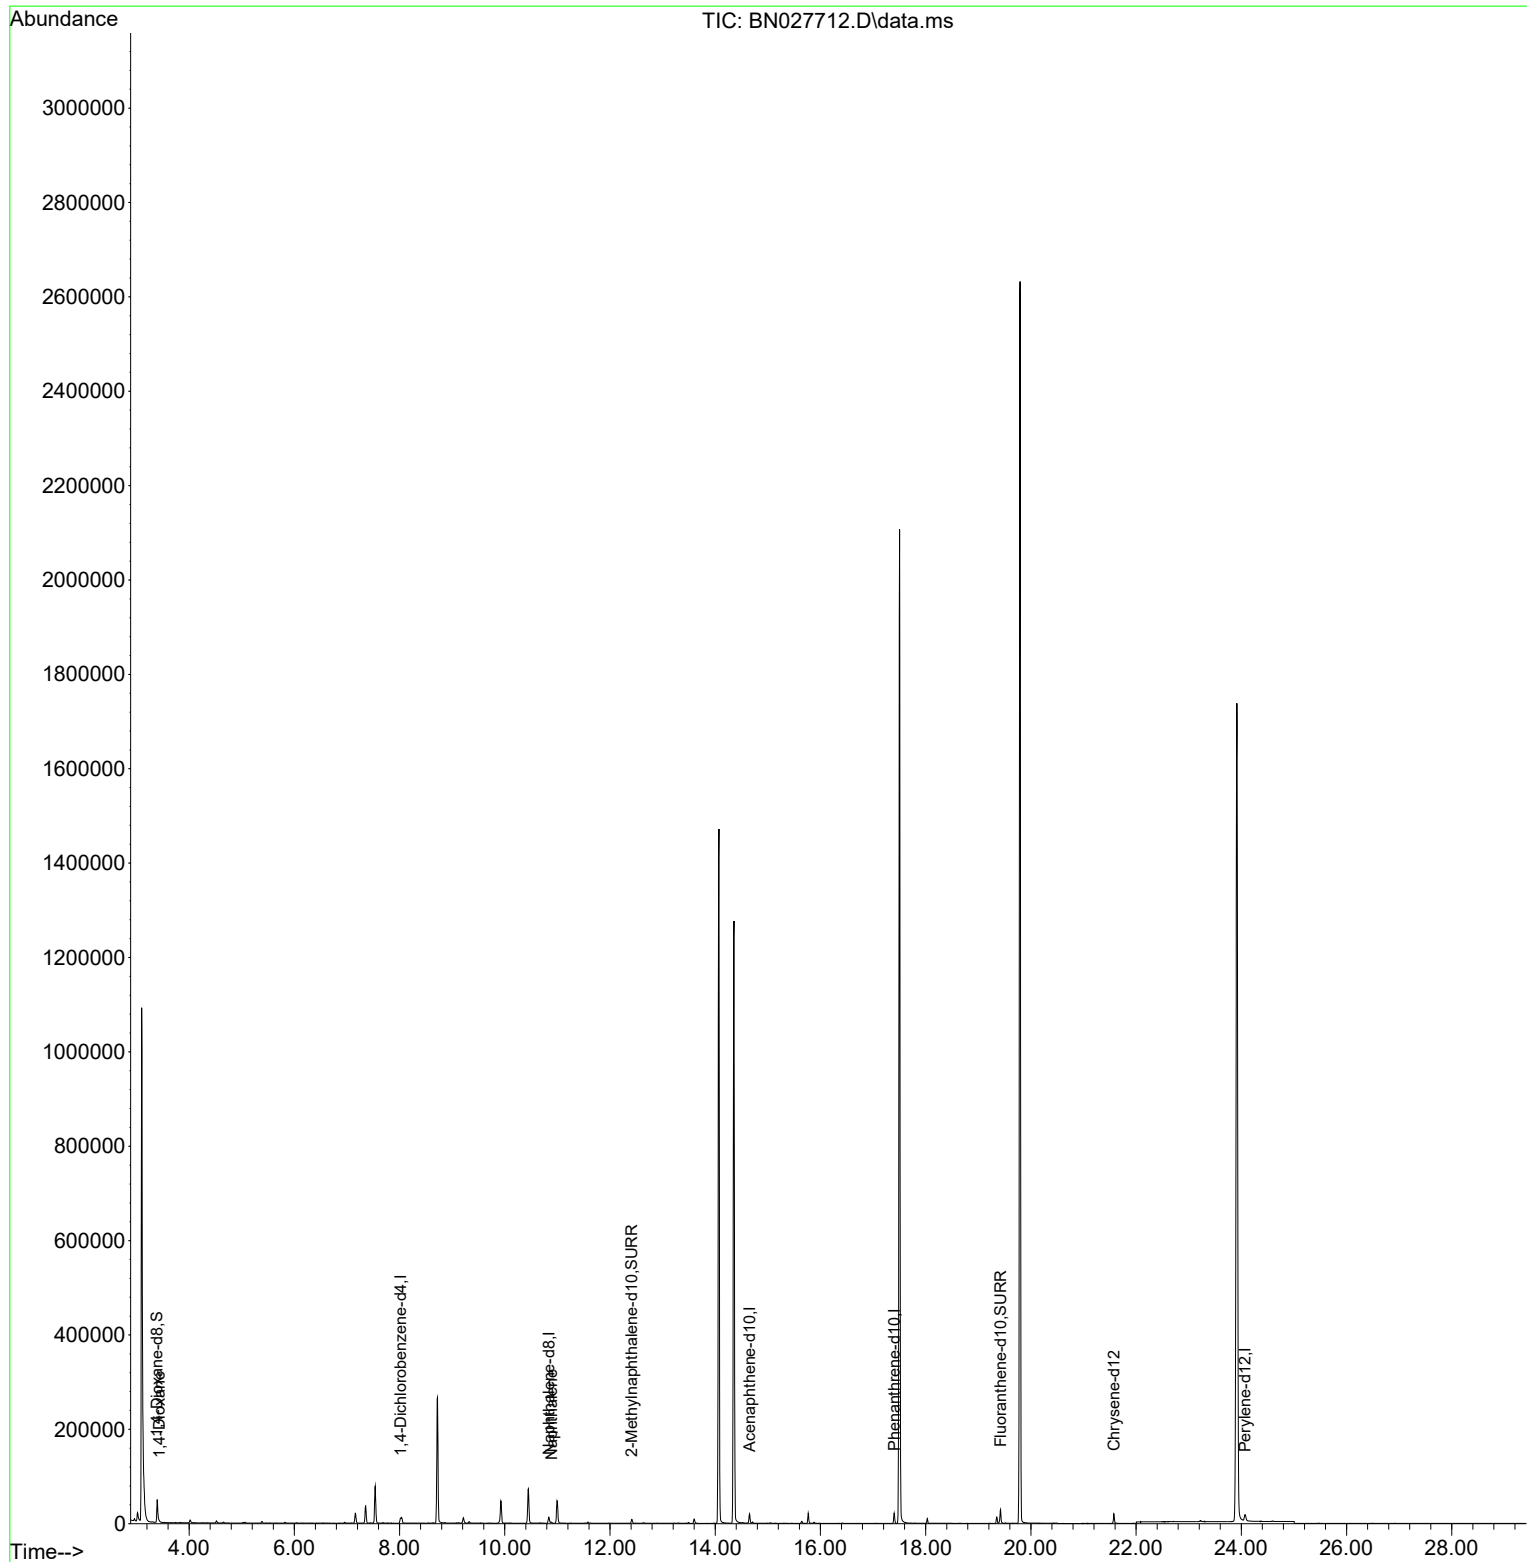


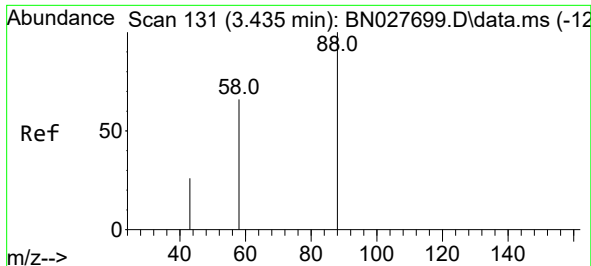

#2
1,4-Dioxane
Concen: 0.079 ng/ul
RT: 3.431 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN027712.D
Acq: 16 Sep 2023 01:46

Instrument :
BNA_N
ClientSampleId :
EZY2

Tgt Ion: 88 Resp: 538
Ion Ratio Lower Upper
88 100
43 45.7 39.6 59.4
58 16.4 48.3 72.5#

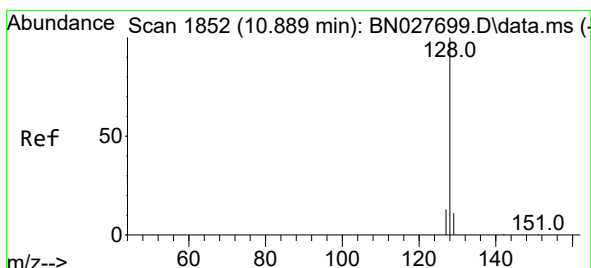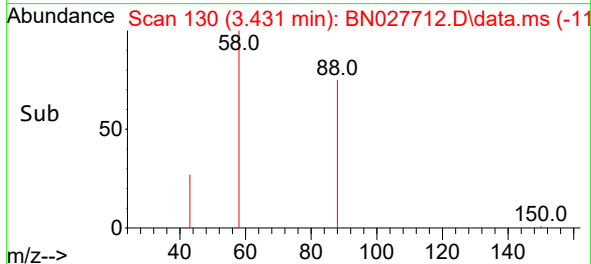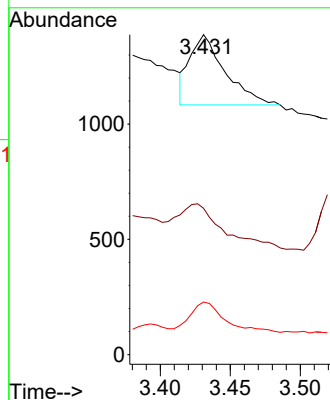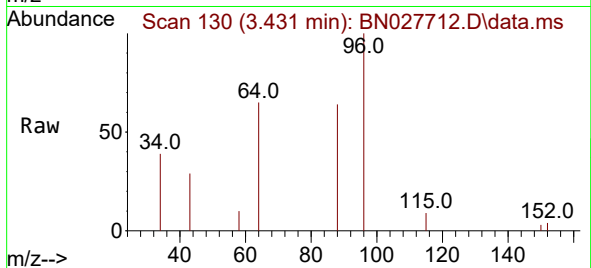

#5
Naphthalene
Concen: 0.042 ng/ul
RT: 10.889 min Scan# 1852
Delta R.T. -0.000 min
Lab File: BN027712.D
Acq: 16 Sep 2023 01:46

Tgt Ion:128 Resp: 2196
Ion Ratio Lower Upper
128 100
129 17.2 9.3 13.9#
127 16.7 10.7 16.1#

