

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027717.D
 Acq On : 16 Sep 2023 05:26
 Operator : MA/JU
 Sample : 04324-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHX0

Quant Time: Sep 16 06:06:21 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.017	152	4884	0.400	ng/ul	0.00
4) Naphthalene-d8	10.834	136	16621	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.647	164	10230	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.400	188	23747	0.400	ng/ul	0.00
17) Chrysene-d12	21.577	240	19274	0.400	ng/ul	0.00
23) Perylene-d12	24.070	264	19871	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	40632	6.605	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.412	152	8517	0.338	ng/ul	0.00
18) Fluoranthene-d10	19.422	212	27188	0.462	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.431	88	12474	1.948	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027717.D
Acq On : 16 Sep 2023 05:26
Operator : MA/JU
Sample : 04324-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHX0

Quant Time: Sep 16 06:06:21 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration

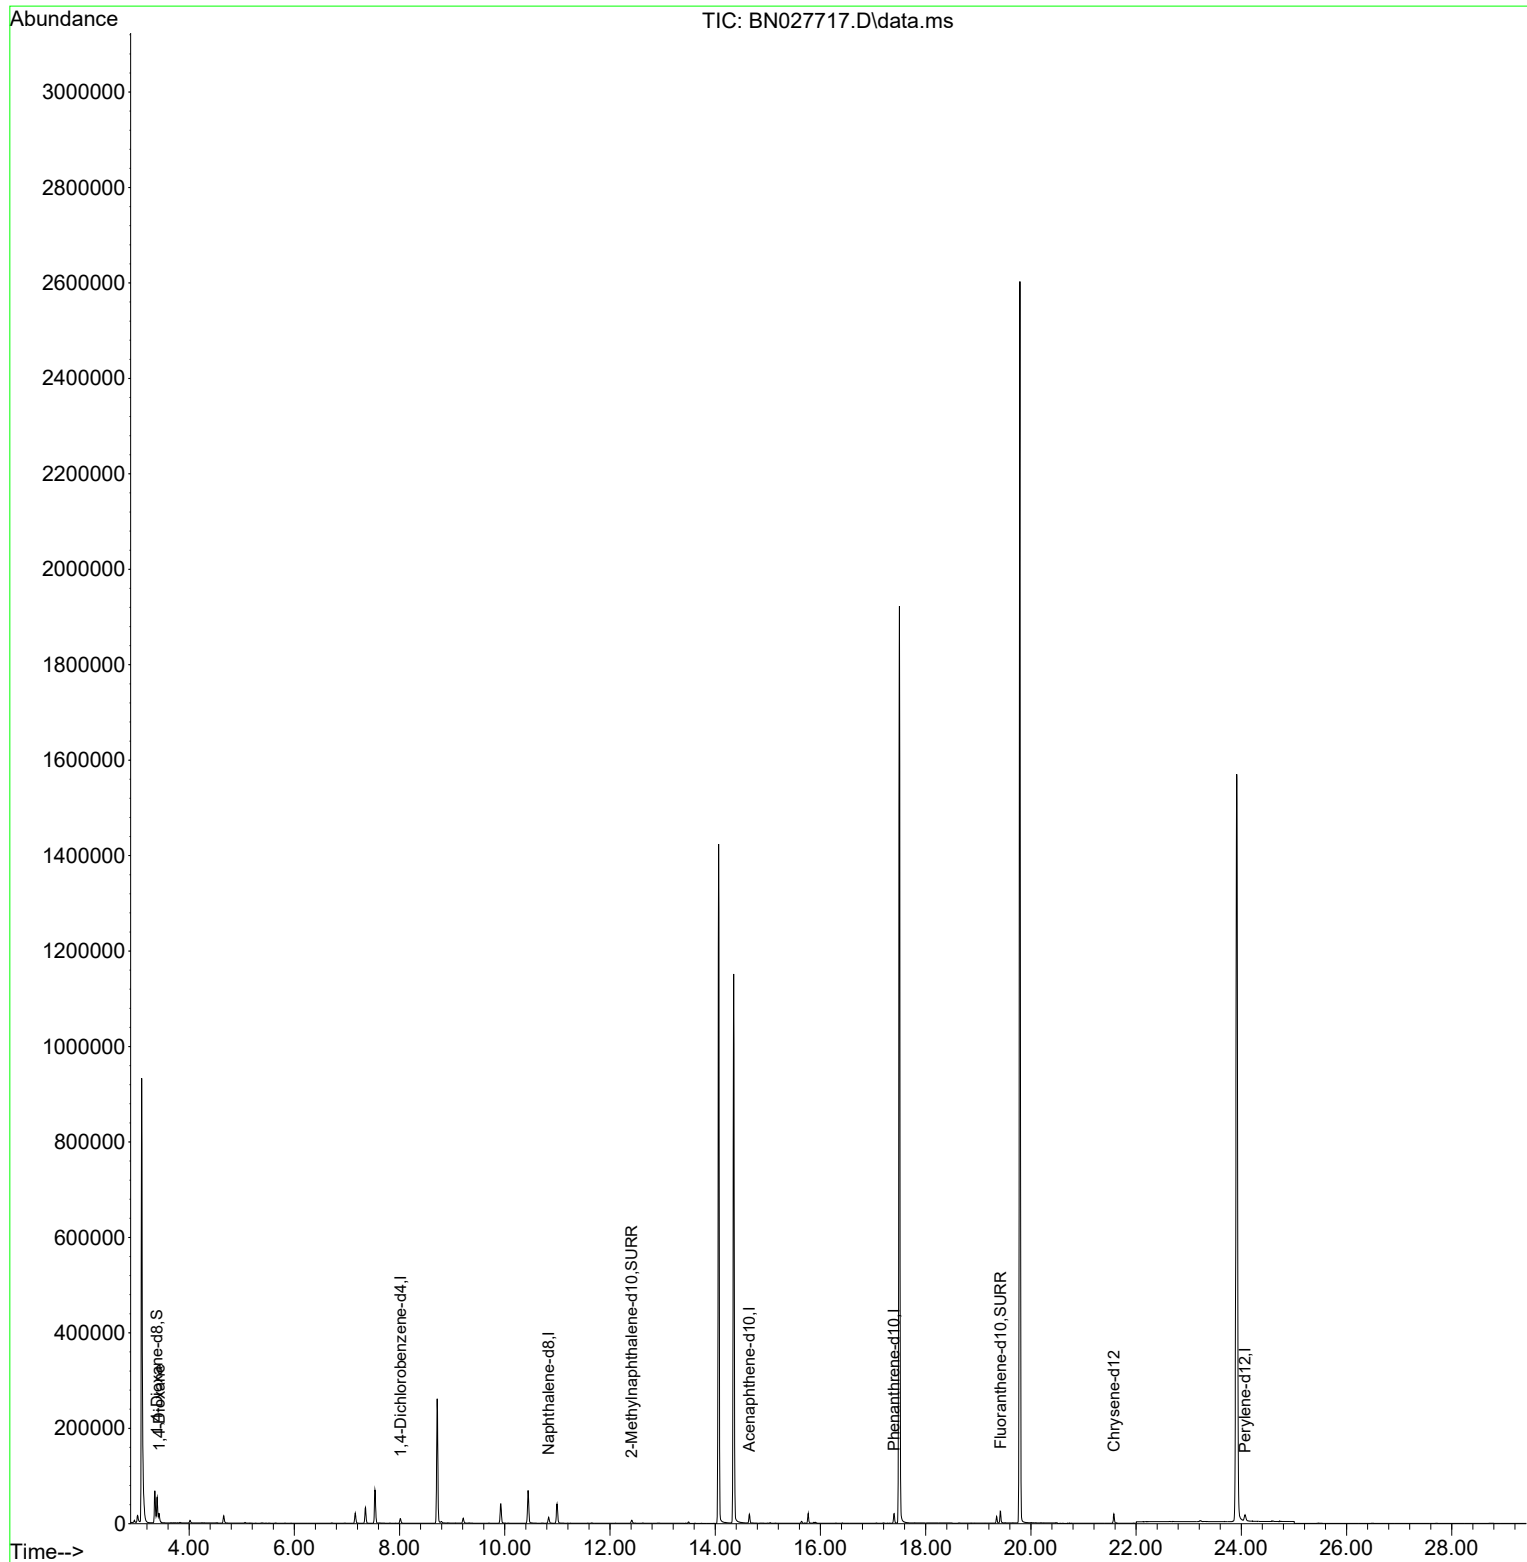

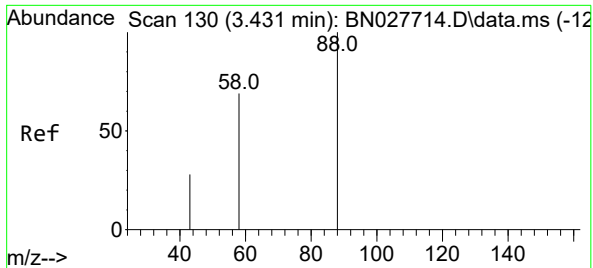

1,4-Dioxane
 Concen: 1.948 ng/ul
 RT: 3.431 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN027717.D
 Acq: 16 Sep 2023 05:26

Instrument :
 BNA_N
 ClientSampleId :
 BBHX0

Tgt Ion:	88	Resp:	12474
Ion	Ratio	Lower	Upper
88	100		
43	28.7	39.6	59.4#
58	63.1	48.3	72.5

