

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027718.D
 Acq On : 16 Sep 2023 06:02
 Operator : MA/JU
 Sample : 04324-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHW6

Quant Time: Sep 16 06:35:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.013	152	4495	0.400	ng/ul	0.00
4) Naphthalene-d8	10.834	136	15350	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.647	164	9506	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.401	188	21738	0.400	ng/ul	0.00
17) Chrysene-d12	21.577	240	17811	0.400	ng/ul	0.00
23) Perylene-d12	24.071	264	18781	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	37348	6.596	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.412	152	8773	0.377	ng/ul	0.00
18) Fluoranthene-d10	19.418	212	26493	0.487	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.431	88	11954	2.029	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027718.D
Acq On : 16 Sep 2023 06:02
Operator : MA/JU
Sample : 04324-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHW6

Quant Time: Sep 16 06:35:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration

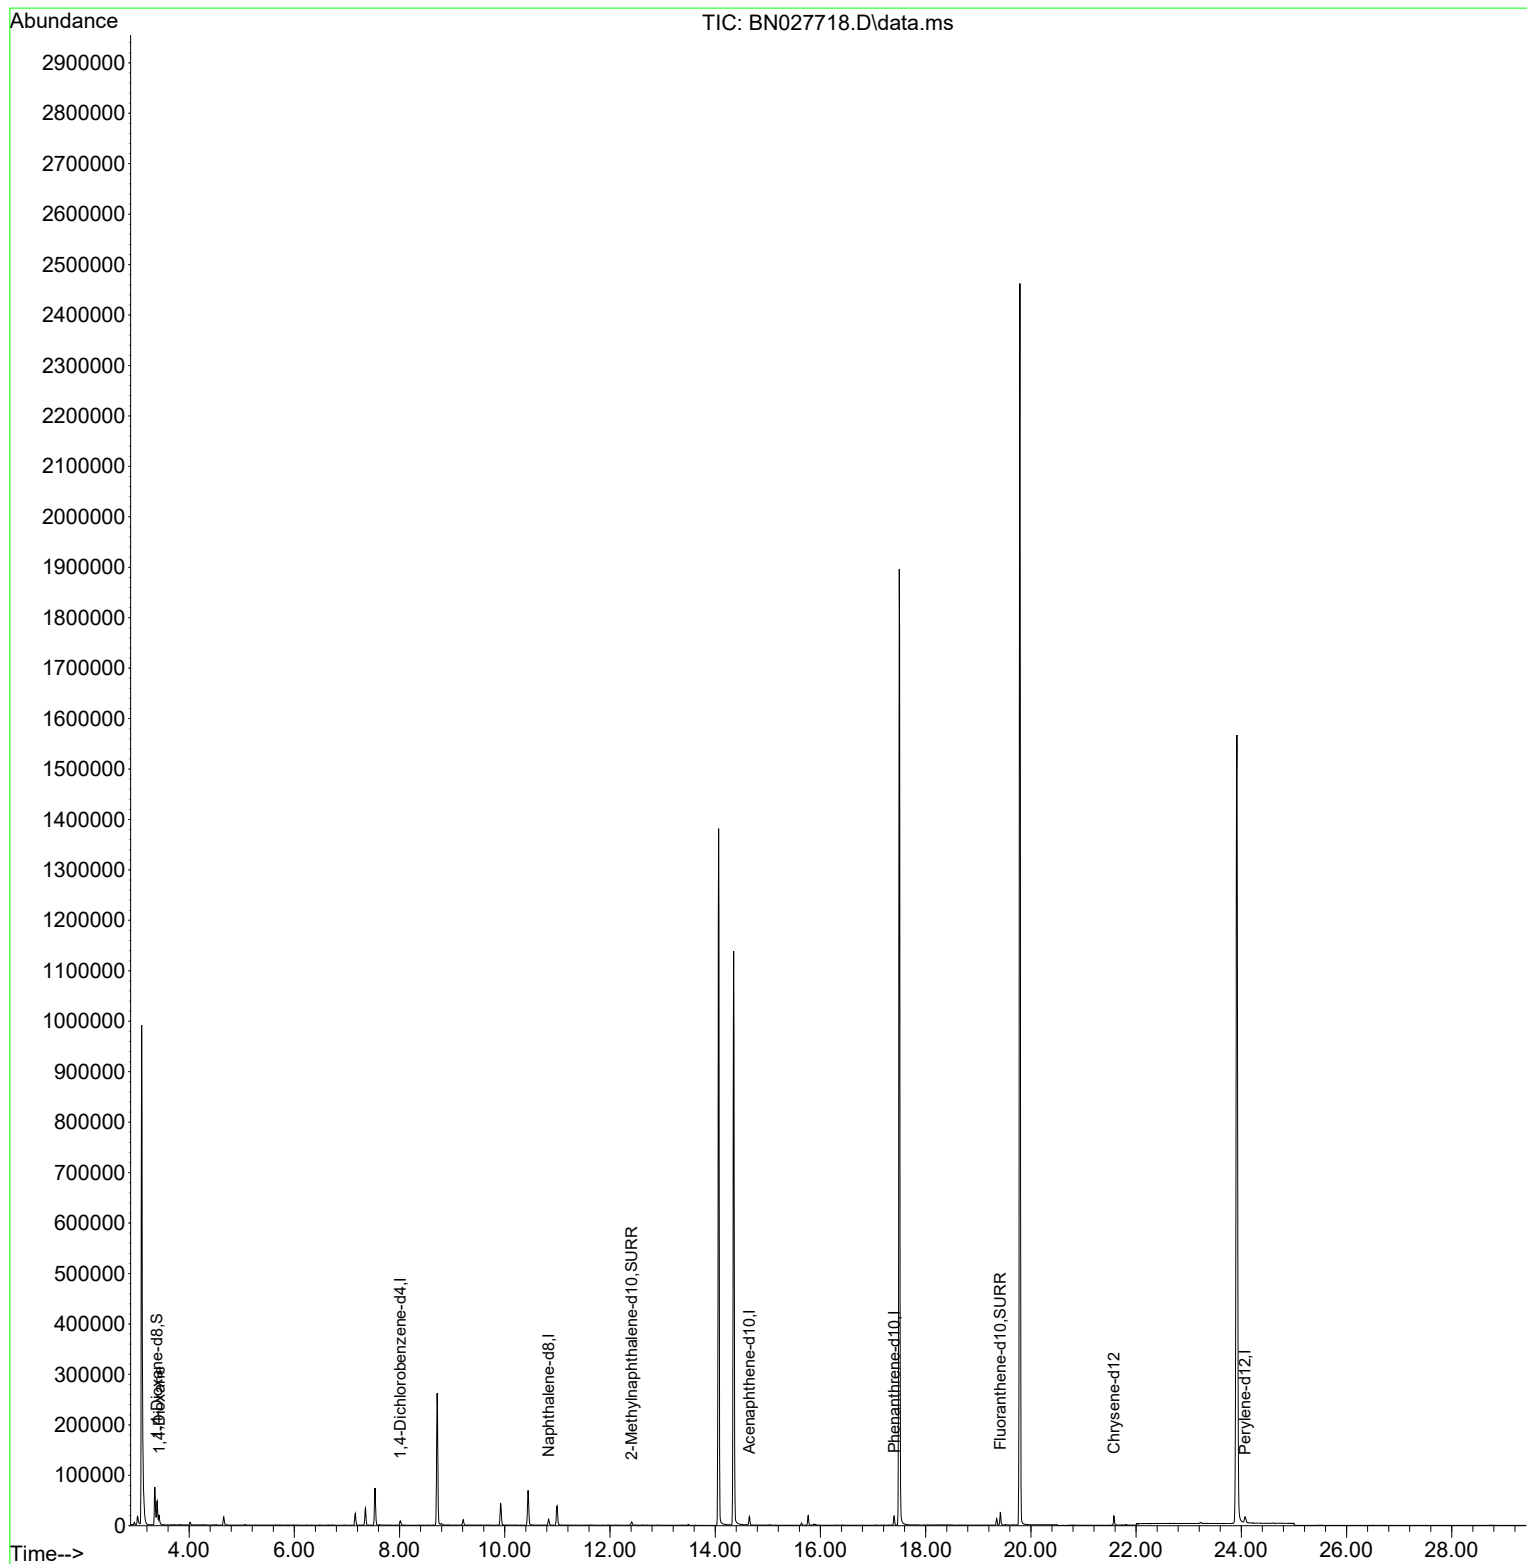

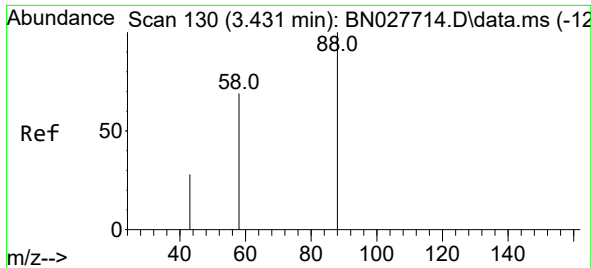

1,4-Dioxane

Concen: 2.029 ng/ul

RT: 3.431 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN027718.D


Acq: 16 Sep 2023 06:02

Instrument :

BNA_N

ClientSampleId :

BBHW6

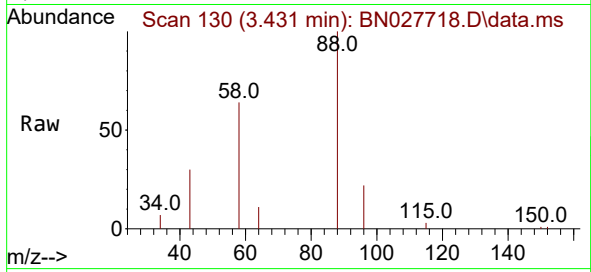

Tgt Ion: 88 Resp: 11954

Ion Ratio Lower Upper

88 100

43 29.5 39.6 59.4#

58 63.9 48.3 72.5

