

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
 Data File : BN027721.D
 Acq On : 16 Sep 2023 07:50
 Operator : MA/JU
 Sample : 04324-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHF1

Quant Time: Sep 18 00:49:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 01:11:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.013	152	4039	0.400	ng/ul	0.00
4) Naphthalene-d8	10.834	136	14005	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.647	164	8761	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.397	188	20675	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.577	240	16974	0.400	ng/ul	0.00
23) Perylene-d12	24.071	264	18359	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	33379	6.561	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.412	152	7740	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.418	212	26734	0.516	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.431	88	1585	0.299	ng/ul	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091523\
Data File : BN027721.D
Acq On : 16 Sep 2023 07:50
Operator : MA/JU
Sample : 04324-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHF1

Quant Time: Sep 18 00:49:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 01:11:24 2023
Response via : Initial Calibration

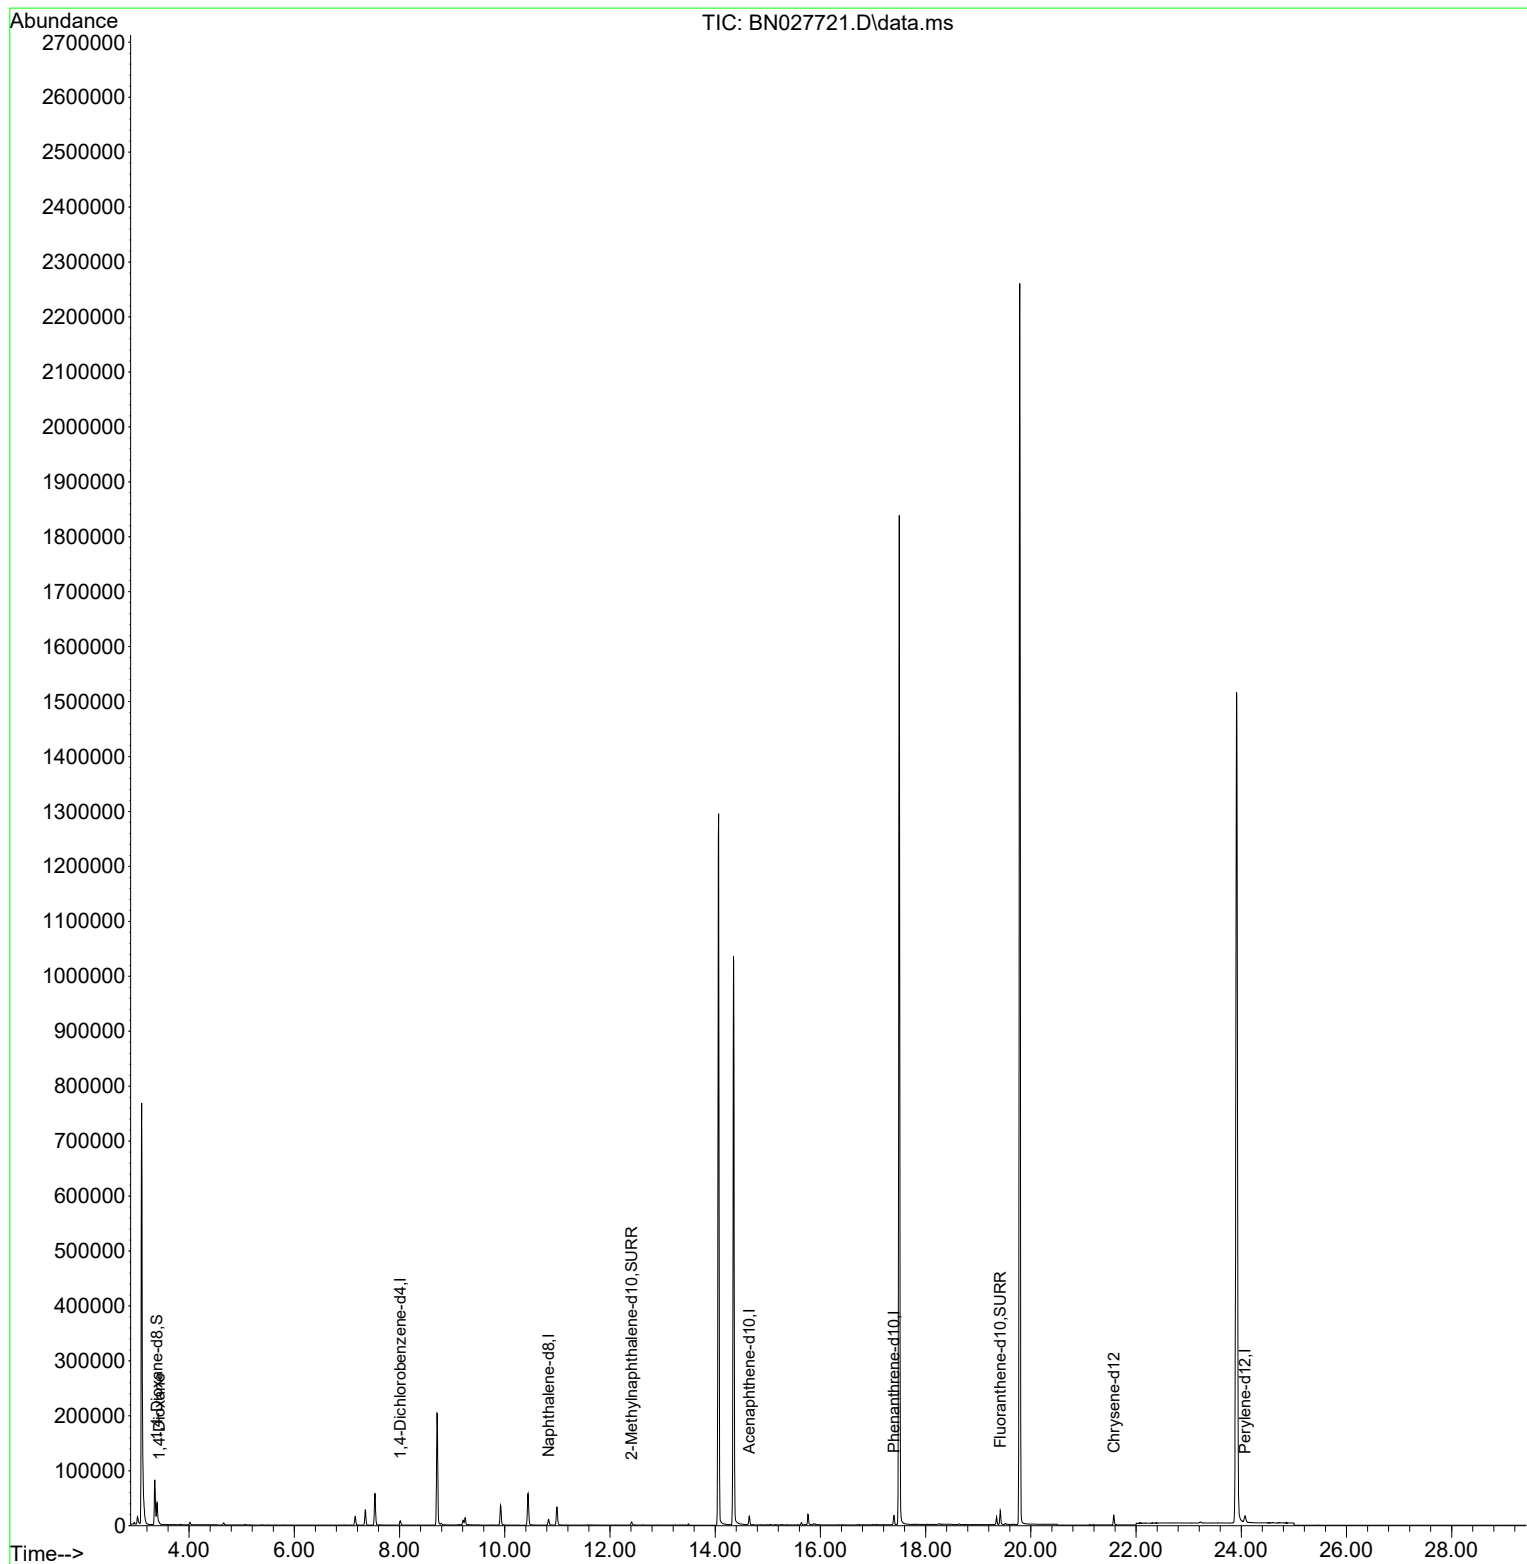

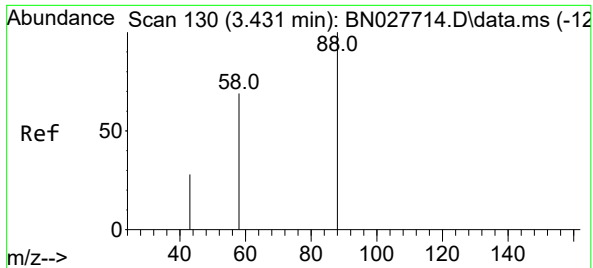

1,4-Dioxane

Concen: 0.299 ng/ul

RT: 3.431 min Scan# 11

Delta R.T. 0.000 min

Lab File: BN027721.D


Acq: 16 Sep 2023 07:50

Instrument :

BNA_N

ClientSampleId :

BBHF1

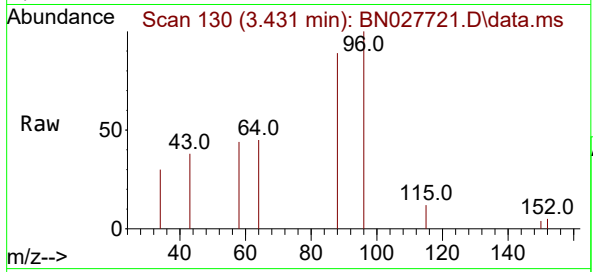

Tgt Ion: 88 Resp: 1585

Ion Ratio Lower Upper

88 100

43 42.5 39.6 59.4

58 49.8 48.3 72.5

