


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091525\
Data File : BN037714.D
Acq On : 15 Sep 2025 09:34
Operator : RC/JU
Sample : DFTPP383
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP383

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Title : SVOA CALIBRATION
Last Update : Fri Sep 12 15:43:05 2025

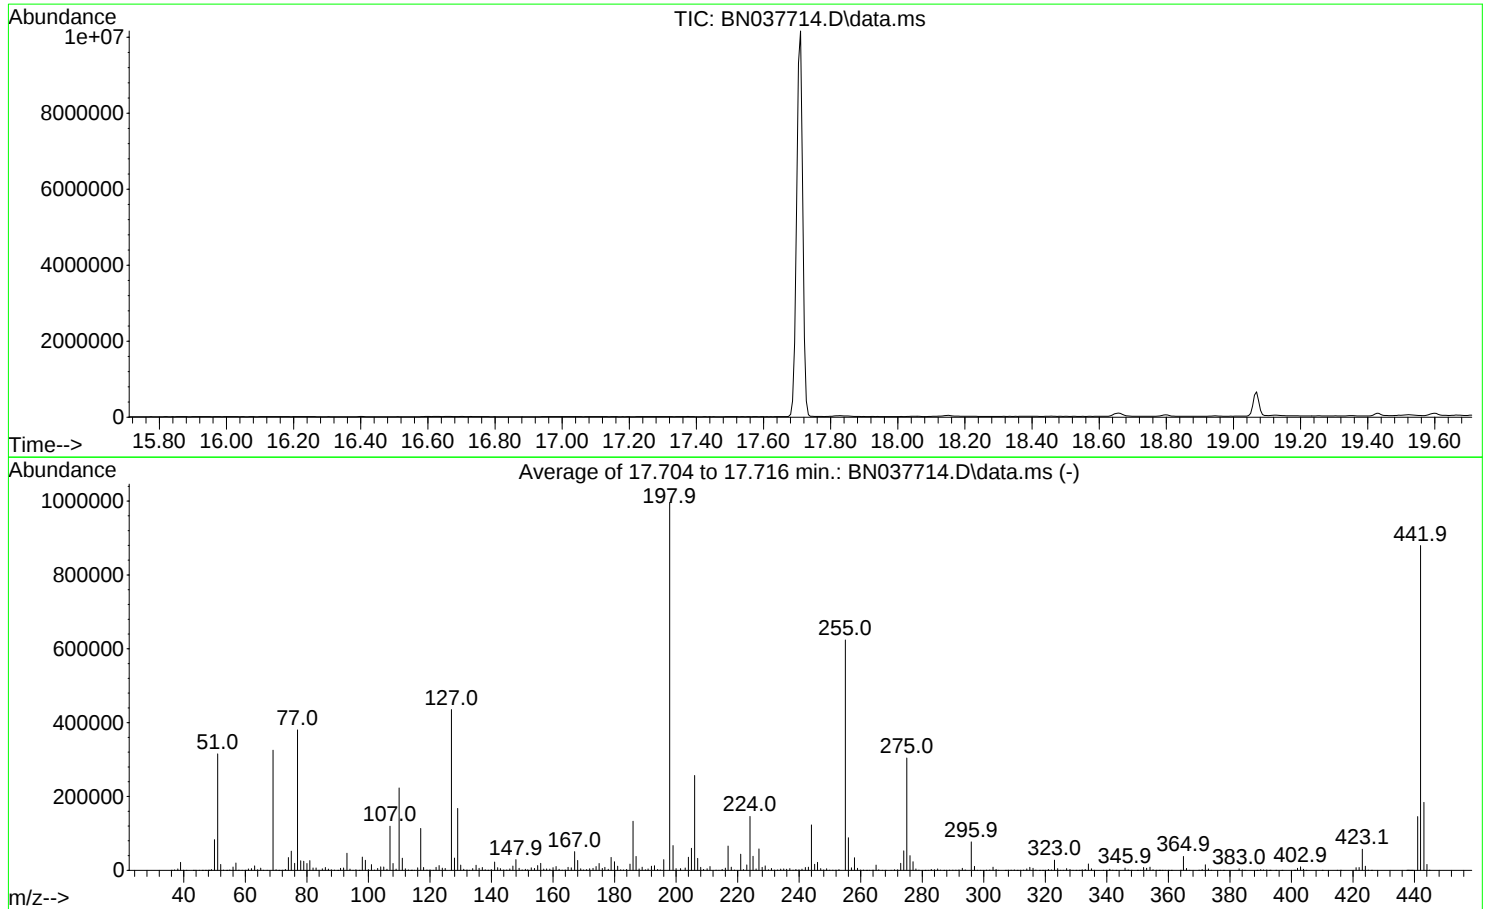

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	315514	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.7	325589	PASS
70	69	0.00	2	0.5	1633	PASS
127	198	10	80	43.7	435520	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	996160	PASS
199	198	5	9	6.7	67064	PASS
275	198	10	60	30.5	304107	PASS
365	198	1	100	3.8	37835	PASS
441	198	0.01	100	14.6	145579	PASS
442	198	50	100	88.3	879573	PASS
443	442	15	24	20.9	184107	PASS