

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091619\
 Data File : BN007671.D
 Acq On : 16 Sep 2019 18:03
 Operator : HP/JU
 Sample : K4780-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0BM2

Quant Time: Sep 17 02:32:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 16 18:09:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	704997	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	2998205	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	1874790	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	3858410	20.00	ng/ul	0.00
77) Chrysene-d12	21.27	240	3637204	20.00	ng/ul	0.00
85) Perylene-d12	23.49	264	4052769	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	69743	3.76	ng/uL	0.00
5) Phenol-d5	6.88	99	433755	6.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	1031735	27.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.24	132	1147160	24.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.40	113	806783	15.77	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	685712	31.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.56	143	671880	32.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	1376935	28.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.61	131	313170	4.95	ng/ul	0.00
43) Dimethylphthalate-d6	13.75	166	4870299	32.65	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	5356187	31.35	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	152472	5.75	ng/ul	0.00
57) Fluorene-d10	15.33	176	4053623	31.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	167246	8.03	ng/ul	0.00
70) Anthracene-d10	17.17	188	6460623	33.64	ng/ul	0.00
78) Pyrene-d10	19.47	212	7193078	36.72	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.35	264	7398839	35.09	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.79	163	493844	3.248	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091619\
Data File : BN007671.D
Acq On : 16 Sep 2019 18:03
Operator : HP/JU
Sample : K4780-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0BM2

Quant Time: Sep 17 02:32:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 16 18:09:41 2019
Response via : Initial Calibration

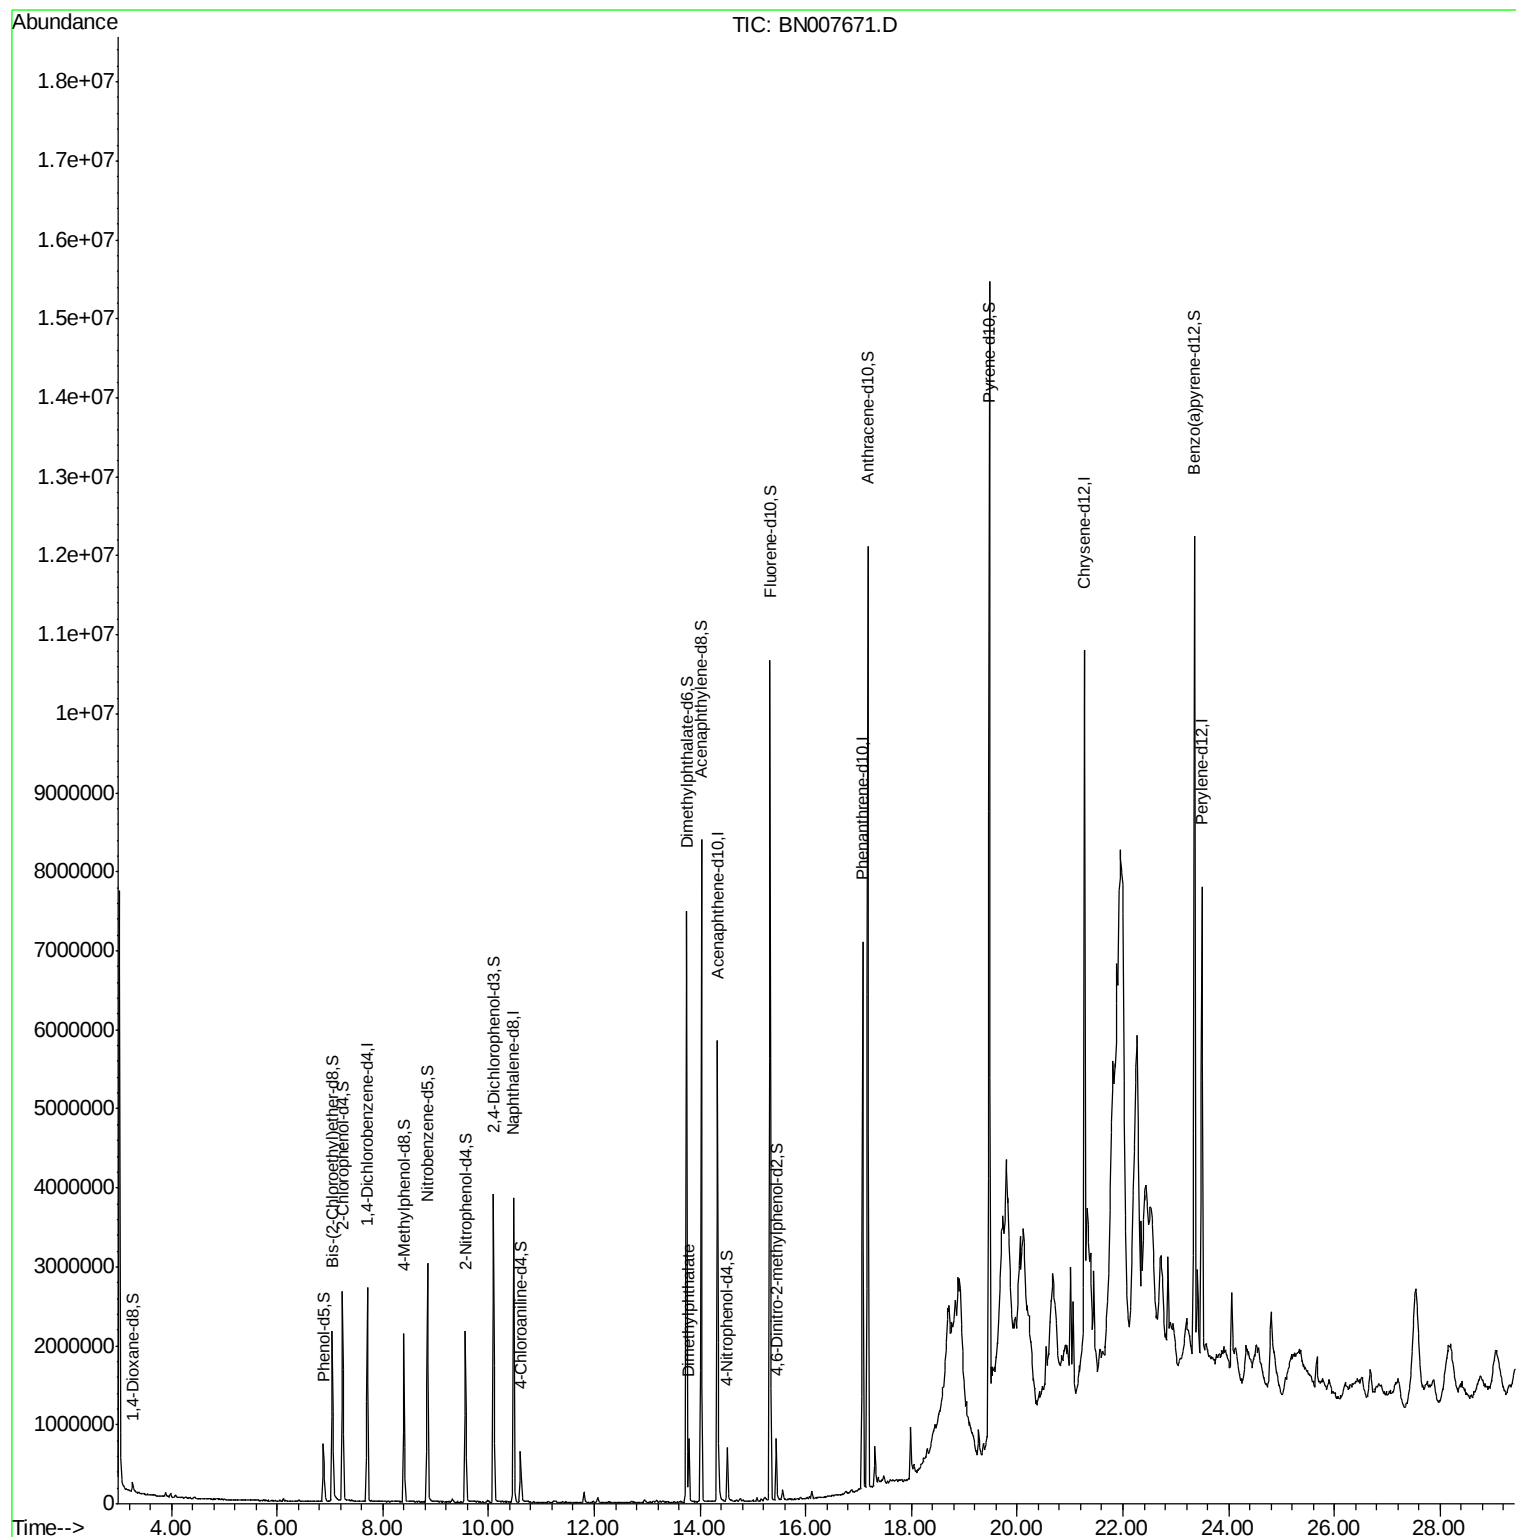

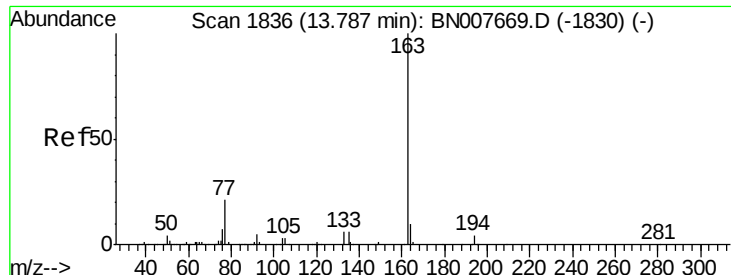

#44

Dimethylphthalate

Concen: 3.248 ng/ul

RT: 13.79 min Scan# 1836

Delta R.T. -0.00 min

Lab File: BN007671.D

Acq: 16 Sep 2019 18:03

Instrument :

BNA_N

ClientSampleId :

H0BM2


Tot Ion:163 Resp: 493844

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2

164 9.9 8.4 12.6

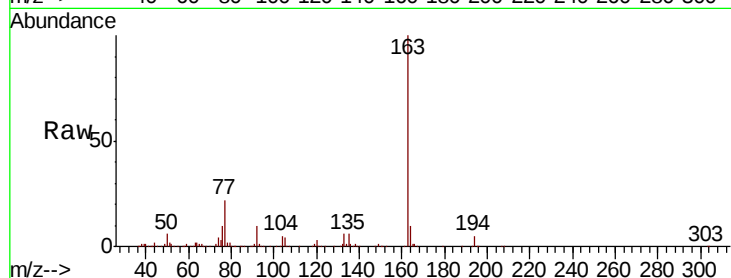

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

