

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN091619\
 Data File : BN007682.D
 Acq On : 17 Sep 2019 00:38
 Operator : HP/JU
 Sample : PB123106BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	17	rVB	459911	566680	3.03%	0.305%
2	3.270	44	48	57	rVB	146605	234280	1.25%	0.126%
3	3.981	166	169	175	rVB2	24719	35648	0.19%	0.019%
4	6.875	654	661	673	rBV	2998513	4668608	25.00%	2.509%
5	7.046	684	690	707	rBV	2020177	3439671	18.42%	1.849%
6	7.240	716	723	737	rVB	3120079	4823666	25.83%	2.593%
7	7.705	795	802	813	rBV	2380497	3689621	19.76%	1.983%
8	8.399	913	920	935	rBV	3667597	5813446	31.13%	3.124%
9	8.846	988	996	1010	rBV	2796965	4537436	24.30%	2.439%
10	9.563	1109	1118	1133	rBV	2115242	3463415	18.55%	1.861%
11	10.093	1200	1208	1223	rBV	3551827	6034237	32.32%	3.243%
12	10.475	1264	1273	1281	rBV	3313008	5434404	29.10%	2.921%
13	10.604	1287	1295	1311	rBV	3668137	6145608	32.91%	3.303%
14	12.063	1536	1543	1548	rVB	64276	99085	0.53%	0.053%
15	13.740	1822	1828	1843	rBV	6462174	9114819	48.82%	4.899%
16	14.022	1868	1876	1890	rBV	7418481	10981651	58.81%	5.902%
17	14.328	1921	1928	1939	rBV2	5099589	7742617	41.47%	4.161%
18	14.522	1952	1961	1976	rBV	2952997	4411872	23.63%	2.371%
19	14.751	1995	2000	2006	rVB8	18226	29906	0.16%	0.016%
20	15.328	2091	2098	2108	rBV	9606038	13743649	73.61%	7.387%
21	15.439	2108	2117	2130	rVV	1891867	2580363	13.82%	1.387%
22	15.563	2133	2138	2146	rVB2	120874	176807	0.95%	0.095%
23	16.110	2224	2231	2236	rVB3	41017	57329	0.31%	0.031%
24	16.757	2335	2341	2344	rBV6	20501	29113	0.16%	0.016%
25	16.857	2353	2358	2365	rBV3	21165	40778	0.22%	0.022%
26	17.075	2388	2395	2402	rBV2	6470398	9502707	50.89%	5.107%
27	17.169	2404	2411	2423	rBV	10678432	15244123	81.64%	8.193%
28	17.310	2430	2435	2439	rBV6	25916	44361	0.24%	0.024%
29	17.981	2546	2549	2554	rBV5	32333	52227	0.28%	0.028%
30	18.033	2555	2558	2563	rVB7	17248	31993	0.17%	0.017%
31	18.292	2599	2602	2608	rBV8	15668	23701	0.13%	0.013%
32	18.510	2636	2639	2644	rBV7	16031	22250	0.12%	0.012%
33	18.863	2696	2699	2702	rBV4	22644	26409	0.14%	0.014%
34	19.039	2724	2729	2732	rBV7	16840	29484	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN091619\
 Data File : BN007682.D
 Acq On : 17 Sep 2019 00:38
 Operator : HP/JU
 Sample : PB123106BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
 Title : SVOA CALIBRATION

35	19.104	2734	2740	2744	rBV	123188	183738	0.98%	0.099%
36	19.269	2766	2768	2775	rVB7	17836	23818	0.13%	0.013%
37	19.357	2779	2783	2790	rVB	110106	149889	0.80%	0.081%
38	19.469	2796	2802	2809	rBV	14044353	18671881	100.00%	10.035%
39	20.292	2940	2942	2946	rBV5	21152	21938	0.12%	0.012%
40	20.951	3050	3054	3058	rBV2	73989	120257	0.64%	0.065%
41	21.004	3060	3063	3067	rVV	127863	168320	0.90%	0.090%
42	21.051	3067	3071	3077	rVV	396591	517826	2.77%	0.278%
43	21.263	3102	3107	3118	rBV	8603258	11181767	59.89%	6.010%
44	21.386	3124	3128	3135	rBV	313487	488349	2.62%	0.262%
45	21.880	3210	3212	3216	rVB2	109296	112245	0.60%	0.060%
46	22.339	3287	3290	3296	rVB	252575	332083	1.78%	0.178%
47	22.845	3373	3376	3382	rVB	353114	498105	2.67%	0.268%
48	23.345	3454	3461	3468	rBV	10030296	17754918	95.09%	9.543%
49	23.410	3468	3472	3477	rVV	444336	712592	3.82%	0.383%
50	23.486	3478	3485	3498	rVB	5973057	10830179	58.00%	5.821%
51	24.051	3577	3581	3590	rVB	365487	643361	3.45%	0.346%
52	24.792	3702	3707	3718	rVB2	366707	778073	4.17%	0.418%


Sum of corrected areas: 186061303

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN091619\
Data File : BN007682.D
Acq On : 17 Sep 2019 00:38
Operator : HP/JU
Sample : PB123106BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

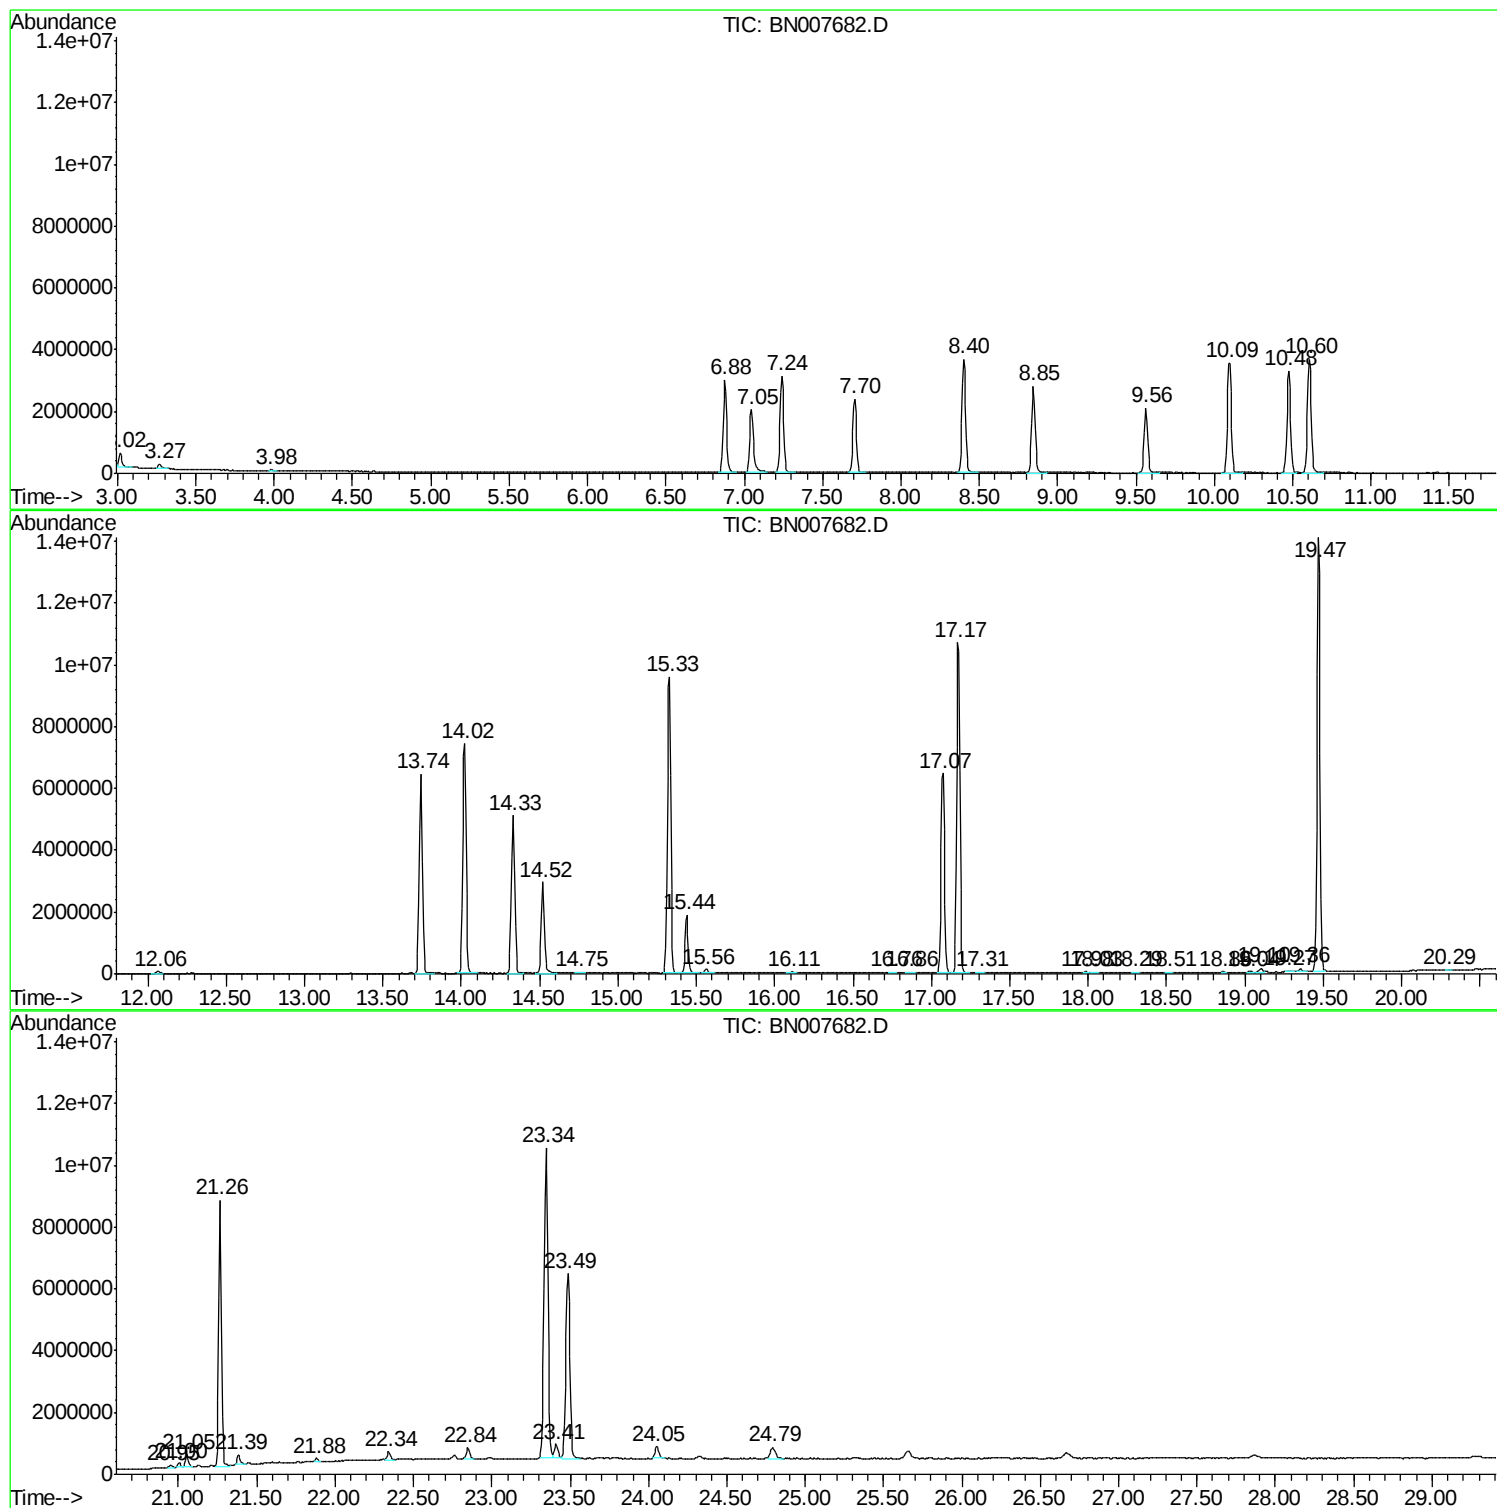

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN091619\
Data File : BN007682.D
Acq On : 17 Sep 2019 00:38
Operator : HP/JU
Sample : PB123106BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.02	3.07 ng/ul	566680	1,4-Dichlorobenzene-d4	7.70

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	43
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			N-Ethylformamide	73	C3H7NO	000627-45-2	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

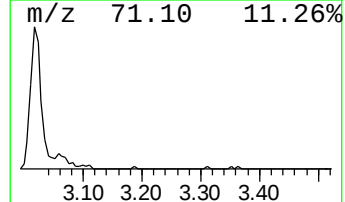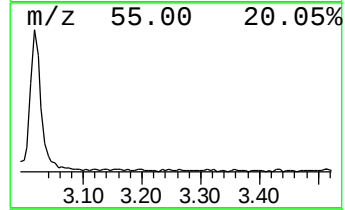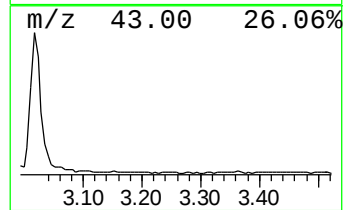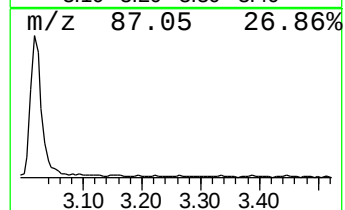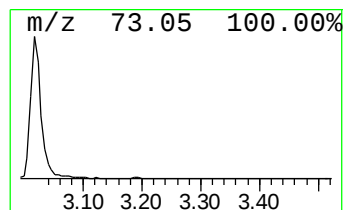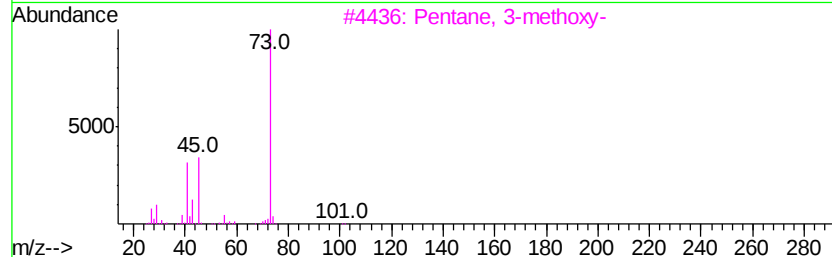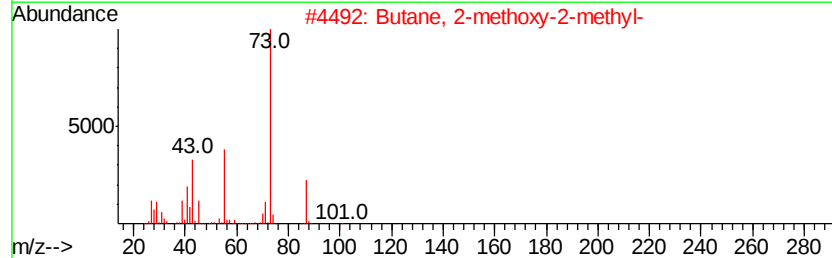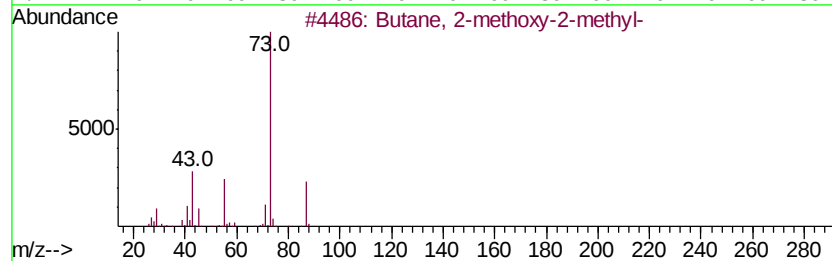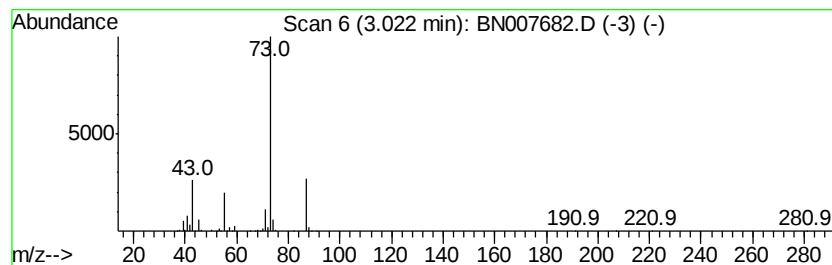

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091619\
Data File : BN007682.D
Acq On : 17 Sep 2019 00:38
Operator : HP/JU
Sample : PB123106BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.02	3.1	ng/ul	566680	1	7.70	3689620	20.0