

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091718\
 Data File : BN002737.D
 Acq On : 17 Sep 2018 21:50
 Operator : JU/SJ
 Sample : PB112909BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 18 02:48:48 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 18 02:47:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	126389	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	543103	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	285160	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	570653	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	529678	20.00	ng/ul	0.00
85) Perylene-d12	23.45	264	551807	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	18774	6.85	ng/uL	0.00
5) Phenol-d5	6.83	99	365417	34.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	236902	35.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	304777	34.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	292047	35.13	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	147338	35.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	168576	35.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	283465	32.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	381666	38.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	864805	38.74	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1105359	37.93	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	104059	28.19	ng/ul	0.00
57) Fluorene-d10	15.28	176	741719	37.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	103016	28.86	ng/ul	0.00
70) Anthracene-d10	17.13	188	1047769	38.46	ng/ul	0.00
78) Pyrene-d10	19.43	212	1044750	37.38	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.31	264	1131642	38.96	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.36	70	6728	1.045	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091718\
Data File : BN002737.D
Acq On : 17 Sep 2018 21:50
Operator : JU/SJ
Sample : PB112909BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 18 02:48:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 18 02:47:57 2018
Response via : Initial Calibration

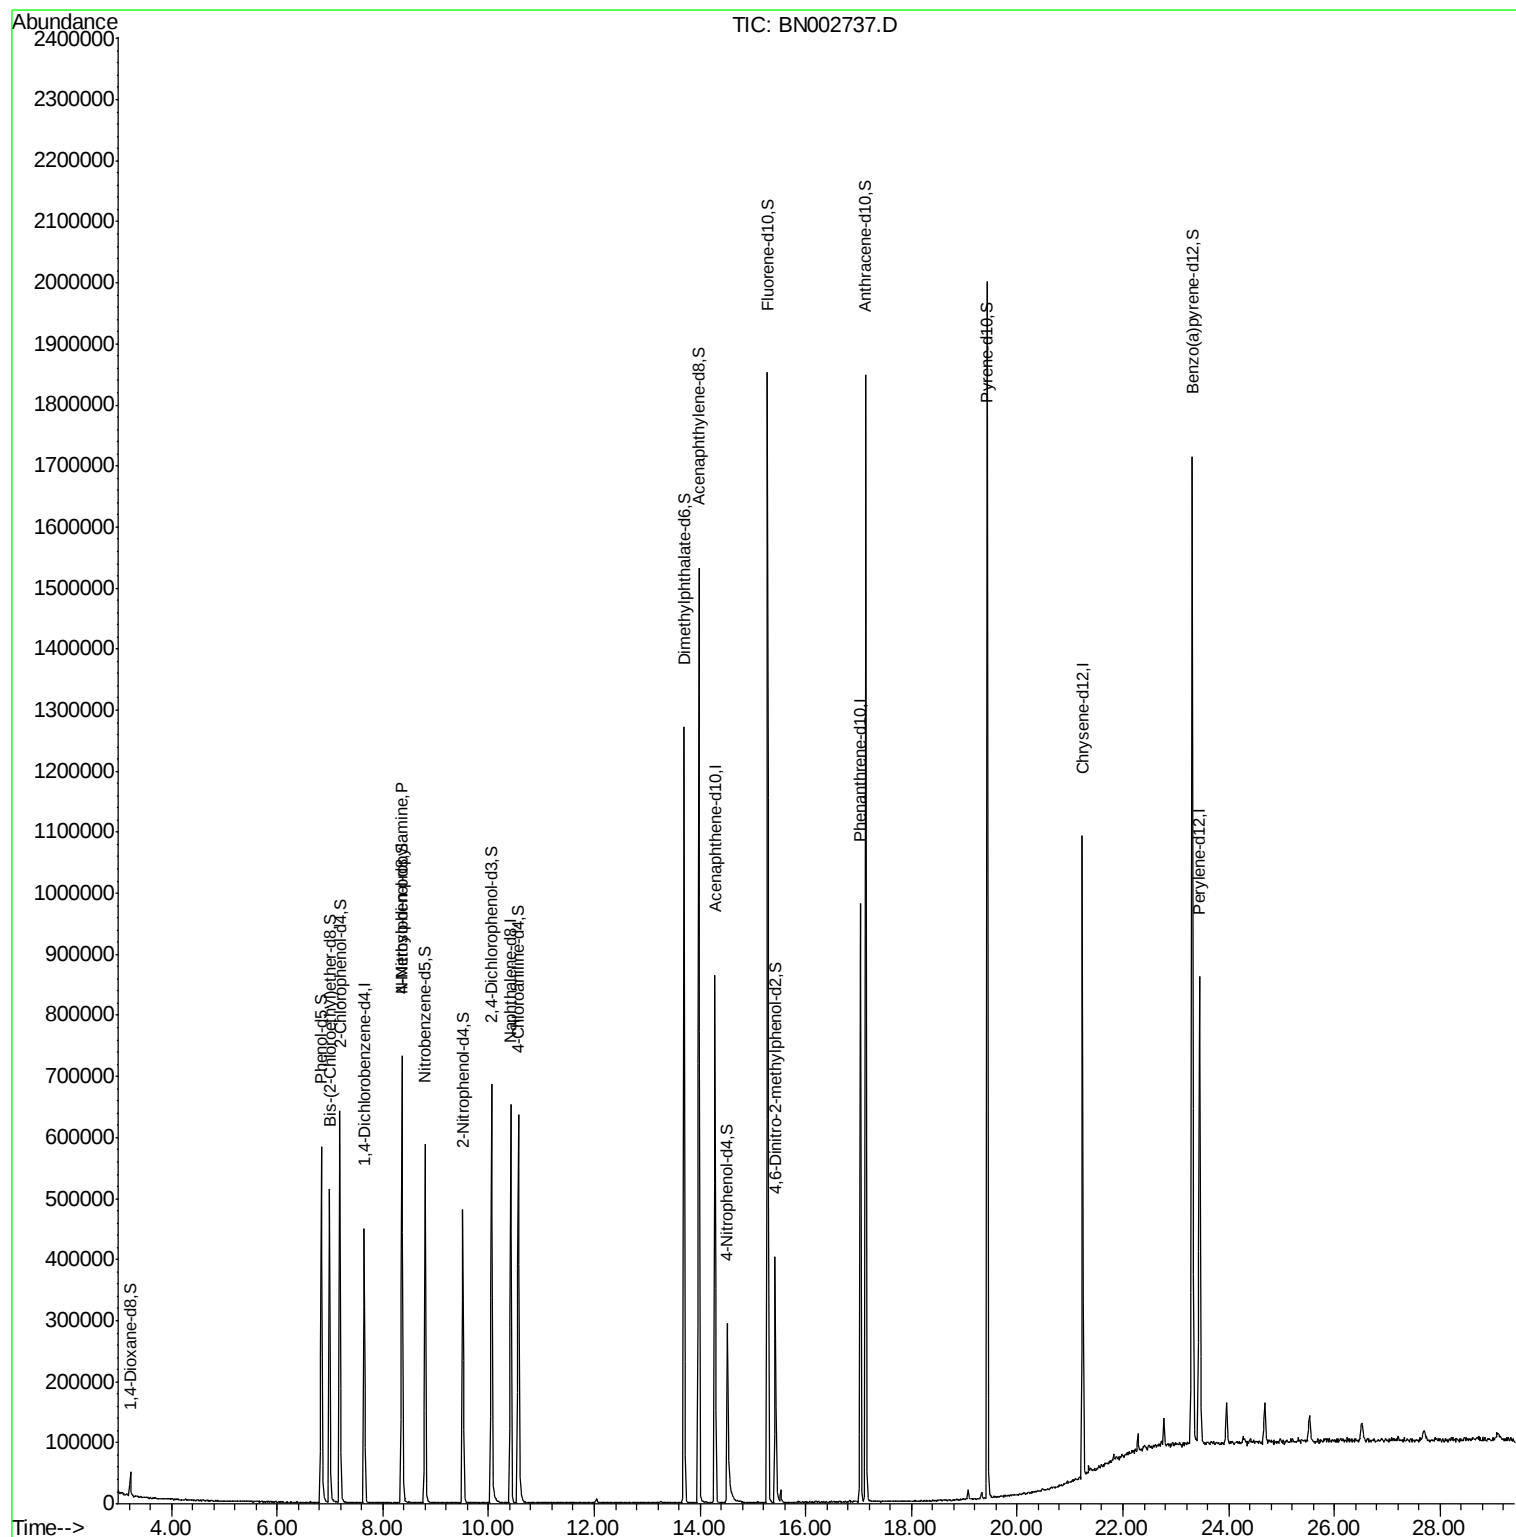

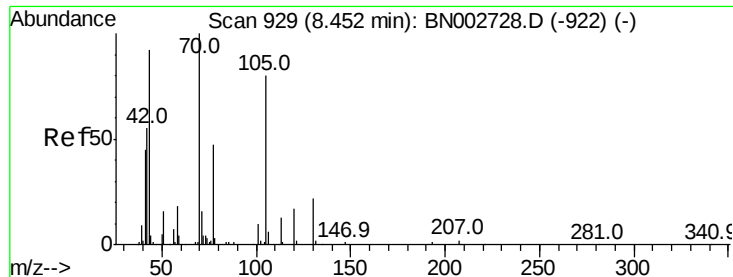

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.045 ng/ul
 RT: 8.36 min Scan# 913
 Delta R.T. -0.09 min
 Lab File: BN002737.D
 Acq: 17 Sep 2018 21:50

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 6728
 Ion Ratio Lower Upper
 70 100
 42 376.4 47.7 71.5#
 101 0.0 8.0 12.0#
 130 0.0 16.0 24.0#

