

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091818\
 Data File : BN002748.D
 Acq On : 18 Sep 2018 12:35
 Operator : JU/SJ
 Sample : PB112908BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 19 01:16:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 19 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	126479	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	572188	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	337730	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	755661	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	658731	20.00	ng/ul	0.00
85) Perylene-d12	23.45	264	594414	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	22821	8.32	ng/uL	0.00
5) Phenol-d5	6.83	99	452995	42.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	297316	44.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	379986	42.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	371819	44.70	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	186591	42.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	220562	43.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	370865	40.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	502940	48.01	ng/ul	0.00
43) Dimethylphthalate-d6	13.70	166	1238492	46.85	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1531922	44.38	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	170981	39.12	ng/ul	0.00
57) Fluorene-d10	15.28	176	1069939	46.20	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	170984	36.17	ng/ul	0.00
70) Anthracene-d10	17.13	188	1607437	44.56	ng/ul	0.00
78) Pyrene-d10	19.43	212	1652536	47.54	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.31	264	1409246	45.04	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.36	70	8822	1.370	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091818\
Data File : BN002748.D
Acq On : 18 Sep 2018 12:35
Operator : JU/SJ
Sample : PB112908BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 19 01:16:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 19 01:15:51 2018
Response via : Initial Calibration

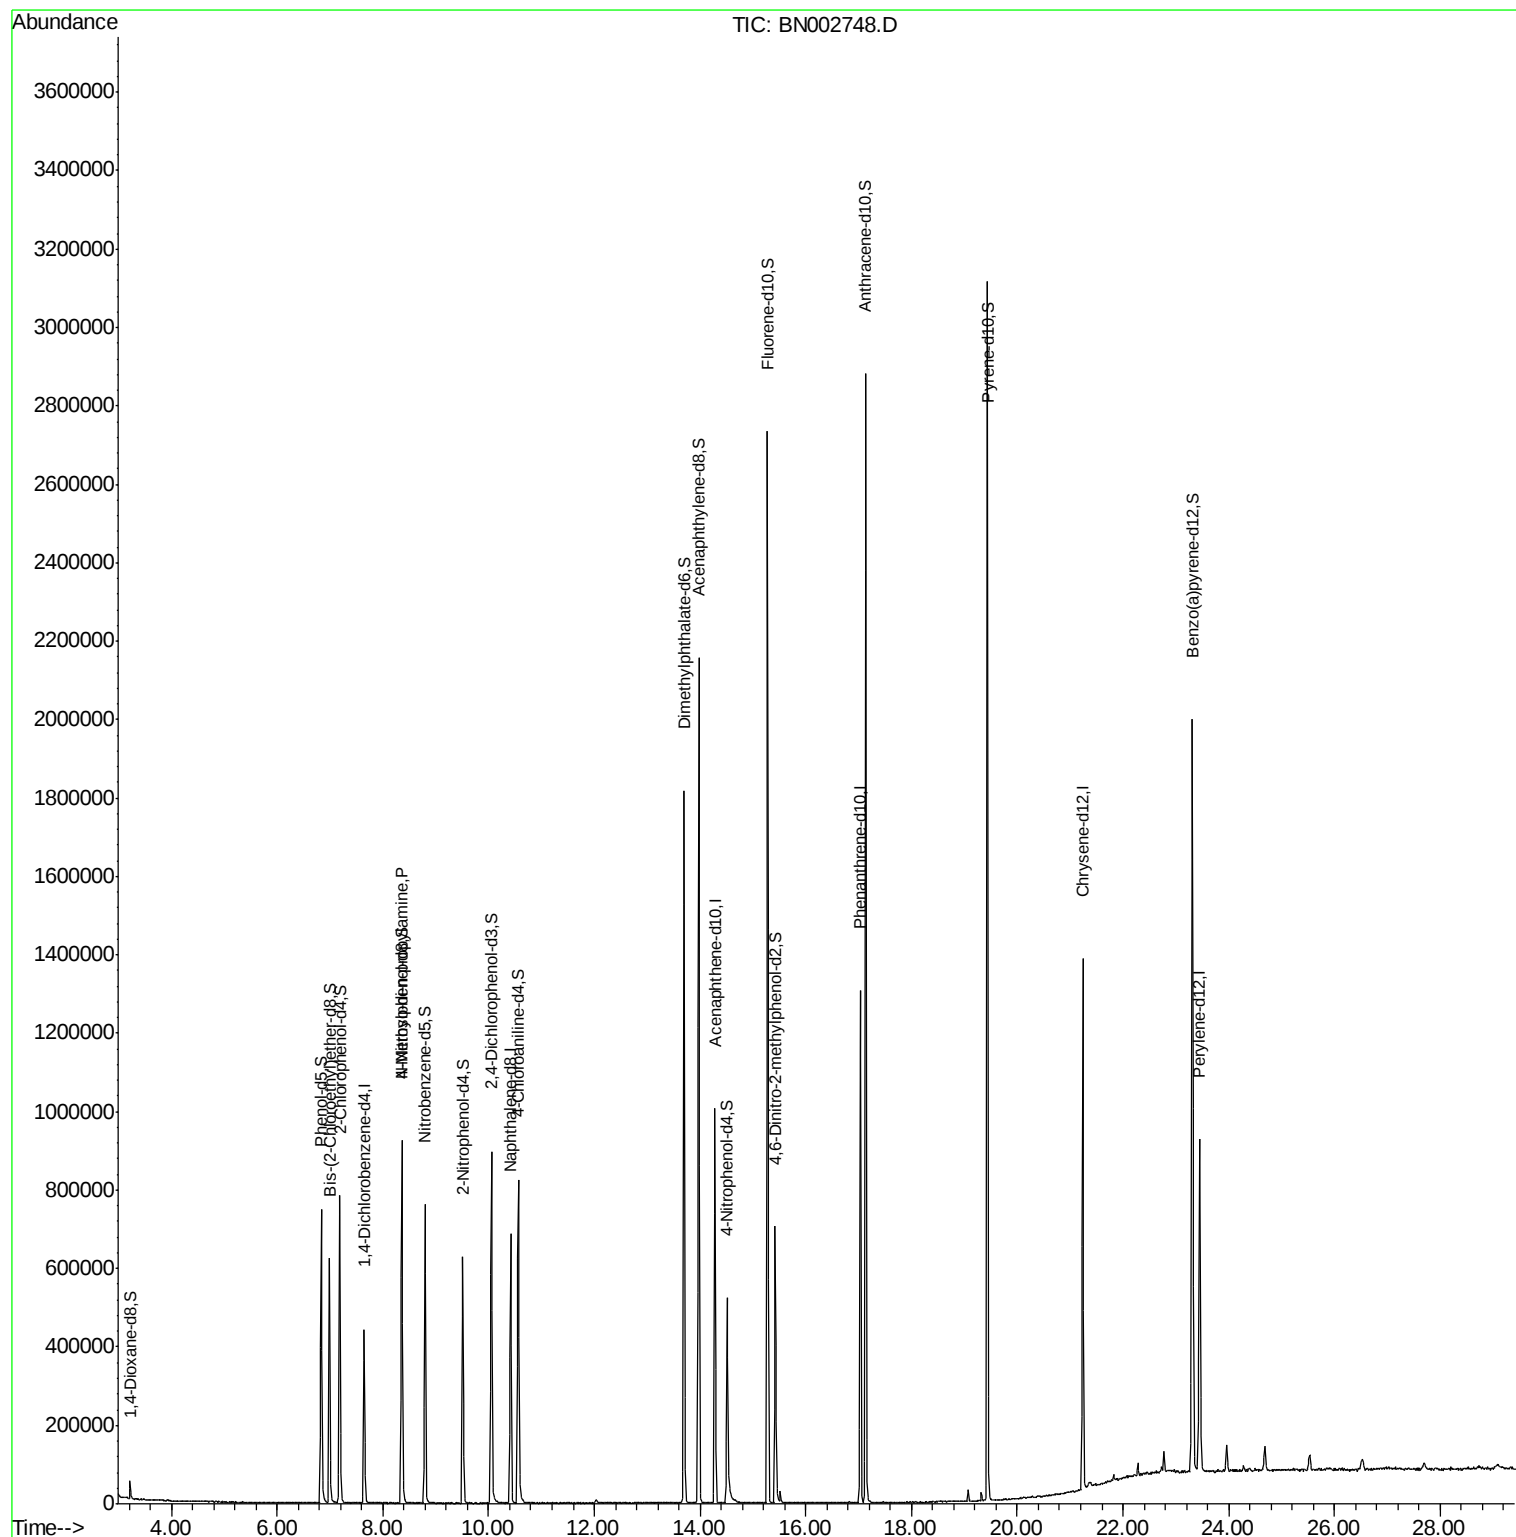

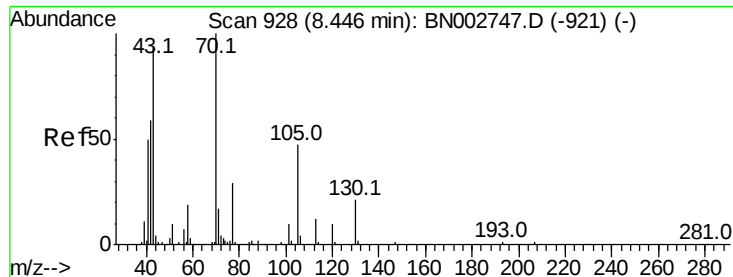

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.370 ng/ul
 RT: 8.36 min Scan# 913
 Delta R.T. -0.09 min
 Lab File: BN002748.D
 Acq: 18 Sep 2018 12:35

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 8822
 Ion Ratio Lower Upper
 70 100
 42 352.9 47.7 71.5#
 101 0.0 8.0 12.0#
 130 0.0 16.0 24.0#

