

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091818\
 Data File : BN002755.D
 Acq On : 18 Sep 2018 16:49
 Operator : JU/SJ
 Sample : J4893-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 19 01:16:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 19 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	128676	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	521470	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	270586	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	541989	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	540166	20.00	ng/ul	0.00
85) Perylene-d12	23.45	264	573760	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	18325	6.57	ng/uL	0.00
5) Phenol-d5	6.83	99	96684	8.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	274619	40.47	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	298371	33.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	175384	20.72	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	171635	42.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	194502	42.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	300082	36.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	22246	2.33	ng/ul	0.02
43) Dimethylphthalate-d6	13.70	166	912950	43.10	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1188227	42.96	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	16491	4.71	ng/ul	0.03
57) Fluorene-d10	15.28	176	802843	43.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	117921	34.78	ng/ul	0.00
70) Anthracene-d10	17.13	188	1171979	45.29	ng/ul	0.00
78) Pyrene-d10	19.43	212	1195728	41.95	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	1358444	44.98	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.75	163	240100	11.615	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091818\
Data File : BN002755.D
Acq On : 18 Sep 2018 16:49
Operator : JU/SJ
Sample : J4893-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 19 01:16:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 19 01:15:51 2018
Response via : Initial Calibration

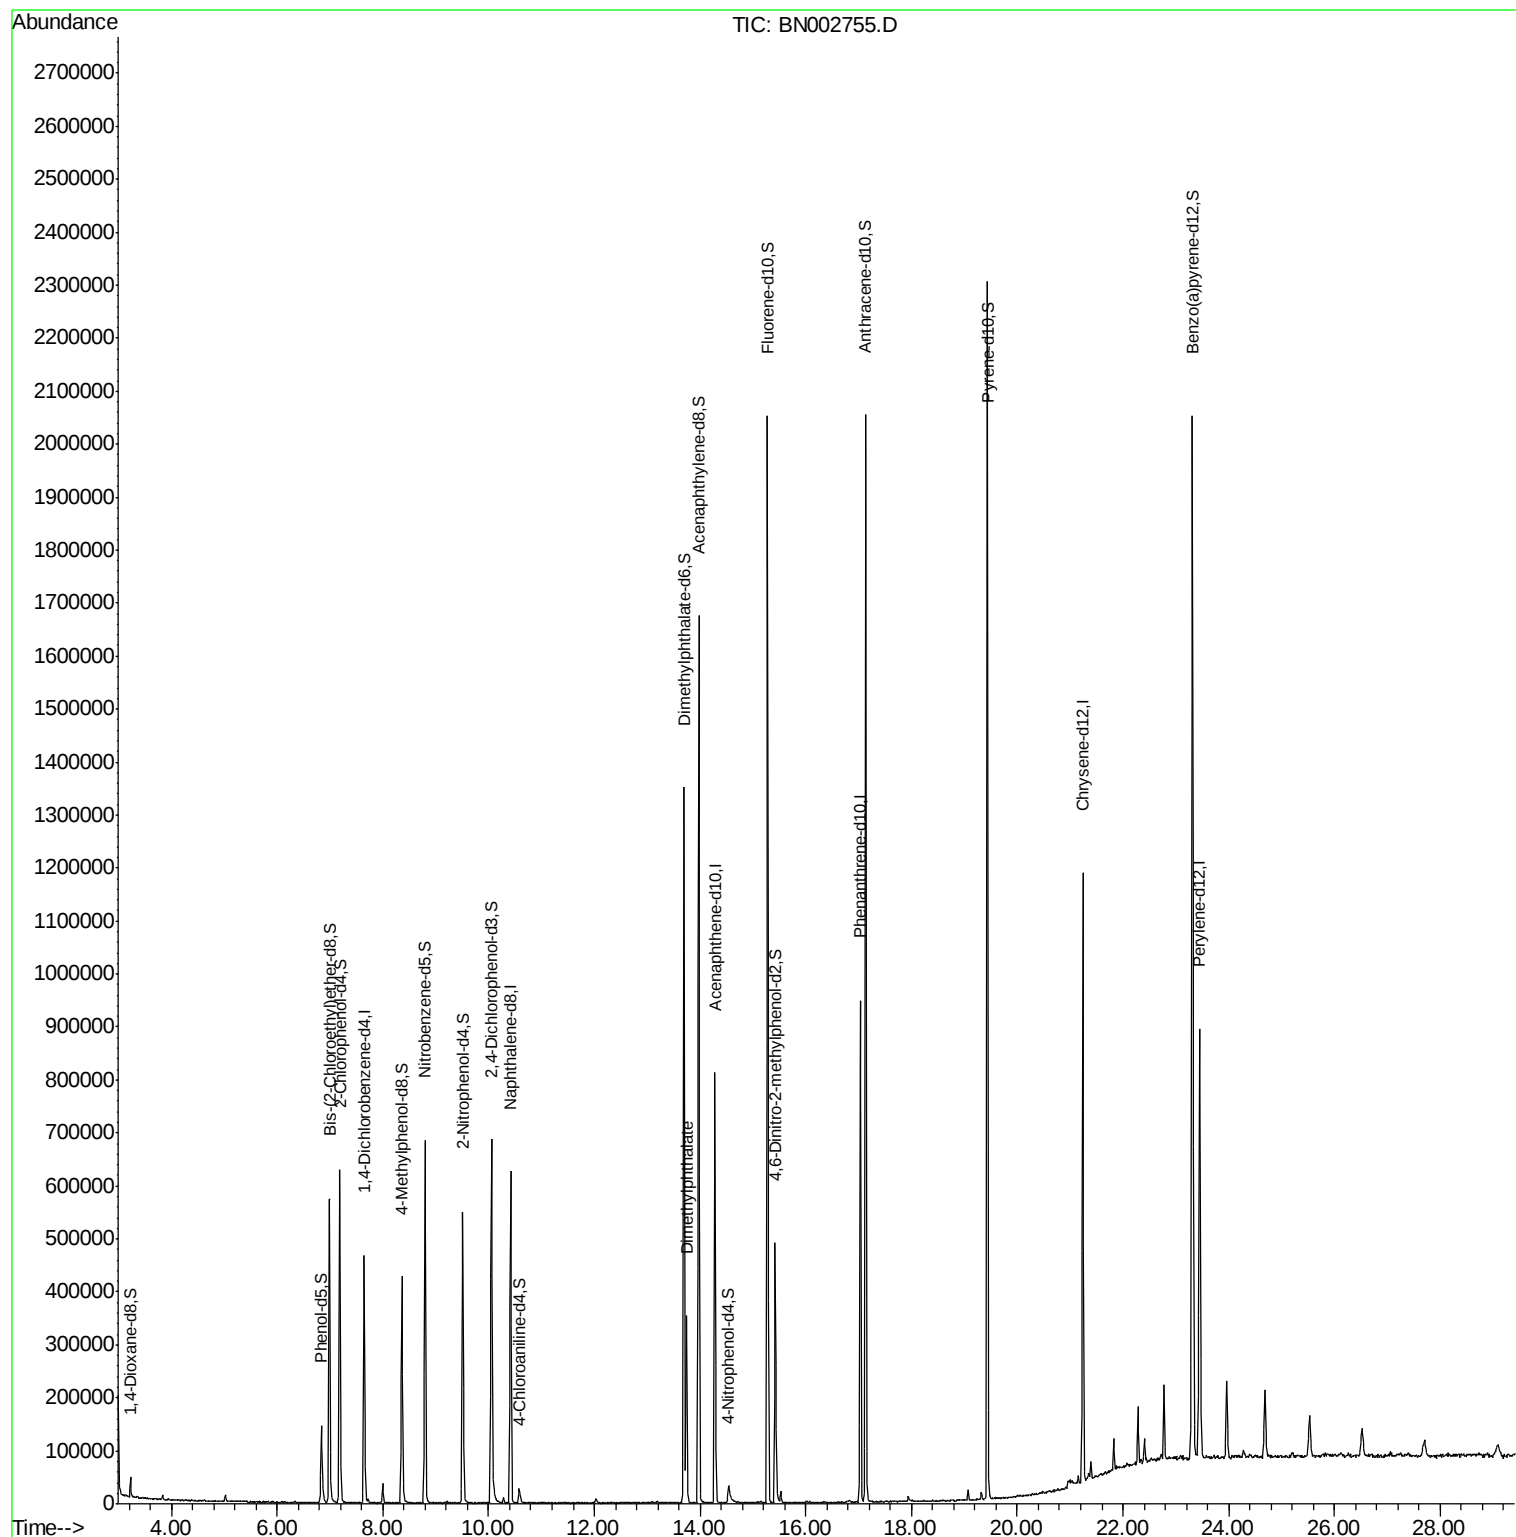

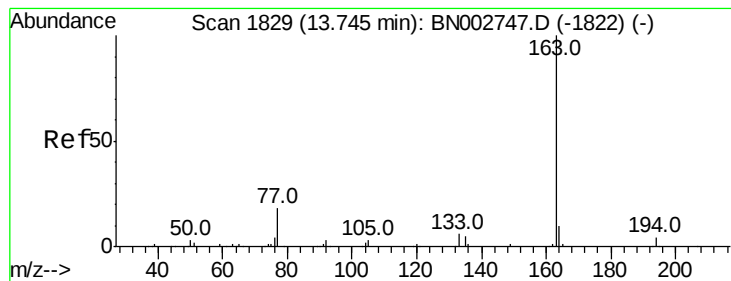

#44

Dimethylphthalate

Concen: 11.615 ng/ul

RT: 13.75 min Scan# 1829

Delta R.T. -0.00 min

Lab File: BN002755.D

Acq: 18 Sep 2018 16:49

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 240100

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 9.8 8.1 12.1

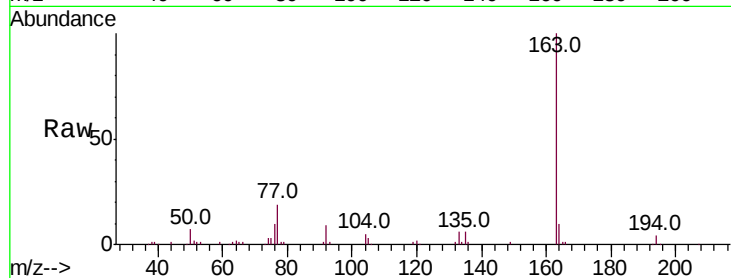

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

