

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091818\
 Data File : BN002752.D
 Acq On : 18 Sep 2018 15:04
 Operator : JU/SJ
 Sample : J4893-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C08N5

Quant Time: Sep 19 01:16:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 19 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	169198	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	707522	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	385246	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	765899	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	659104	20.00	ng/ul	0.00
85) Perylene-d12	23.45	264	686139	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	4466	1.22	ng/uL	0.00
5) Phenol-d5	6.83	99	87053	6.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	250482	28.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	265474	22.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	164225	14.76	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	159423	29.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	183808	29.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	297551	26.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	16617	1.28	ng/ul	0.02
43) Dimethylphthalate-d6	13.70	166	986655	32.72	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1189656	30.21	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	23251	4.66	ng/ul	0.02
57) Fluorene-d10	15.28	176	856626	32.43	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	143881	30.03	ng/ul	0.00
70) Anthracene-d10	17.13	188	1271074	34.76	ng/ul	0.00
78) Pyrene-d10	19.44	212	1276151	36.69	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	1308695	36.24	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.75	163	173594	5.898	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091818\
Data File : BN002752.D
Acq On : 18 Sep 2018 15:04
Operator : JU/SJ
Sample : J4893-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
C08N5

Quant Time: Sep 19 01:16:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 19 01:15:51 2018
Response via : Initial Calibration

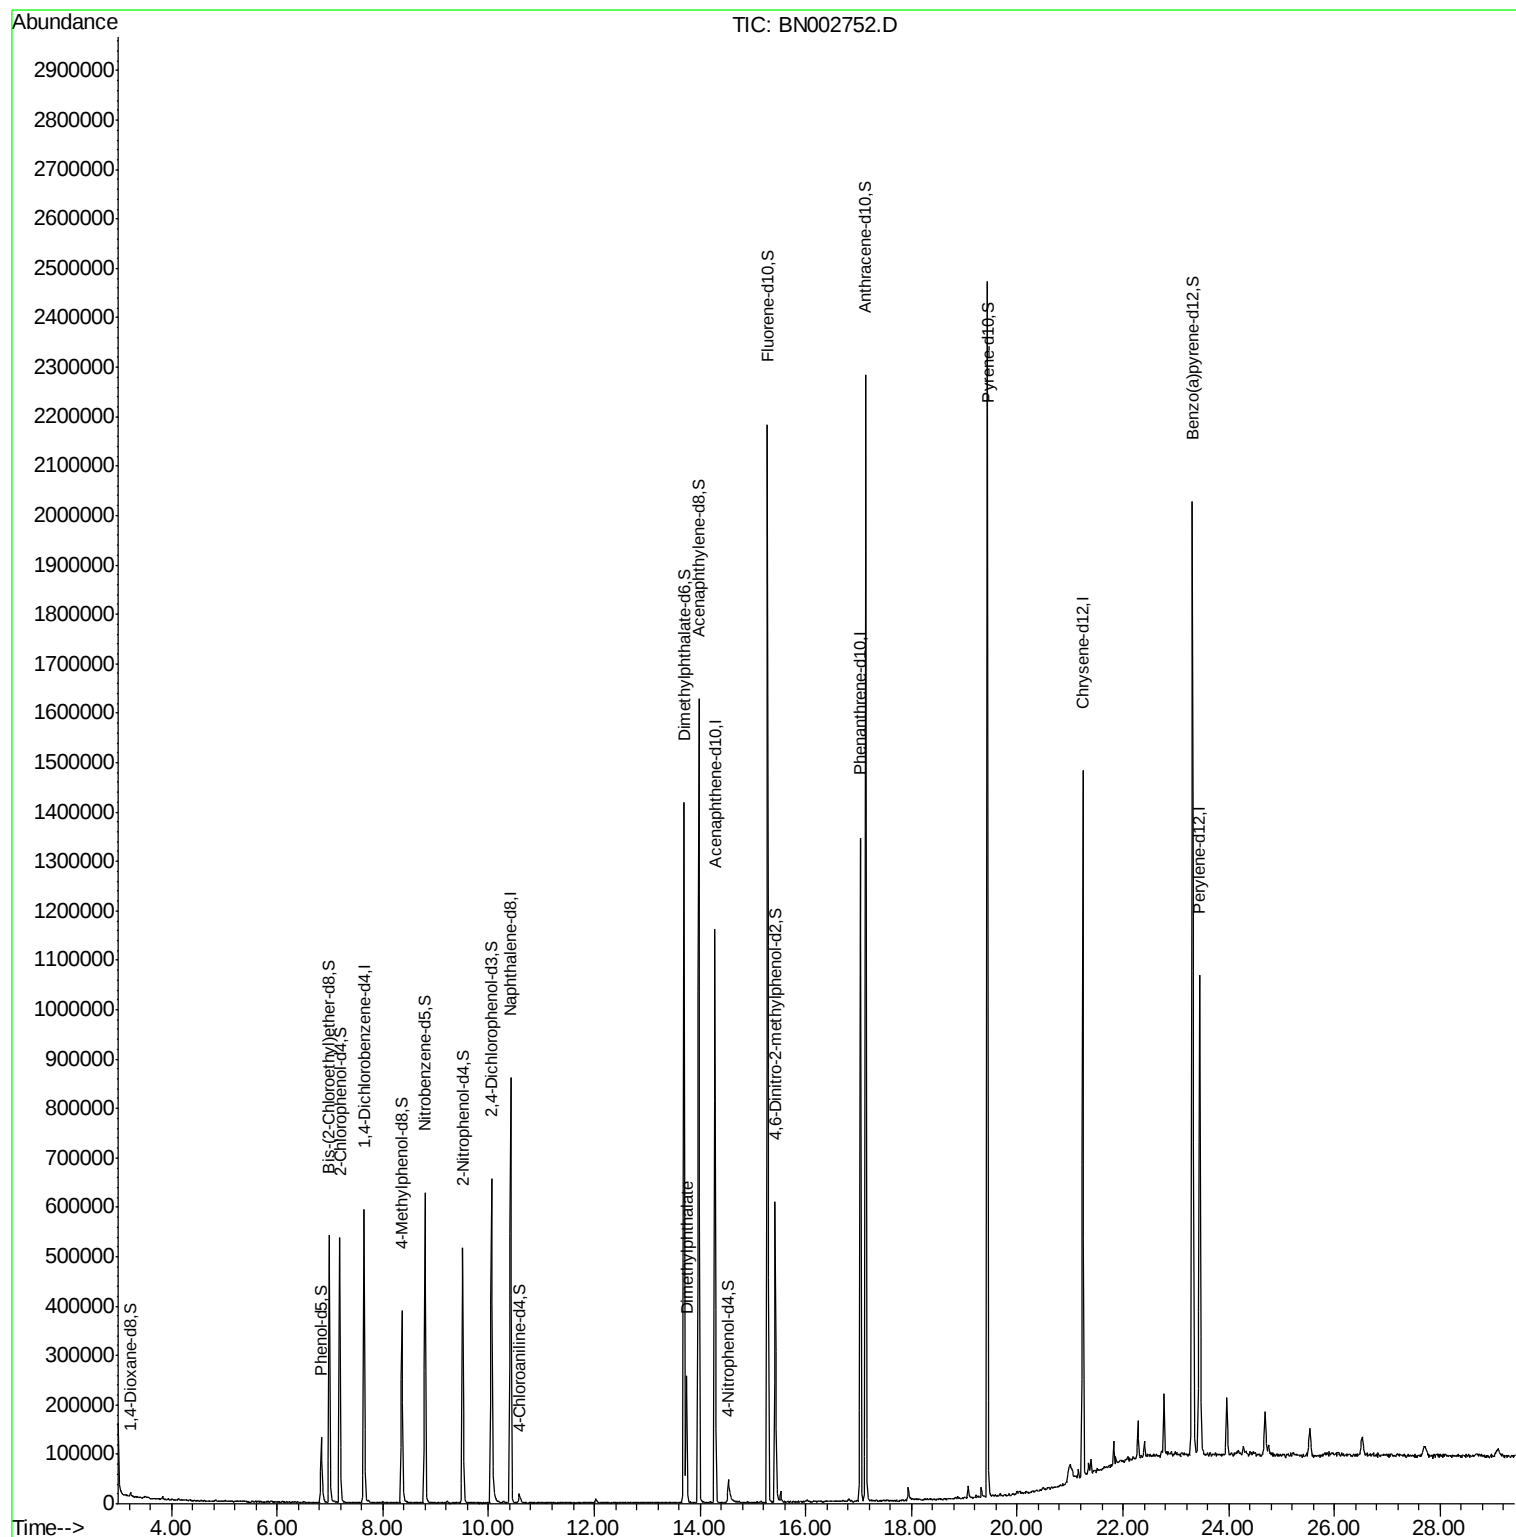

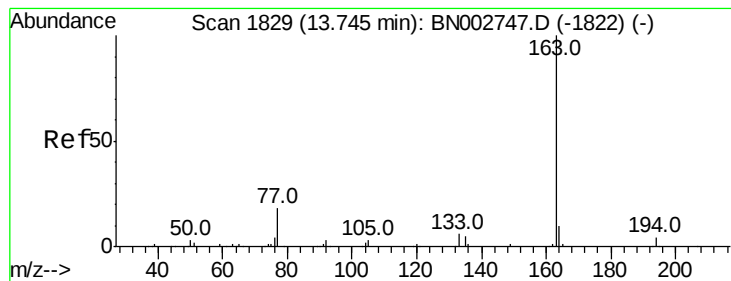

#44

Dimethylphthalate

Concen: 5.898 ng/ul

RT: 13.75 min Scan# 1829

Delta R.T. -0.00 min

Lab File: BN002752.D

Acq: 18 Sep 2018 15:04

Instrument :

BNA_N

ClientSampleId :

C08N5


Tot Ion:163 Resp: 173594

Ion Ratio Lower Upper

163 100

194 3.8 3.5 5.3

164 10.1 8.1 12.1

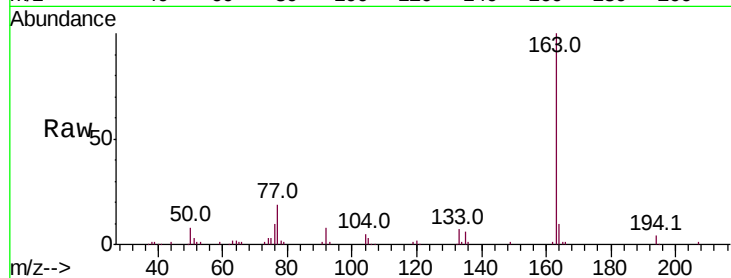

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

