

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091818\
 Data File : BN002753.D
 Acq On : 18 Sep 2018 15:39
 Operator : JU/SJ
 Sample : J4893-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C08N9

Manual Integrations
 APPROVED

Sohil
 9/19/2018 5:12:01 PM

Quant Time: Sep 19 01:32:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 19 01:15:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	179530	20.00	ng/ul	0.00
18) Naphthalene-d8	10.42	136	716465	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.28	164	371590	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	763602	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	802314	20.00	ng/ul	0.00
85) Perylene-d12	23.45	264	851771	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	6058	1.56	ng/uL	0.00
5) Phenol-d5	6.83	99	109660	7.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	319370	33.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	344616	27.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	193983	16.43	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	202558	36.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.51	143	233205	37.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	367464	32.41	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	24655	1.88	ng/ul	0.02
43) Dimethylphthalate-d6	13.70	166	1093672	37.60	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	1404387	36.98	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	26436m	5.50	ng/ul	0.02
57) Fluorene-d10	15.28	176	946299	37.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	153171	32.07	ng/ul	0.00
70) Anthracene-d10	17.13	188	1372860	37.66	ng/ul	0.00
78) Pyrene-d10	19.43	212	1470374	34.73	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	1698829	37.89	ng/ul	0.00
Target Compounds						
36) 1,2,4,5-Tetrachlorobenzene	12.46	216	66857m	5.416	ng/ul	Ovalue
44) Dimethylphthalate	13.75	163	236557	8.333	ng/ul	100
72) 1,2,3,4-Tetrachlorobenzene	13.08	216	61998	4.753	ng/uL	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091818\
Data File : BN002753.D
Acq On : 18 Sep 2018 15:39
Operator : JU/SJ
Sample : J4893-12
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C08N9

Manual Integrations
APPROVED

Sohil
9/19/2018 5:12:01 PM

Quant Time: Sep 19 01:32:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 19 01:15:51 2018
Response via : Initial Calibration

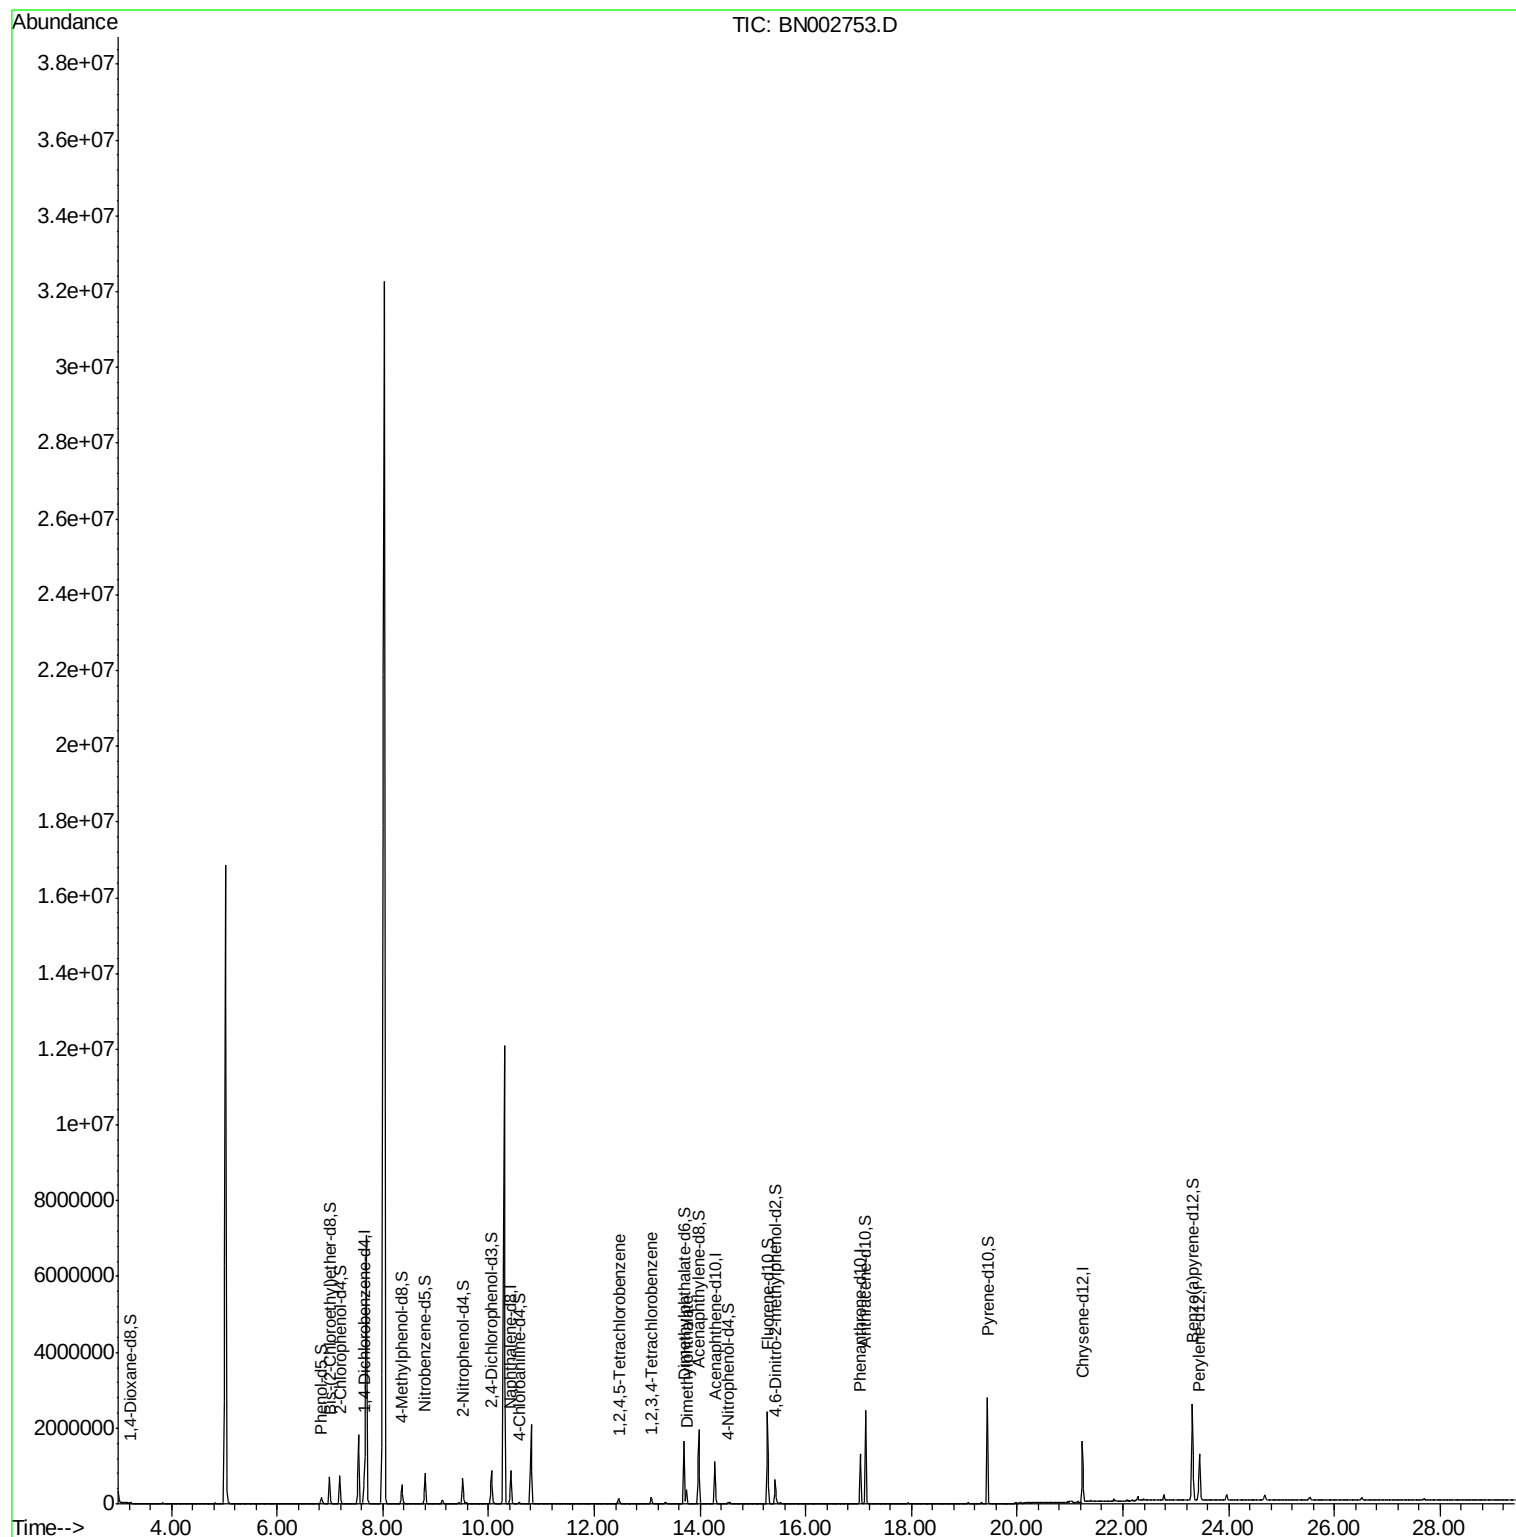

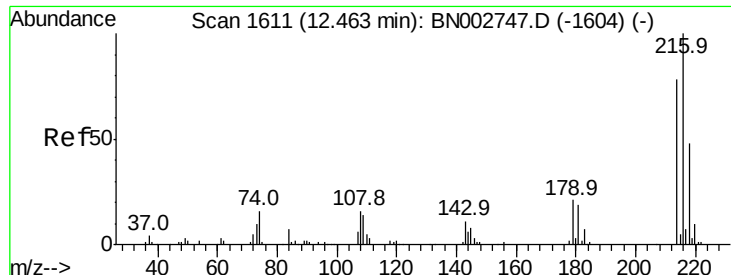





#36
 1,2,4,5-Tetrachlorobenzene
 Concen: 5.416 ng/ul m
 RT: 12.46 min Scan# 1611
 Delta R.T. 0.00 min
 Lab File: BN002753.D
 Acq: 18 Sep 2018 15:39

Instrument :
 BNA_N
 ClientSampled :
 C08N9

Tot Ion	Ratio	Resp	Lower	Upper
216	100	66857		
214	69.5		63.5	95.3
179	21.3		16.5	24.7
108	16.1		13.4	20.2




Manual Integrations
 APPROVED


Sohil
 9/19/2018 5:12:01 PM

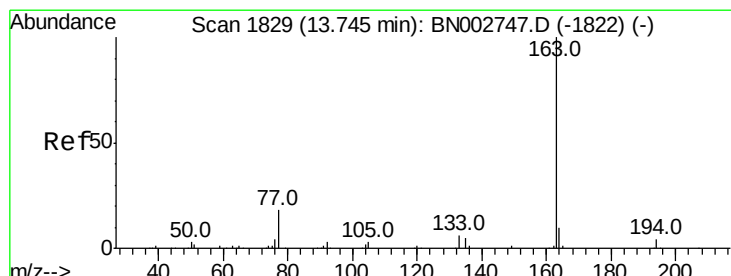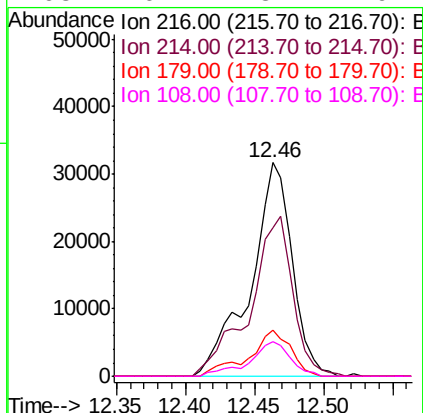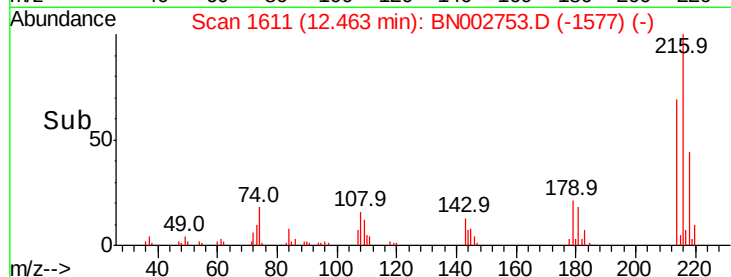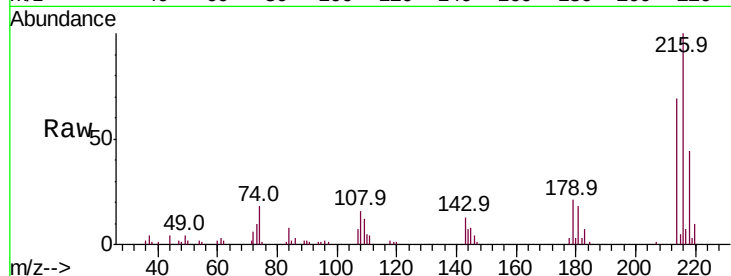

#44
 Dimethylphthalate
 Concen: 8.333 ng/ul
 RT: 13.75 min Scan# 1829
 Delta R.T. 0.00 min
 Lab File: BN002753.D
 Acq: 18 Sep 2018 15:39

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	236557		
194	4.4		3.5	5.3
164	10.2		8.1	12.1

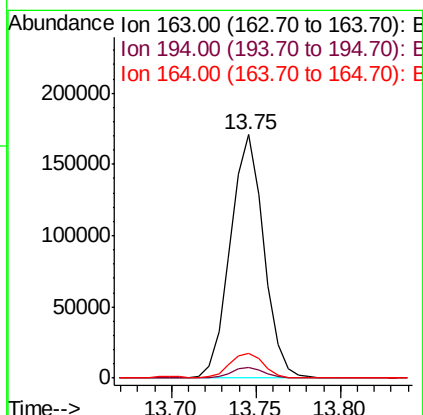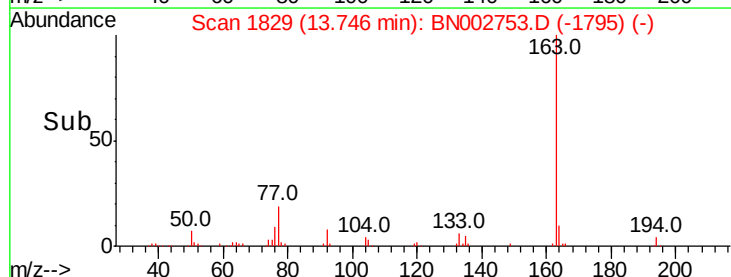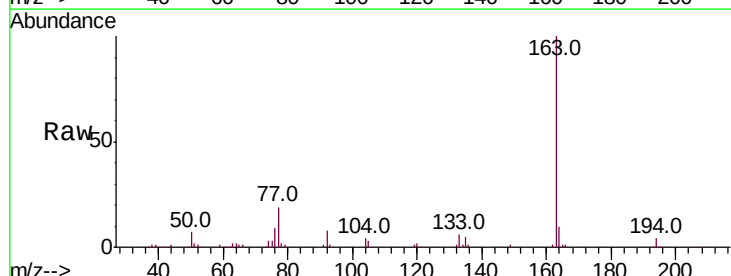

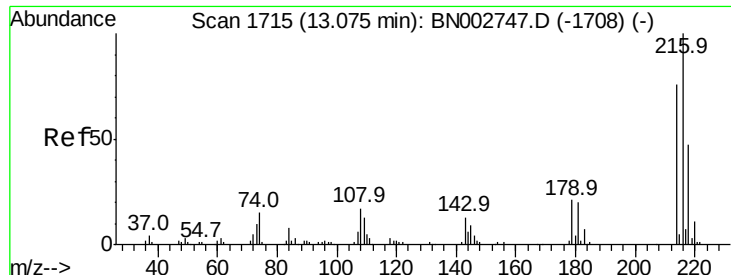


#72
 1,2,3,4-Tetrachlorobenzene
 Concen: 4.753 ng/uL
 RT: 13.08 min Scan# 1716
 Delta R.T. 0.01 min
 Lab File: BN002753.D
 Acq: 18 Sep 2018 15:39

Instrument :
 BNA_N
 ClientSampleId :
 C08N9

Tot Ion	Ratio	Resp Lower	Upper
216	100		
214	77.7	62.9	94.3
218	47.0	37.8	56.6

Manual Integrations
 APPROVED

Sohil
 9/19/2018 5:12:01 PM

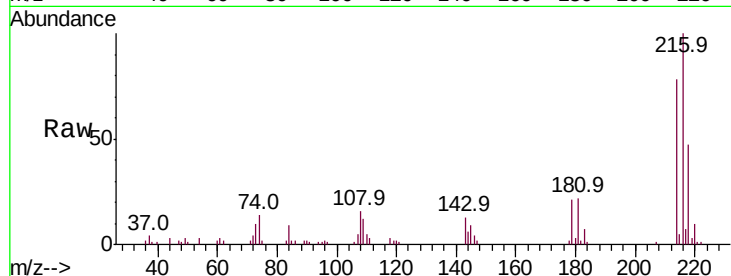

Abundance

Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

