

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091819\
 Data File : BN007719.D
 Acq On : 18 Sep 2019 23:16
 Operator : HP/JU
 Sample : K4896-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE123D3-20190912

Quant Time: Sep 19 07:26:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 18:24:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	6165	0.40	ng	0.00
7) Naphthalene-d8	10.47	136	24638	0.40	ng	0.00
13) Acenaphthene-d10	14.32	164	16017	0.40	ng	0.00
19) Phenanthrene-d10	17.07	188	36481	0.40	ng	0.00
27) Chrysene-d12	21.26	240	40197	0.40	ng	-0.01
34) Perylene-d12	23.48	264	44077	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.32	112	2154	0.10	ng	0.00
5) Phenol-d6	6.87	99	1726	0.06	ng	0.00
8) Nitrobenzene-d5	8.83	82	7055	0.33	ng	0.00
11) 2-Methylnaphthalene-d10	12.06	152	14138	0.34	ng	0.00
14) 2,4,6-Tribromophenol	15.82	330	2230	0.26	ng	0.00
15) 2-Fluorobiphenyl	12.94	172	27211	0.41	ng	0.00
25) Fluoranthene-d10	19.10	212	42994	0.35	ng	0.00
29) Terphenyl-d14	19.71	244	45425	0.46	ng	0.00
Target Compounds						
3) n-Nitrosodimethylamine	3.01	42	95427	30.320	ng	Qvalue # 69
32) Bis(2-ethylhexyl)phthalate	21.20	149	8279	0.109	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091819\
Data File : BN007719.D
Acq On : 18 Sep 2019 23:16
Operator : HP/JU
Sample : K4896-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE123D3-20190912

Quant Time: Sep 19 07:26:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

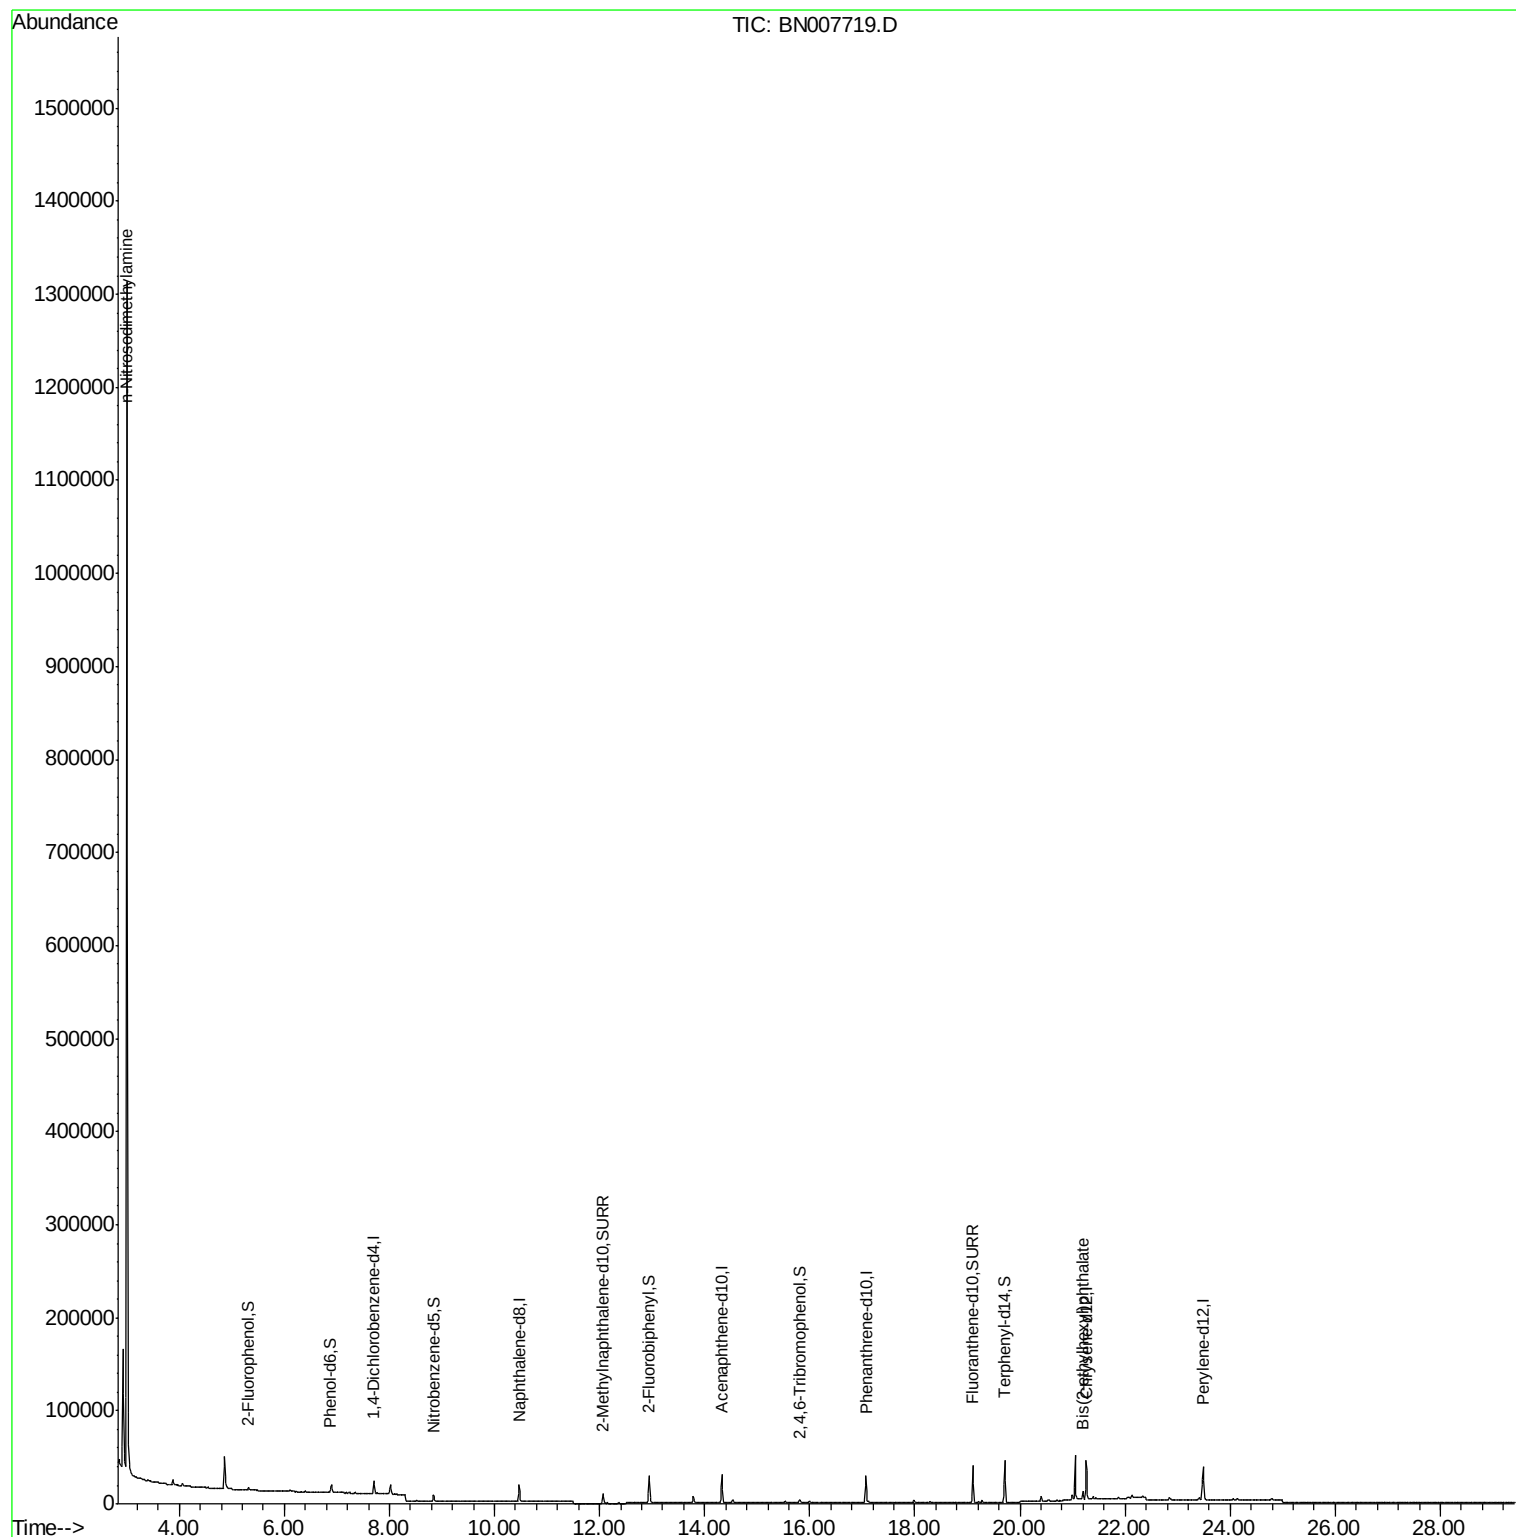




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.70 min Scan# 605
Delta R.T. -0.00 min
Lab File: BN007719.D
Acq: 18 Sep 2019 23:16

Instrument :
BNA_N
ClientSampleId :
RE123D3-20190912

Tot Ion:152 Resp: 6165
Ion Ratio Lower Upper
152 100
150 156.6 125.6 188.4
115 65.0 53.3 79.9

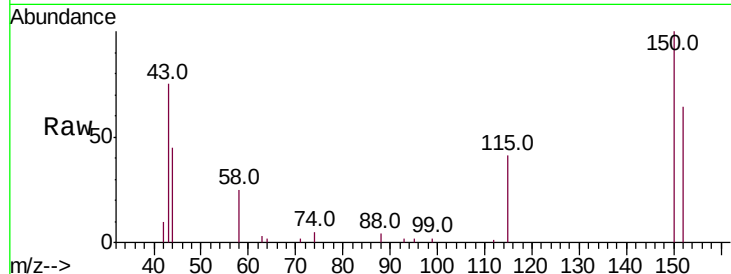


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

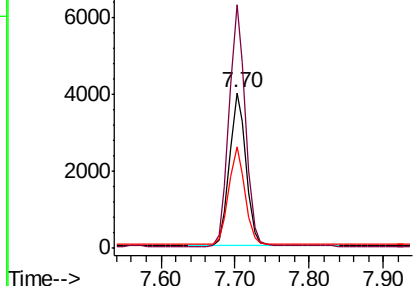



#3


n-Nitrosodimethylamine
Concen: 30.320 ng
RT: 3.01 min Scan# 22
Delta R.T. -0.00 min
Lab File: BN007719.D
Acq: 18 Sep 2019 23:16

Tgt Ion: 42 Resp: 95427
Ion Ratio Lower Upper
42 100
74 147.3 87.9 131.9#
44 26.8 29.4 44.0#

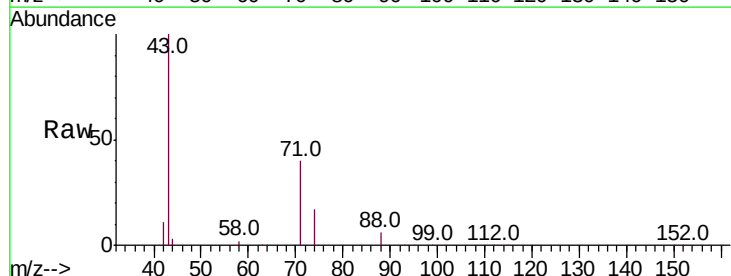

Abundance Ion 42.00 (41.70 to 42.70): BNC
Ion 74.00 (73.70 to 74.70): BNC
Ion 44.00 (43.70 to 44.70): BNC

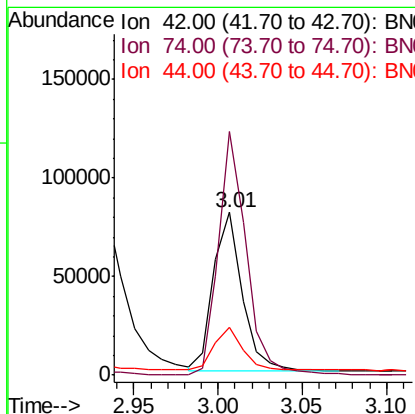

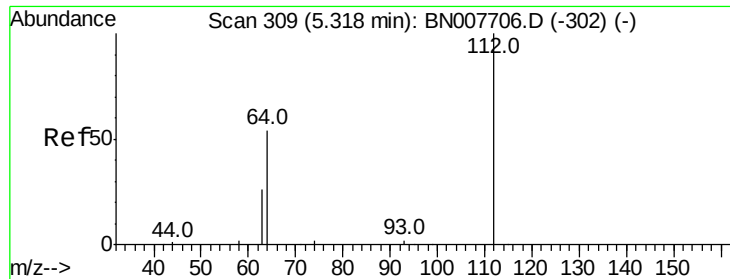

#4

2-Fluorophenol

Concen: 0.102 ng

RT: 5.32 min Scan# 309

Delta R.T. -0.00 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16

Instrument :

BNA_N

ClientSampleId :

RE123D3-20190912


Tot Ion:112 Resp: 2154

Ion Ratio Lower Upper

112 100

64 58.6 46.6 70.0




63 29.3 23.1 34.7

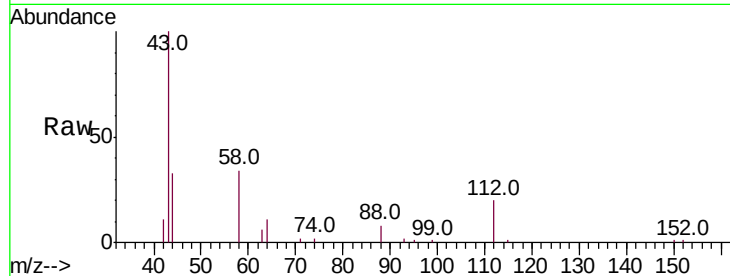

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BN0

Ion 63.00 (62.70 to 63.70): BN0

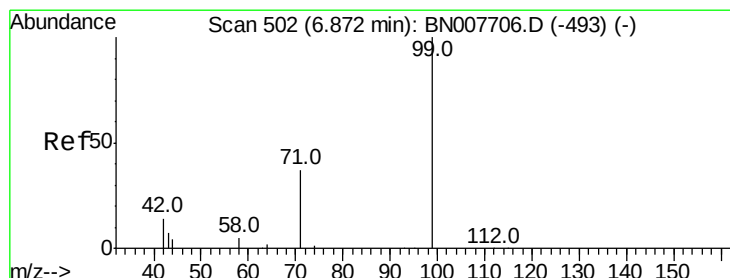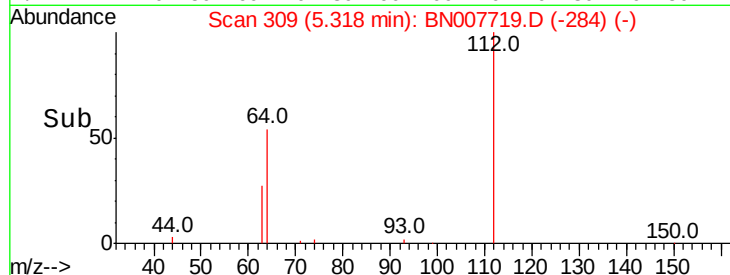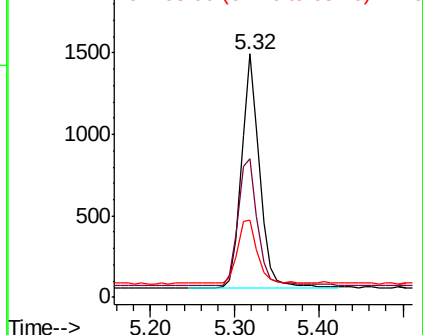

#5

Phenol-d6

Concen: 0.060 ng

RT: 6.87 min Scan# 502

Delta R.T. 0.00 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16


Tgt Ion: 99 Resp: 1726

Ion Ratio Lower Upper

99 100

42 0.0 12.8 19.2#



71 40.6 27.6 41.4

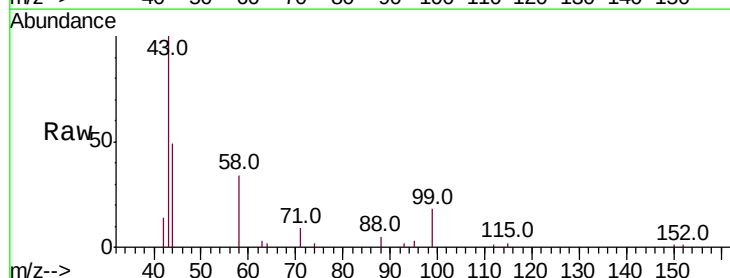


Abundance Ion 99.00 (98.70 to 99.70): BN0

Ion 42.00 (41.70 to 42.70): BN0

Ion 71.00 (70.70 to 71.70): BN0

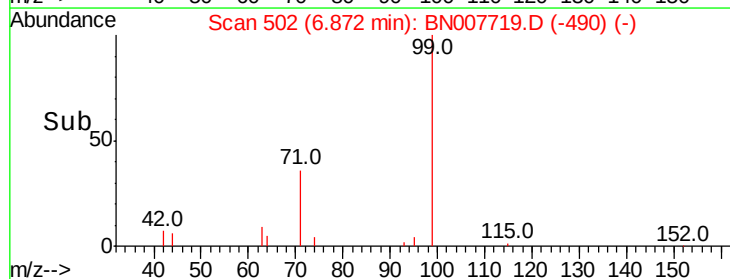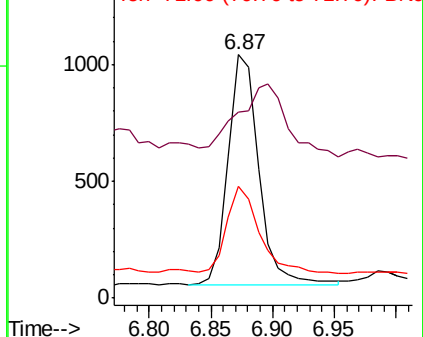

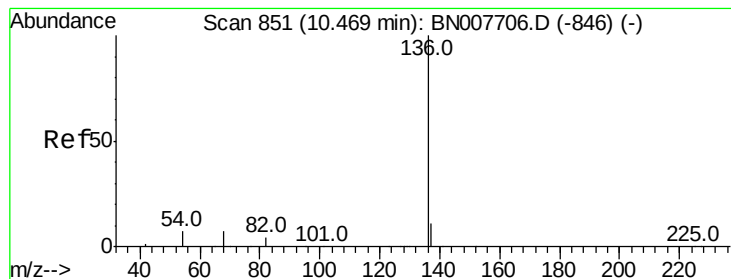

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.47 min Scan# 851

Delta R.T. -0.00 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16

Instrument :

BNA_N

ClientSampleId :

RE123D3-20190912

Tot Ion:136 Resp: 24638


Ion Ratio Lower Upper

136 100

137 11.2 9.2 13.8

54 6.8 5.8 8.8

68 7.5 6.5 9.7






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

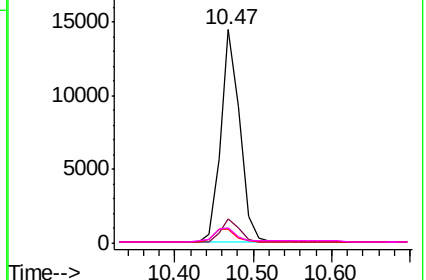

#8

Nitrobenzene-d5

Concen: 0.327 ng

RT: 8.83 min Scan# 722

Delta R.T. -0.00 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16


Tgt Ion: 82 Resp: 7055

Ion Ratio Lower Upper

82 100

128 30.9 24.5 36.7



54 44.6 35.2 52.8




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

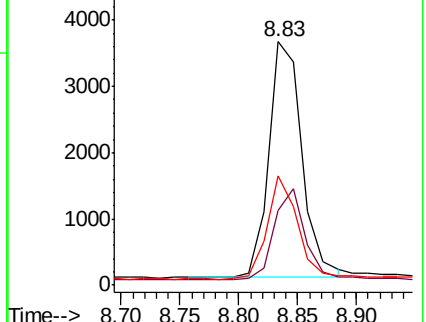

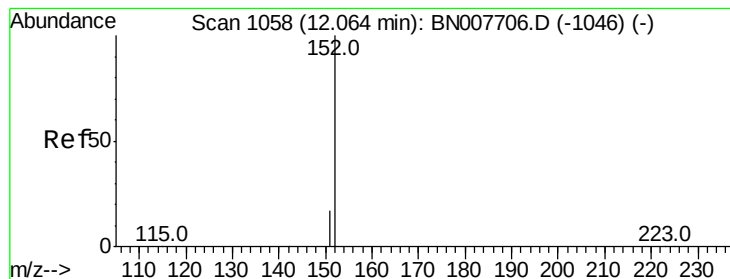

#11

2-Methylnaphthalene-d10

Concen: 0.341 ng

RT: 12.06 min Scan# 1058

Delta R.T. -0.00 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16

Instrument :

BNA_N

ClientSampleId :


RE123D3-20190912

Tot Ion:152 Resp: 14138

Ion Ratio Lower Upper




152 100

151 19.3 15.4 23.2

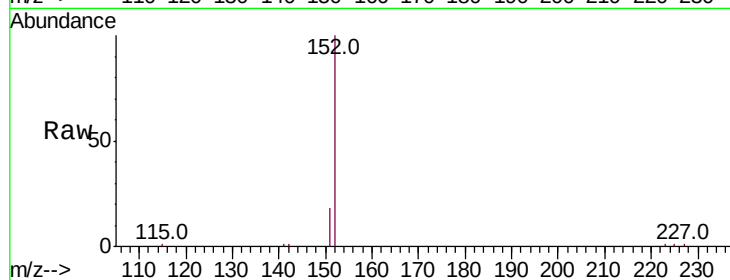

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

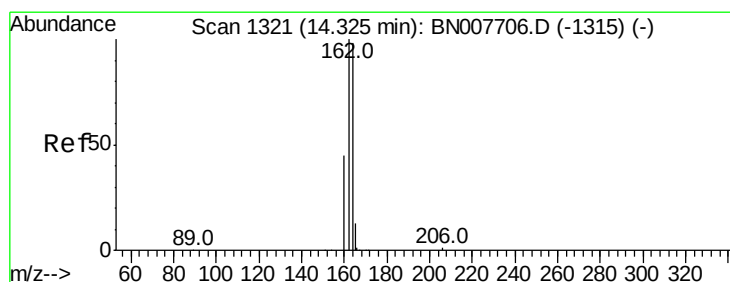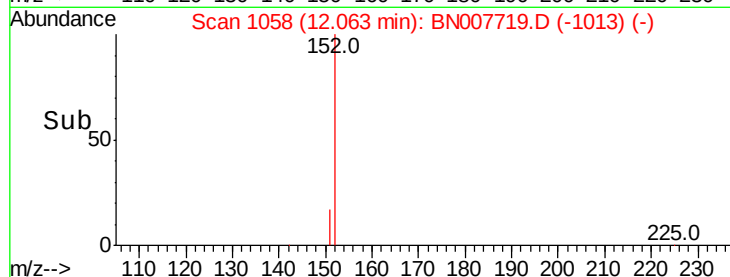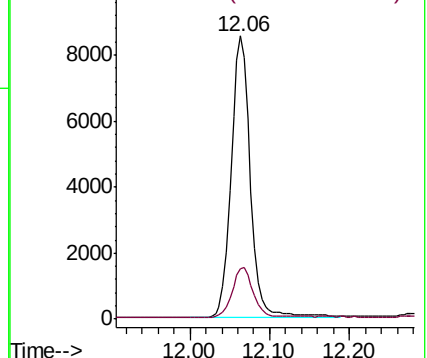

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.32 min Scan# 1321

Delta R.T. -0.00 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16


Tgt Ion:164 Resp: 16017

Ion Ratio Lower Upper

164 100

162 101.7 81.7 122.5



160 45.5 37.0 55.4

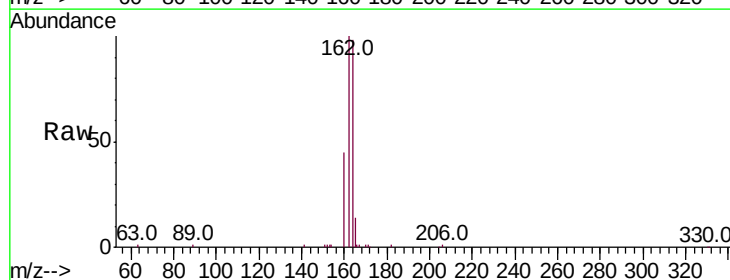


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

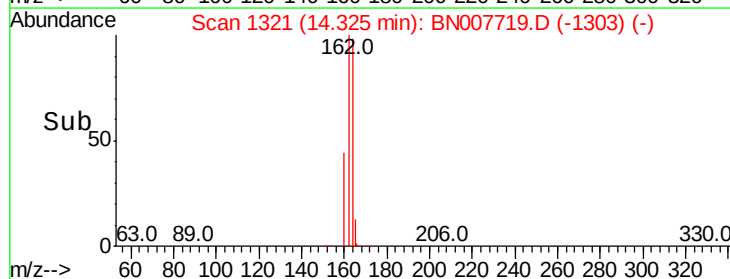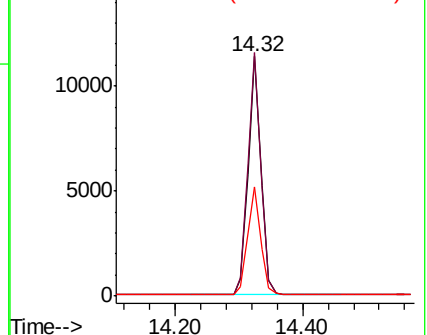







#14
 2,4,6-Tribromophenol
 Concen: 0.256 ng
 RT: 15.82 min Scan# 1455
 Delta R.T. -0.00 min
 Lab File: BN007719.D
 Acq: 18 Sep 2019 23:16

Instrument :
 BNA_N
 ClientSampleId :
 RE123D3-20190912

Tot Ion:330 Resp: 2230
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 34.1 28.7 43.1

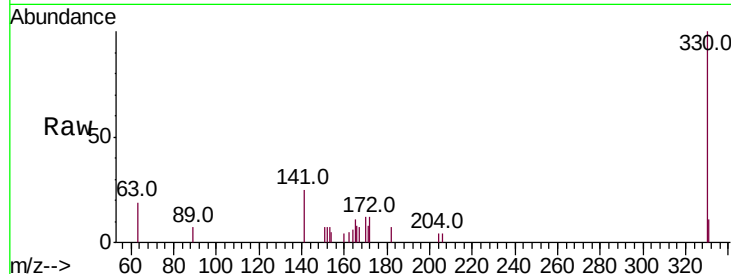


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


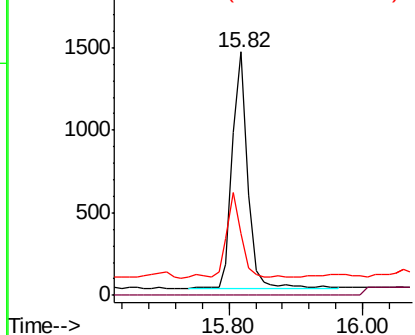



#15
 2-Fluorobiphenyl
 Concen: 0.412 ng
 RT: 12.94 min Scan# 1197
 Delta R.T. -0.00 min
 Lab File: BN007719.D
 Acq: 18 Sep 2019 23:16

Tgt Ion:172 Resp: 27211
 Ion Ratio Lower Upper
 172 100
 171 36.1 28.8 43.2
 170 24.0 19.5 29.3

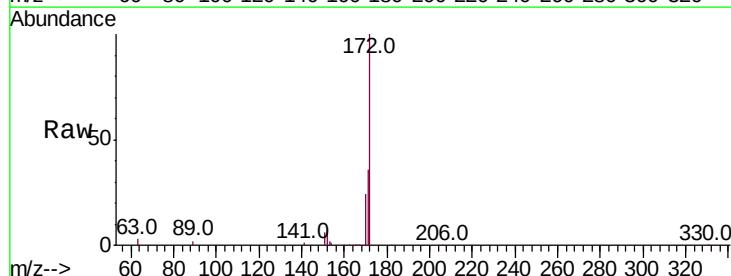

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

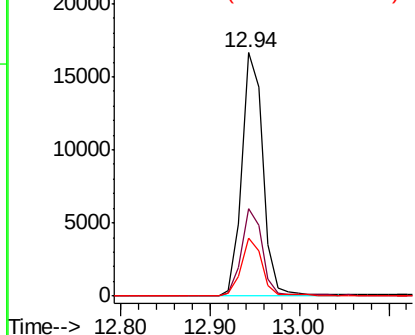

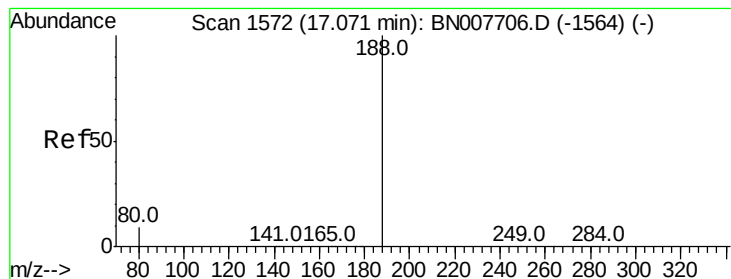

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.07 min Scan# 1572

Delta R.T. -0.00 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16

Instrument :

BNA_N

ClientSampleId :

RE123D3-20190912


Tot Ion:188 Resp: 36481

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 9.1 7.4 11.2



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

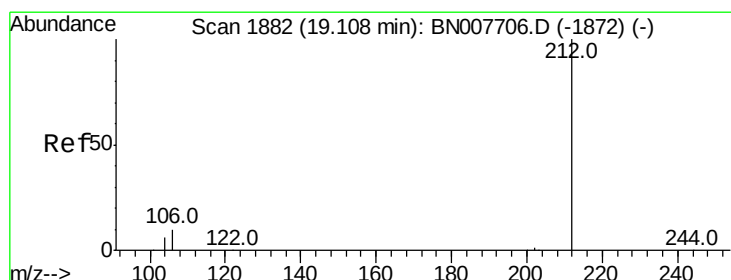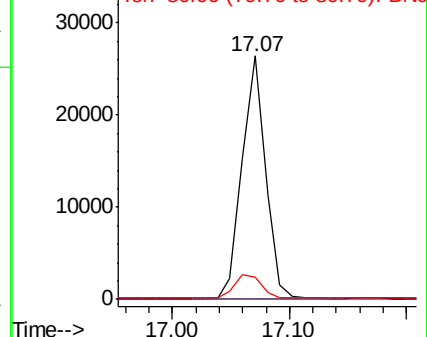

#25

Fluoranthene-d10

Concen: 0.350 ng

RT: 19.10 min Scan# 1881

Delta R.T. -0.01 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16


Tgt Ion:212 Resp: 42994

Ion Ratio Lower Upper

212 100

106 11.9 9.4 14.0



104 6.6 5.3 7.9




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

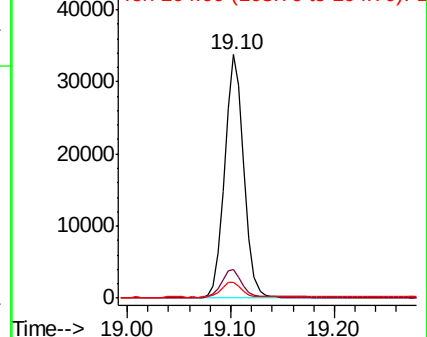



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.26 min Scan# 2181

Delta R.T. -0.01 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16

Instrument :

BNA_N

ClientSampleId :

RE123D3-20190912


Tot Ion:240 Resp: 40197

Ion Ratio Lower Upper

240 100

120 11.5 5.4 8.2#




236 27.0 21.0 31.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

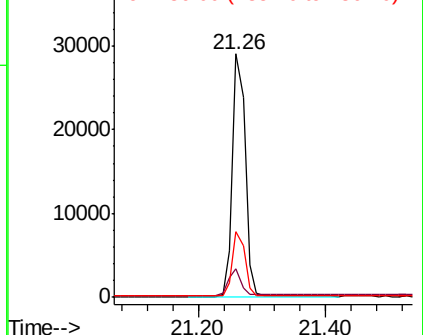

#29

Terphenyl-d14

Concen: 0.460 ng

RT: 19.71 min Scan# 2003

Delta R.T. -0.01 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16


Tgt Ion:244 Resp: 45425

Ion Ratio Lower Upper

244 100

212 7.3 5.9 8.9



122 10.1 7.4 11.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

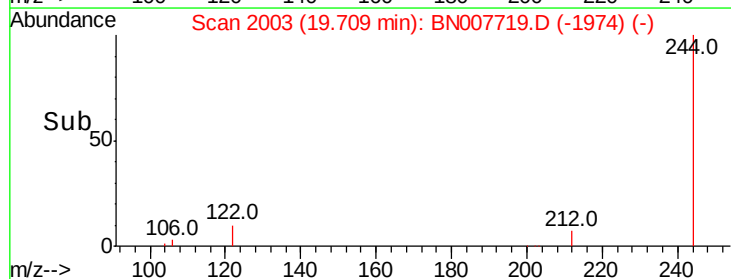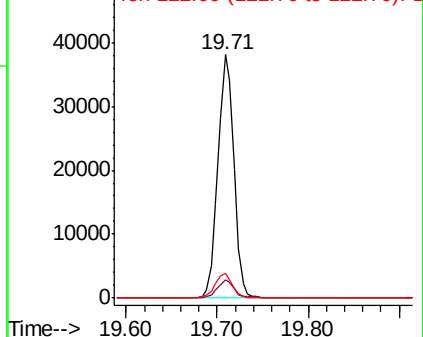



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.109 ng

RT: 21.20 min Scan# 2175

Delta R.T. -0.01 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16

Instrument :

BNA_N

ClientSampleId :

RE123D3-20190912


Tot Ion:149 Resp: 8279

Ion Ratio Lower Upper




149 100

167 27.9 23.7 35.5

279 4.8 4.2 6.2



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

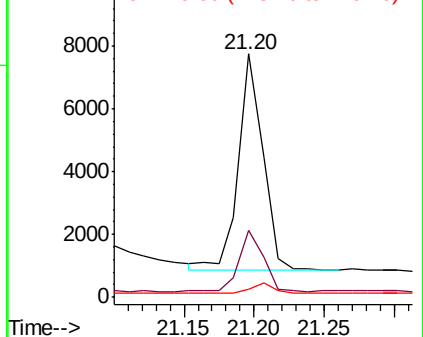

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.48 min Scan# 2603

Delta R.T. -0.01 min

Lab File: BN007719.D

Acq: 18 Sep 2019 23:16


Tgt Ion:264 Resp: 44077

Ion Ratio Lower Upper

264 100

260 24.2 19.3 28.9

265 31.7 26.9 40.3



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

