

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091819\
 Data File : BN007724.D
 Acq On : 19 Sep 2019 02:15
 Operator : HP/JU
 Sample : K4896-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 19 07:26:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 18:24:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	6220	0.40	ng	0.00
7) Naphthalene-d8	10.47	136	24295	0.40	ng	0.00
13) Acenaphthene-d10	14.32	164	15001	0.40	ng	0.00
19) Phenanthrene-d10	17.07	188	34473	0.40	ng	0.00
27) Chrysene-d12	21.26	240	38761	0.40	ng	0.00
34) Perylene-d12	23.48	264	42852	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.32	112	2555	0.12	ng	0.00
5) Phenol-d6	6.87	99	1970	0.07	ng	0.00
8) Nitrobenzene-d5	8.83	82	7164	0.34	ng	0.00
11) 2-Methylnaphthalene-d10	12.06	152	14513	0.35	ng	0.00
14) 2,4,6-Tribromophenol	15.81	330	2116	0.26	ng	0.00
15) 2-Fluorobiphenyl	12.95	172	25473	0.41	ng	0.00
25) Fluoranthene-d10	19.10	212	43064	0.37	ng	0.00
29) Terphenyl-d14	19.71	244	41555	0.44	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.30	88	2442	0.352	ng	# 70
3) n-Nitrosodimethylamine	3.01	42	105783	33.314	ng	# 70
6) bis(2-Chloroethyl)ether	7.15	93	1356	0.077	ng	# 85
32) Bis(2-ethylhexyl)phthalate	21.20	149	4326	0.059	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091819\
Data File : BN007724.D
Acq On : 19 Sep 2019 02:15
Operator : HP/JU
Sample : K4896-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 19 07:26:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

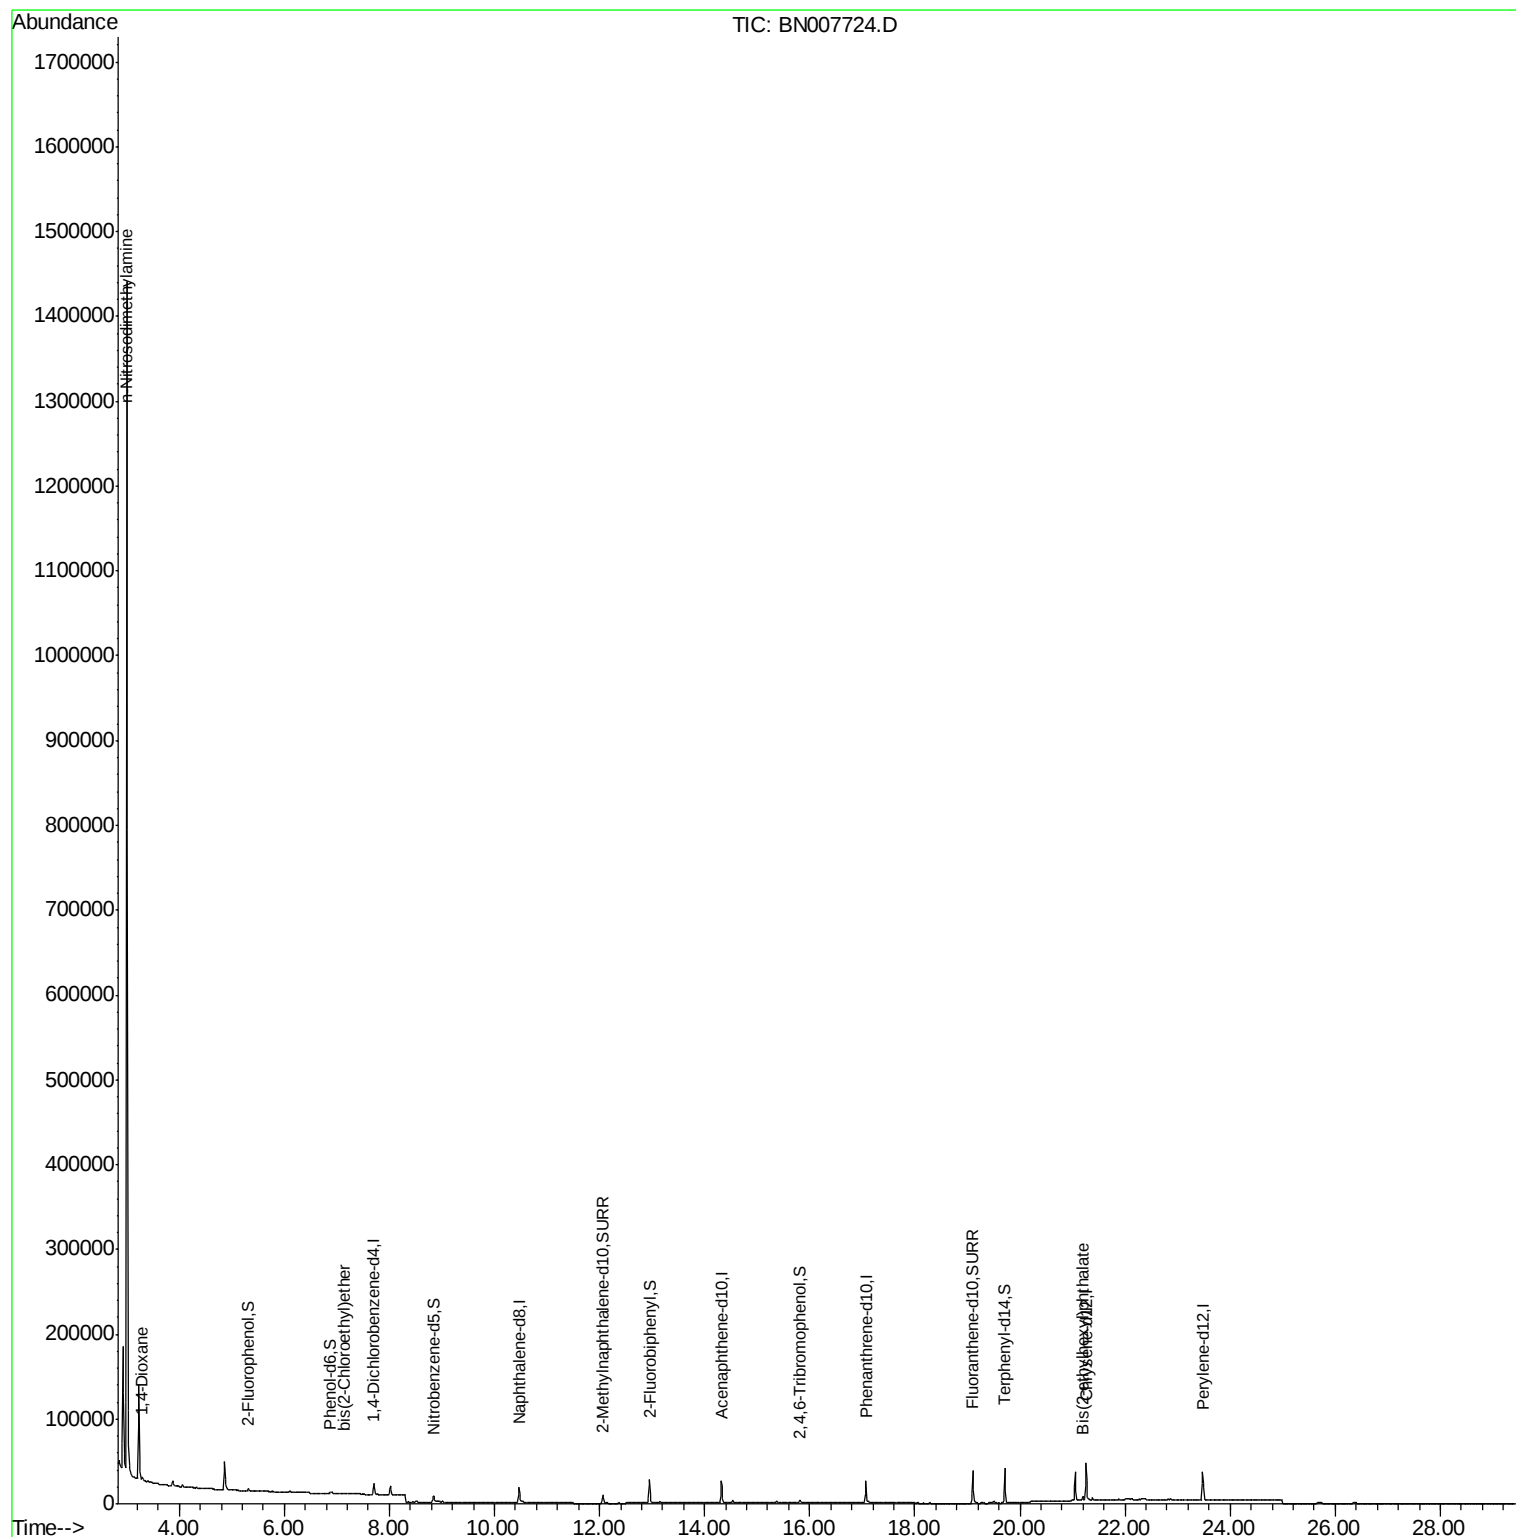




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.70 min Scan# 605
Delta R.T. 0.00 min
Lab File: BN007724.D
Acq: 19 Sep 2019 02:15

Instrument :
BNA_N
ClientSampleId :

Tot Ion:152 Resp: 6220
Ion Ratio Lower Upper
152 100
150 155.7 125.6 188.4
115 64.7 53.3 79.9

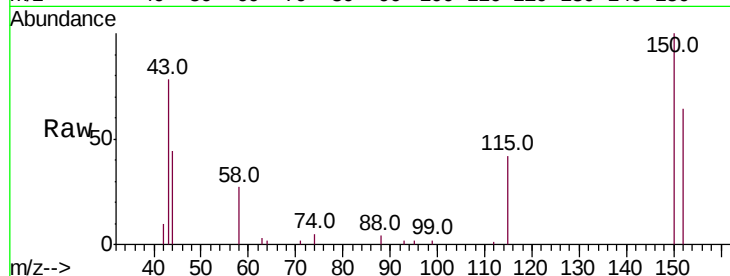


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

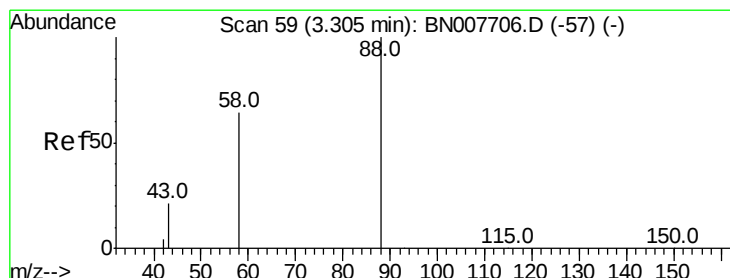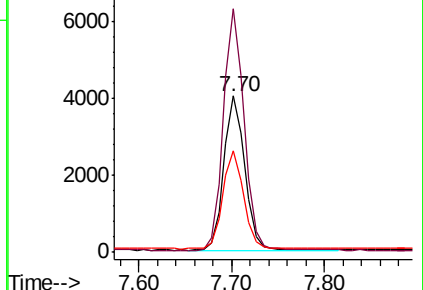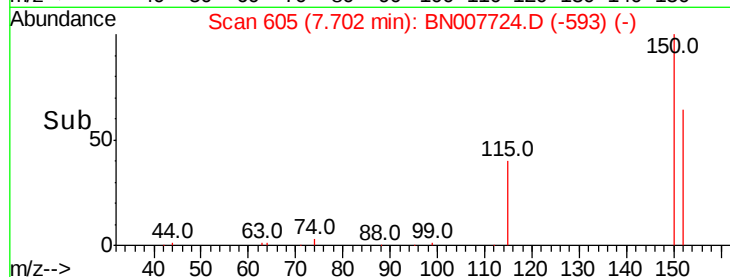



#2

1,4-Dioxane
Concen: 0.352 ng
RT: 3.30 min Scan# 59
Delta R.T. 0.00 min
Lab File: BN007724.D
Acq: 19 Sep 2019 02:15

Tgt Ion: 88 Resp: 2442
Ion Ratio Lower Upper
88 100
58 74.9 44.6 66.8#
43 0.0 14.4 21.6#

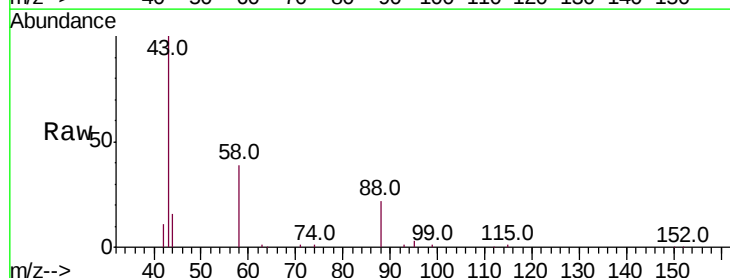

Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC



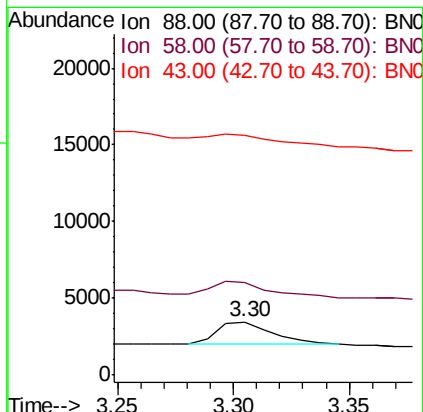
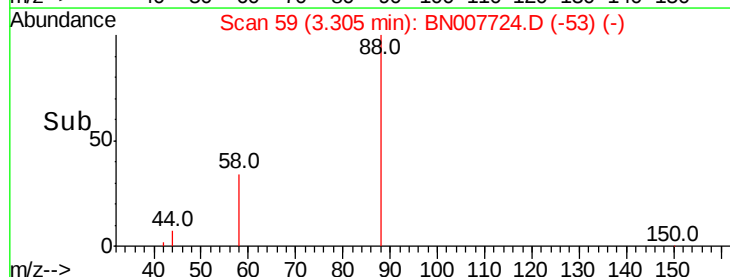




#3
 n-Nitrosodimethylamine
 Concen: 33.314 ng
 RT: 3.01 min Scan# 22
 Delta R.T. 0.00 min
 Lab File: BN007724.D
 Acq: 19 Sep 2019 02:15




Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 42 Resp: 105783
 Ion Ratio Lower Upper
 42 100
 74 146.7 87.9 131.9#
 44 26.5 29.4 44.0#

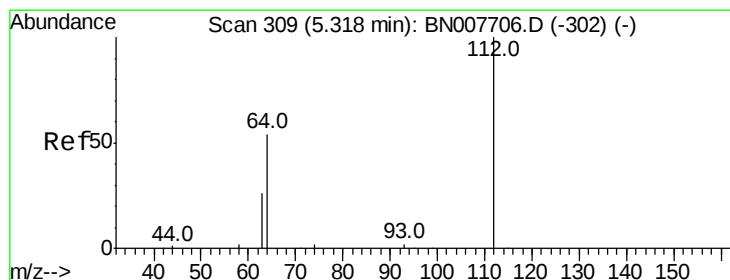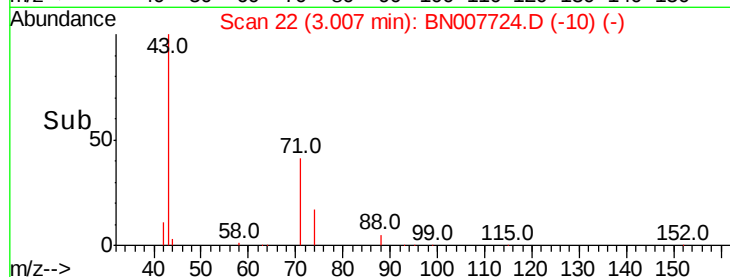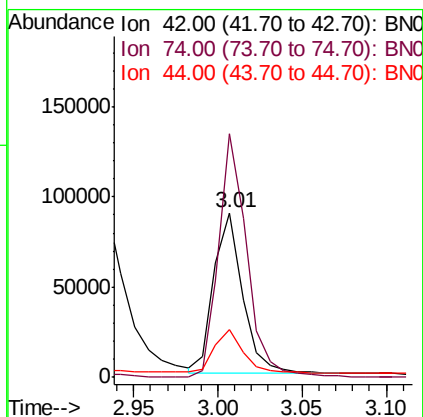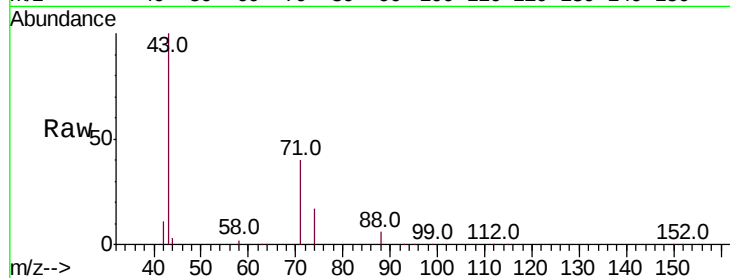

#4
 2-Fluorophenol
 Concen: 0.119 ng
 RT: 5.32 min Scan# 309
 Delta R.T. 0.00 min
 Lab File: BN007724.D
 Acq: 19 Sep 2019 02:15

Tgt Ion: 112 Resp: 2555
 Ion Ratio Lower Upper
 112 100
 64 59.8 46.6 70.0
 63 30.2 23.1 34.7

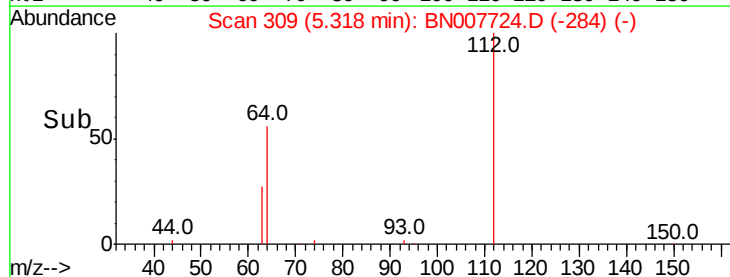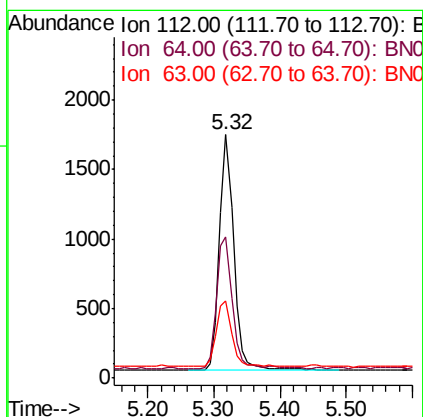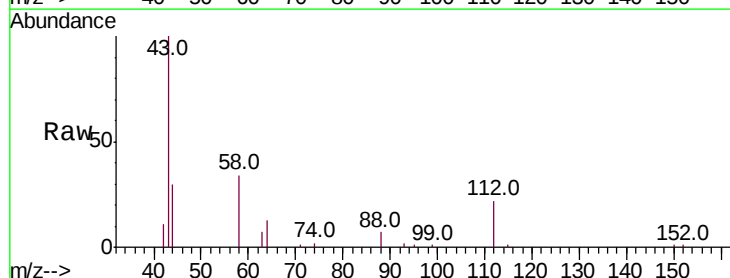



#5

Phenol-d6

Concen: 0.069 ng

RT: 6.87 min Scan# 502

Delta R.T. 0.00 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15

Instrument :

BNA_N

ClientSampled :


Tot Ion: 99 Resp: 1970

Ion Ratio Lower Upper

99 100

42 17.0 12.8 19.2




71 39.3 27.6 41.4

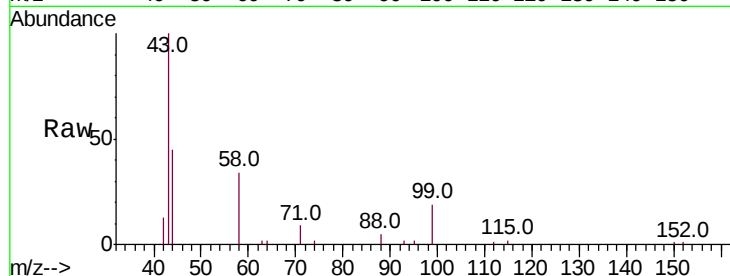

Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

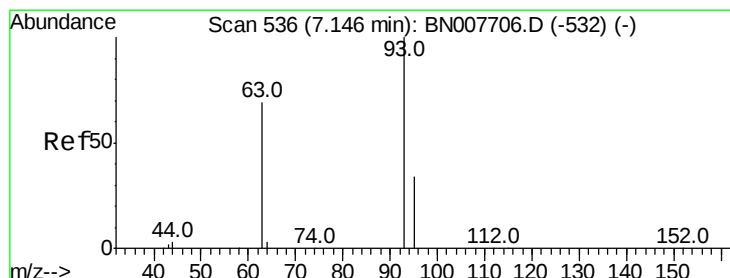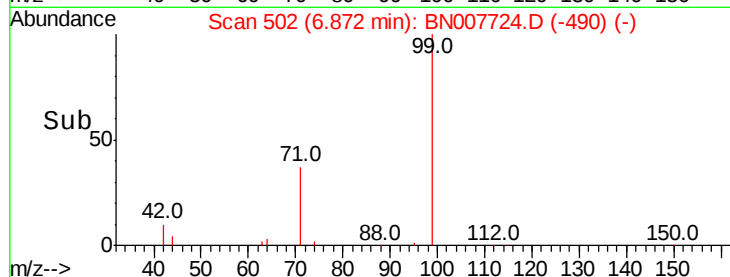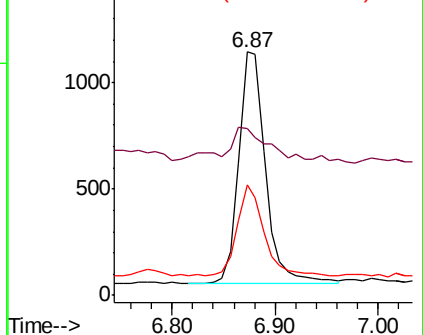

#6

bis(2-Chloroethyl)ether

Concen: 0.077 ng

RT: 7.15 min Scan# 536

Delta R.T. 0.00 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15


Tgt Ion: 93 Resp: 1356

Ion Ratio Lower Upper

93 100

63 57.8 59.3 88.9#



95 34.5 31.4 47.0

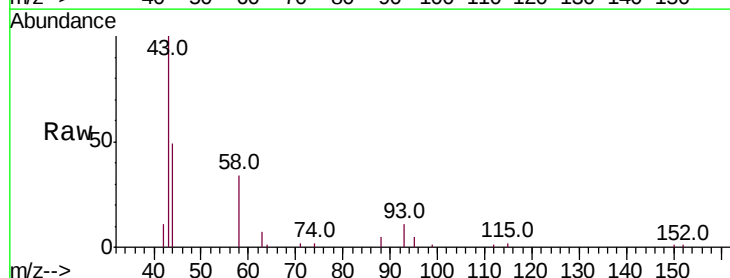


Abundance Ion 93.00 (92.70 to 93.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

Ion 95.00 (94.70 to 95.70): BNC

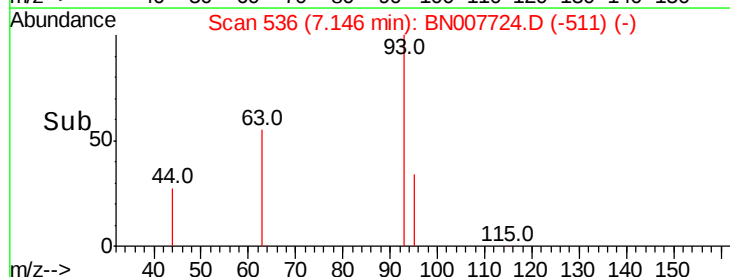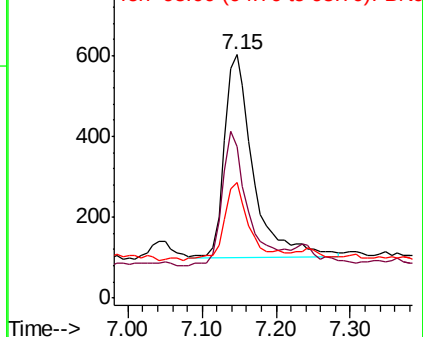



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.47 min Scan# 851

Delta R.T. 0.00 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15

Instrument :

BNA_N

ClientSampleId :

Tot Ion:136 Resp: 24295


Ion Ratio Lower Upper

136 100

137 11.2 9.2 13.8

54 6.9 5.8 8.8

68 7.3 6.5 9.7



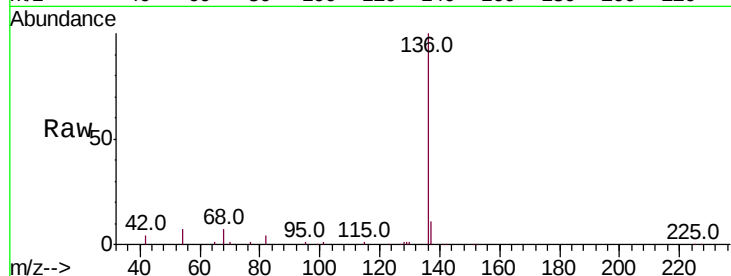


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

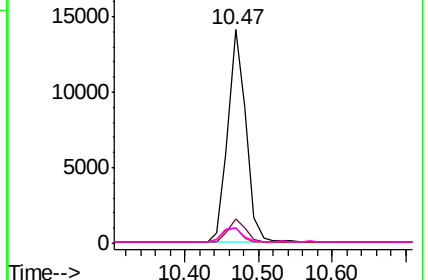

#8

Nitrobenzene-d5

Concen: 0.337 ng

RT: 8.83 min Scan# 722

Delta R.T. 0.00 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15


Tgt Ion: 82 Resp: 7164

Ion Ratio Lower Upper

82 100

128 31.1 24.5 36.7



54 44.6 35.2 52.8




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

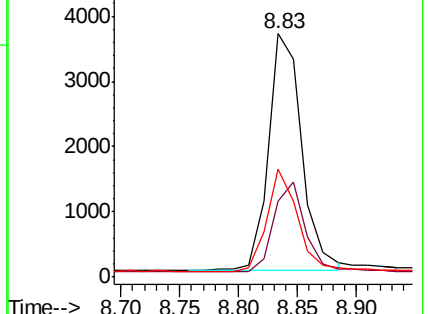

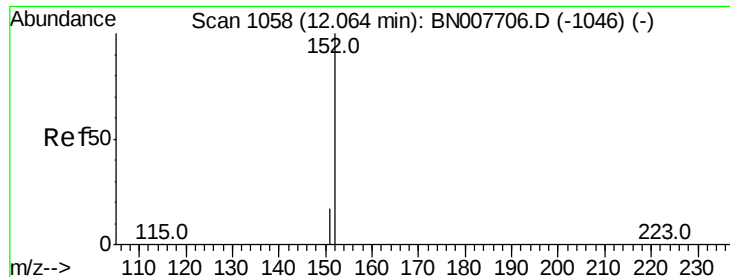

#11

2-Methylnaphthalene-d10

Concen: 0.355 ng

RT: 12.06 min Scan# 1058

Delta R.T. 0.00 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15

Instrument :

BNA_N


ClientSampleId :

Tot Ion:152 Resp: 14513

Ion Ratio Lower Upper




152 100

151 19.0 15.4 23.2

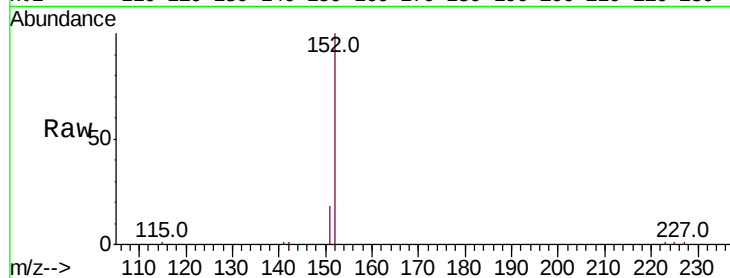

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

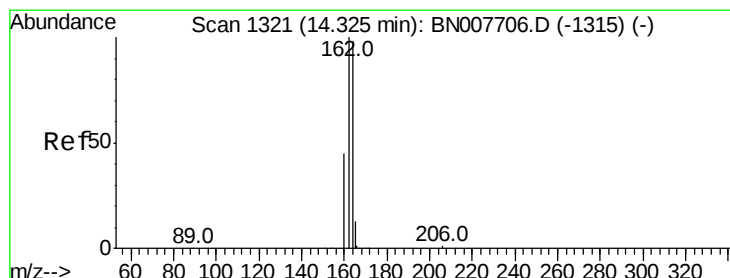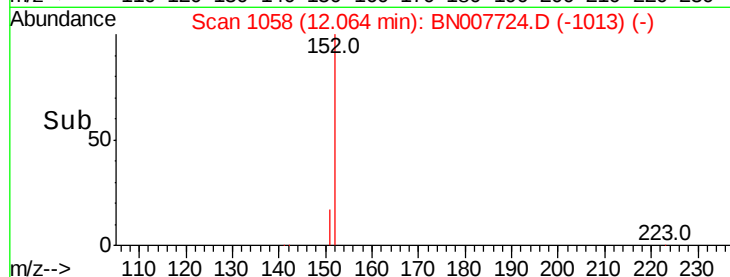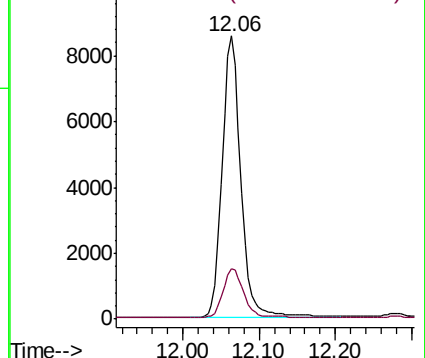

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.32 min Scan# 1320

Delta R.T. -0.00 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15


Tgt Ion:164 Resp: 15001

Ion Ratio Lower Upper

164 100

162 103.4 81.7 122.5



160 47.4 37.0 55.4

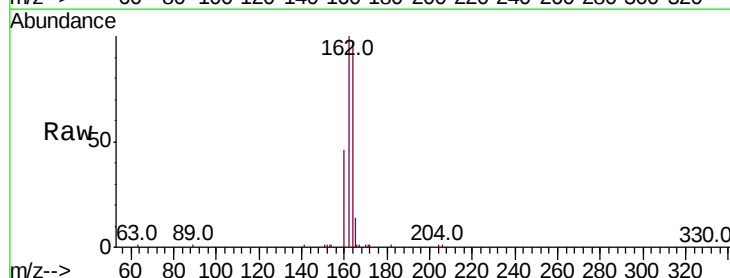

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

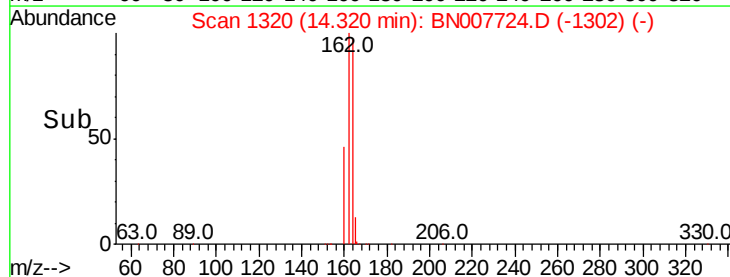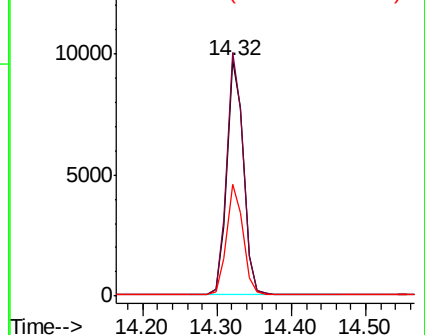







#14
 2,4,6-Tribromophenol
 Concen: 0.259 ng
 RT: 15.81 min Scan# 1454
 Delta R.T. -0.00 min
 Lab File: BN007724.D
 Acq: 19 Sep 2019 02:15

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:330 Resp: 2116
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 34.1 28.7 43.1

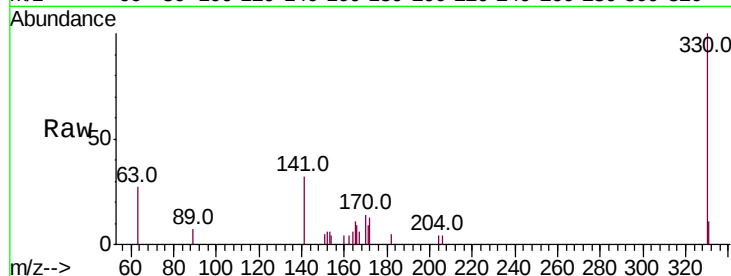


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


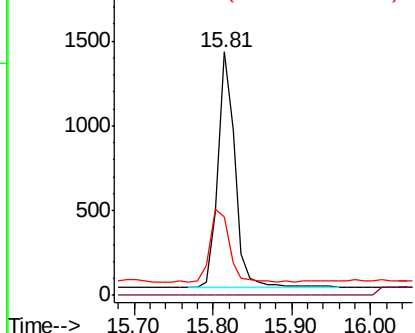



#15
 2-Fluorobiphenyl
 Concen: 0.412 ng
 RT: 12.95 min Scan# 1197
 Delta R.T. 0.01 min
 Lab File: BN007724.D
 Acq: 19 Sep 2019 02:15

Tgt Ion:172 Resp: 25473
 Ion Ratio Lower Upper
 172 100
 171 34.3 28.8 43.2
 170 22.1 19.5 29.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

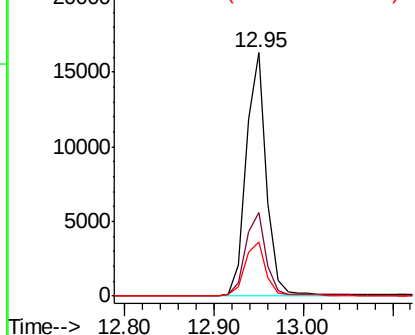

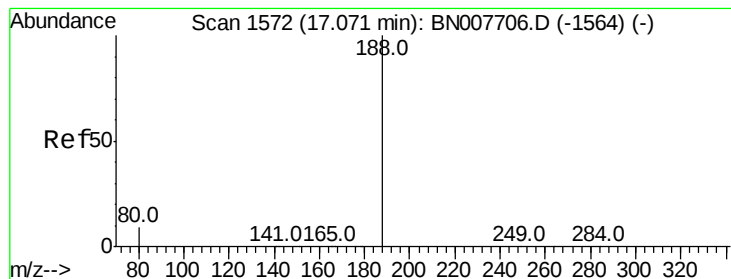

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.07 min Scan# 1571

Delta R.T. -0.00 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15

Instrument :

BNA_N

ClientSampleId :


Tot Ion:188 Resp: 34473

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 11.5 7.4 11.2#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

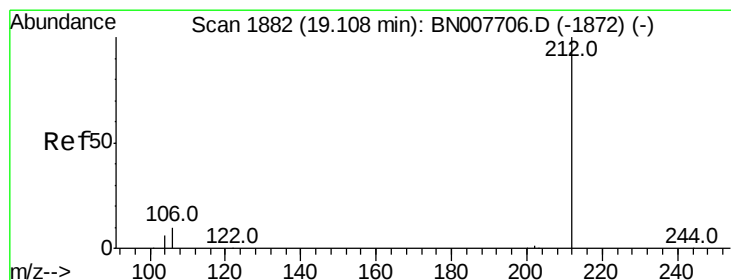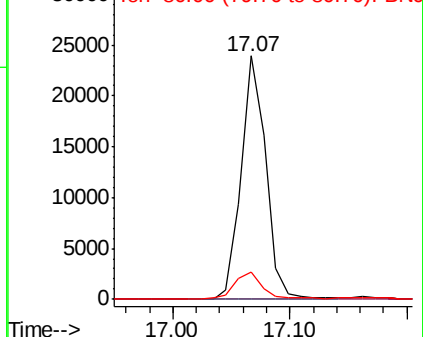

#25

Fluoranthene-d10

Concen: 0.371 ng

RT: 19.10 min Scan# 1880

Delta R.T. -0.00 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15


Tgt Ion:212 Resp: 43064

Ion Ratio Lower Upper

212 100

106 11.8 9.4 14.0



104 6.6 5.3 7.9




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

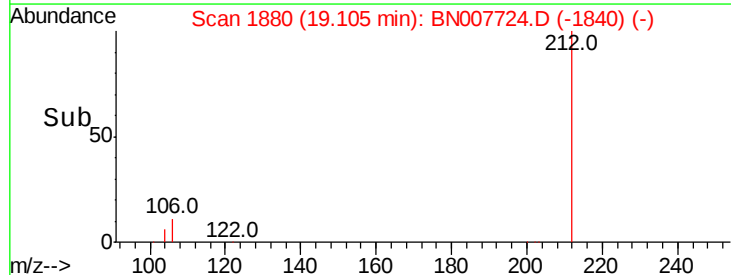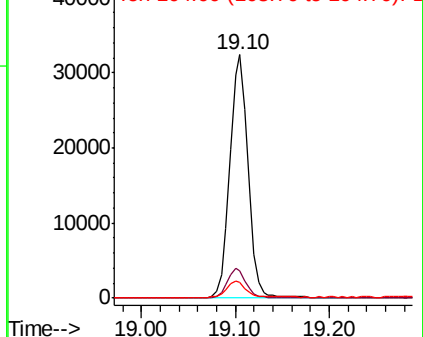



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.26 min Scan# 2180

Delta R.T. -0.01 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15

Instrument :

BNA_N

ClientSampleId :


Tot Ion:240 Resp: 38761

Ion Ratio Lower Upper

240 100

120 9.3 5.4 8.2#




236 26.6 21.0 31.4

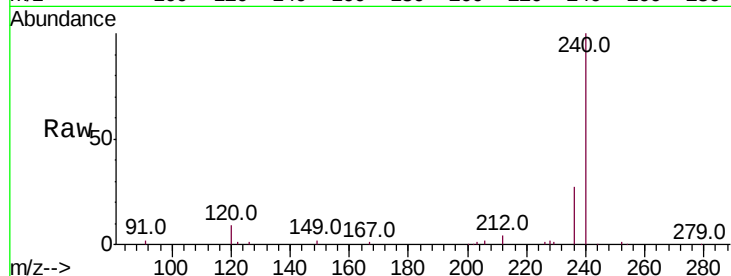

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

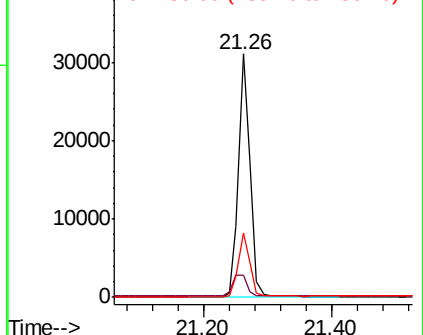

#29

Terphenyl-d14

Concen: 0.436 ng

RT: 19.71 min Scan# 2002

Delta R.T. -0.00 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15


Tgt Ion:244 Resp: 41555

Ion Ratio Lower Upper

244 100

212 7.2 5.9 8.9



122 9.1 7.4 11.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

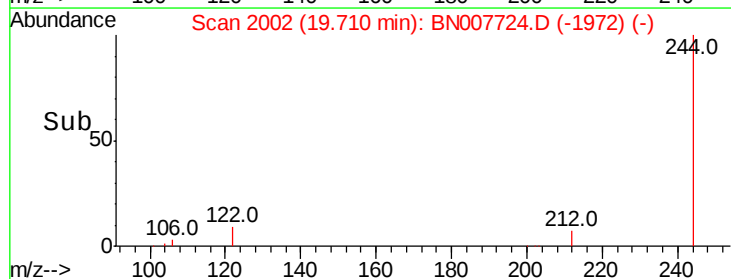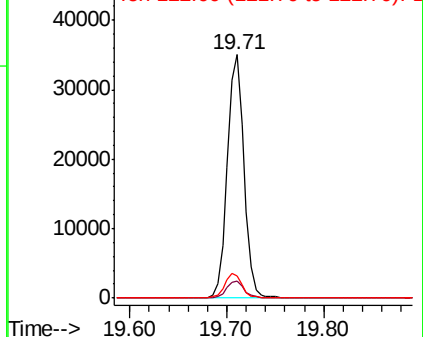



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.059 ng

RT: 21.20 min Scan# 2174

Delta R.T. -0.01 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15

Instrument :

BNA_N

ClientSampleId :


Tot Ion:149 Resp: 4326

Ion Ratio Lower Upper

149 100

167 26.9 23.7 35.5




279 5.1 4.2 6.2



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

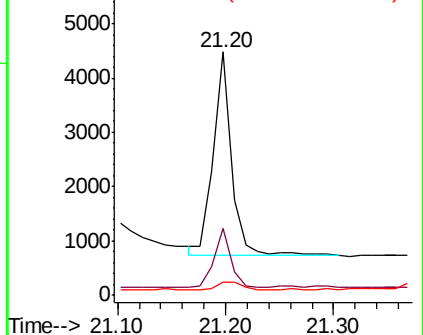

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.48 min Scan# 2601

Delta R.T. -0.01 min

Lab File: BN007724.D

Acq: 19 Sep 2019 02:15


Tgt Ion:264 Resp: 42852

Ion Ratio Lower Upper

264 100

260 24.1 19.3 28.9

265 31.9 26.9 40.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

