


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091819\
 Data File : BN007703.D
 Acq On : 18 Sep 2019 13:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 18 18:24:40 2019

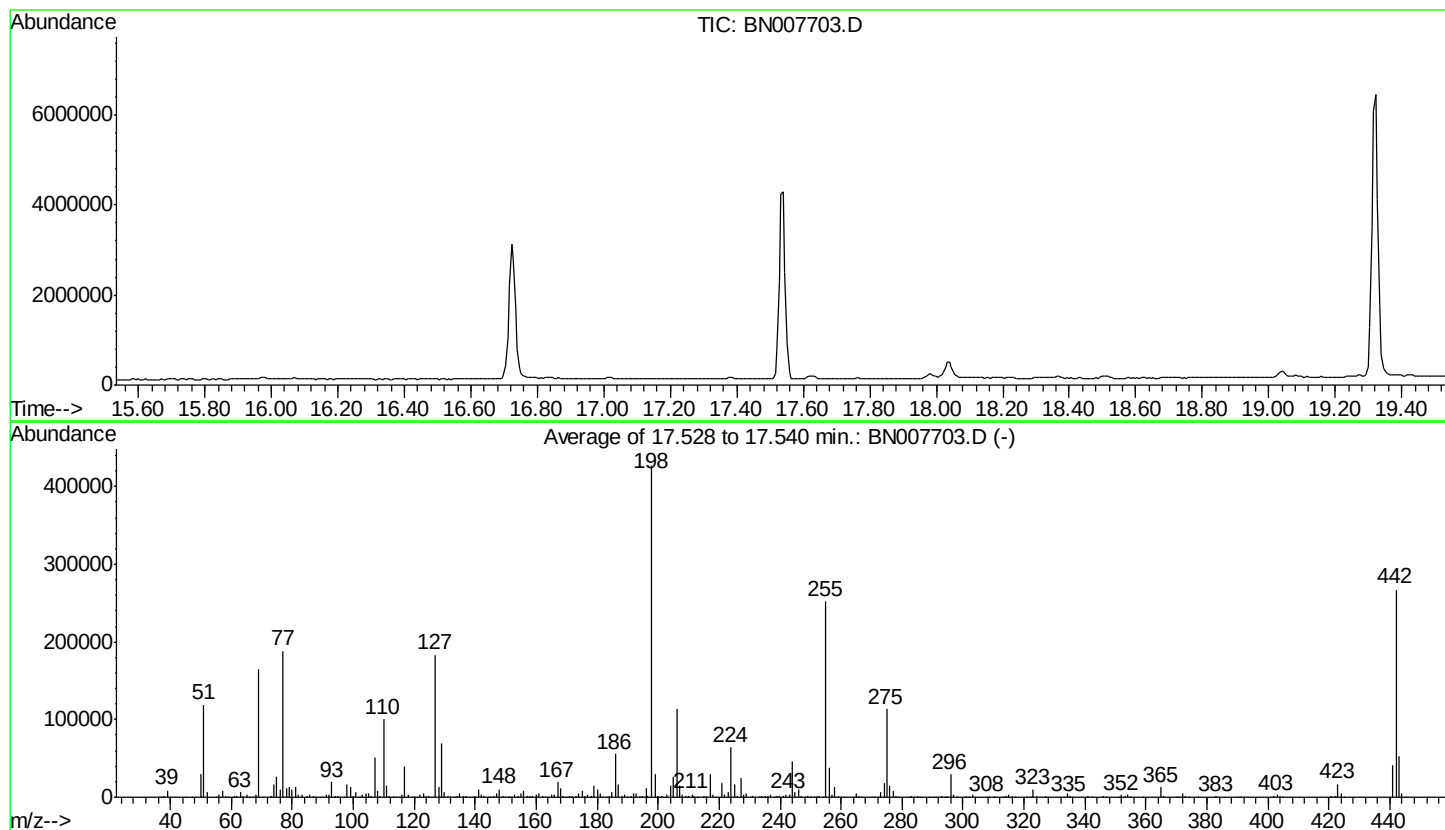

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	118821	PASS
68	69	0.00	2	1.9	3197	PASS
69	198	0.00	100	38.7	165270	PASS
70	69	0.00	2	0.5	752	PASS
127	198	10	80	42.9	182949	PASS
197	198	0.00	2	0.3	1081	PASS
198	198	100	100	100.0	426944	PASS
199	198	5	9	6.9	29514	PASS
275	198	10	60	26.6	113418	PASS
365	198	1	100	3.0	12619	PASS
441	198	0.01	100	9.6	40880	PASS
442	198	50	100	62.7	267528	PASS
443	442	15	24	19.6	52314	PASS