


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091819\
 Data File : BN007712.D
 Acq On : 18 Sep 2019 19:05
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 18 18:24:40 2019

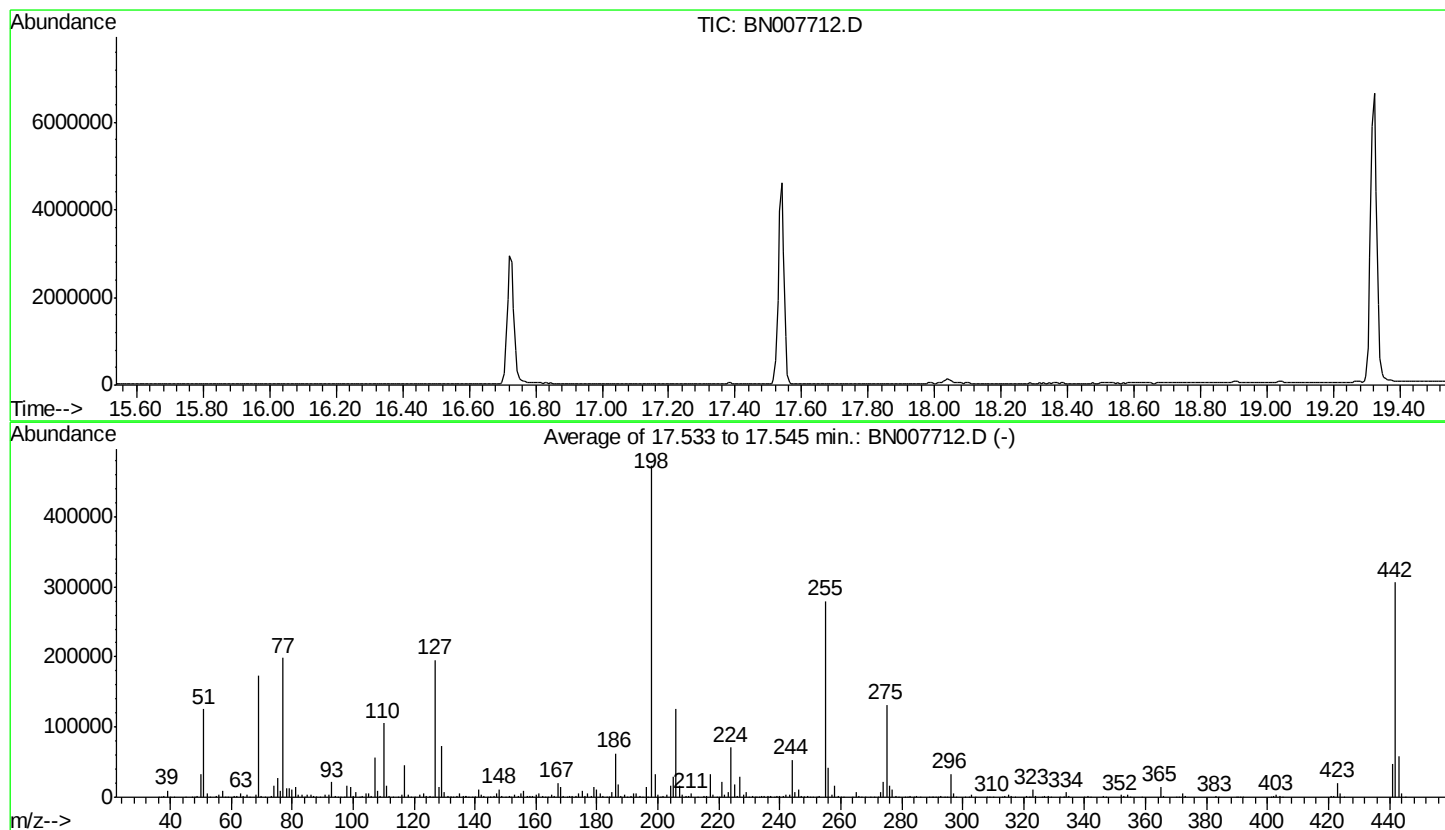

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	125065	PASS
68	69	0.00	2	2.0	3413	PASS
69	198	0.00	100	36.7	173549	PASS
70	69	0.00	2	0.6	980	PASS
127	198	10	80	41.4	195861	PASS
197	198	0.00	2	0.1	639	PASS
198	198	100	100	100.0	472704	PASS
199	198	5	9	6.8	32341	PASS
275	198	10	60	27.9	131880	PASS
365	198	1	100	3.1	14771	PASS
441	198	0.01	100	10.2	48362	PASS
442	198	50	100	64.7	305962	PASS
443	442	15	24	19.3	58909	PASS