


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN091819\  
Data File : BN007731.D  
Acq On : 19 Sep 2019 07:01  
Operator : HP/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN091819.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Sep 18 18:24:40 2019

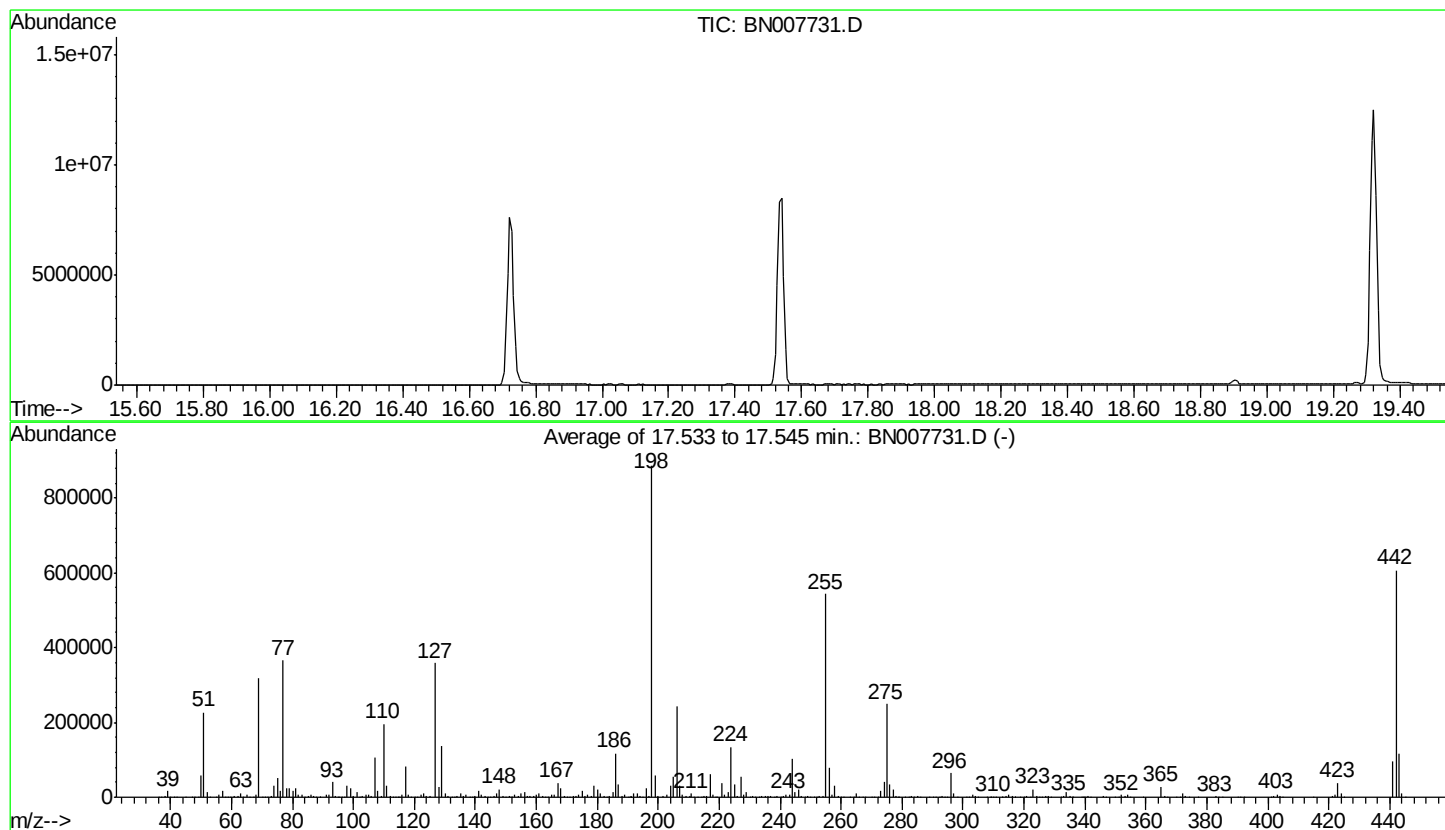

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 25.6      | 227088  | PASS             |
| 68          | 69           | 0.00         | 2            | 1.9       | 6162    | PASS             |
| 69          | 198          | 0.00         | 100          | 35.9      | 318357  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 1417    | PASS             |
| 127         | 198          | 10           | 80           | 40.4      | 358421  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 3716    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 886720  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 58501   | PASS             |
| 275         | 198          | 10           | 60           | 28.0      | 248704  | PASS             |
| 365         | 198          | 1            | 100          | 3.2       | 28170   | PASS             |
| 441         | 198          | 0.01         | 100          | 10.9      | 96376   | PASS             |
| 442         | 198          | 50           | 100          | 68.4      | 606698  | PASS             |
| 443         | 442          | 15           | 24           | 19.4      | 117408  | PASS             |