


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091823\
Data File : BN027726.D
Acq On : 18 Sep 2023 09:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 18 14:40:21 2023

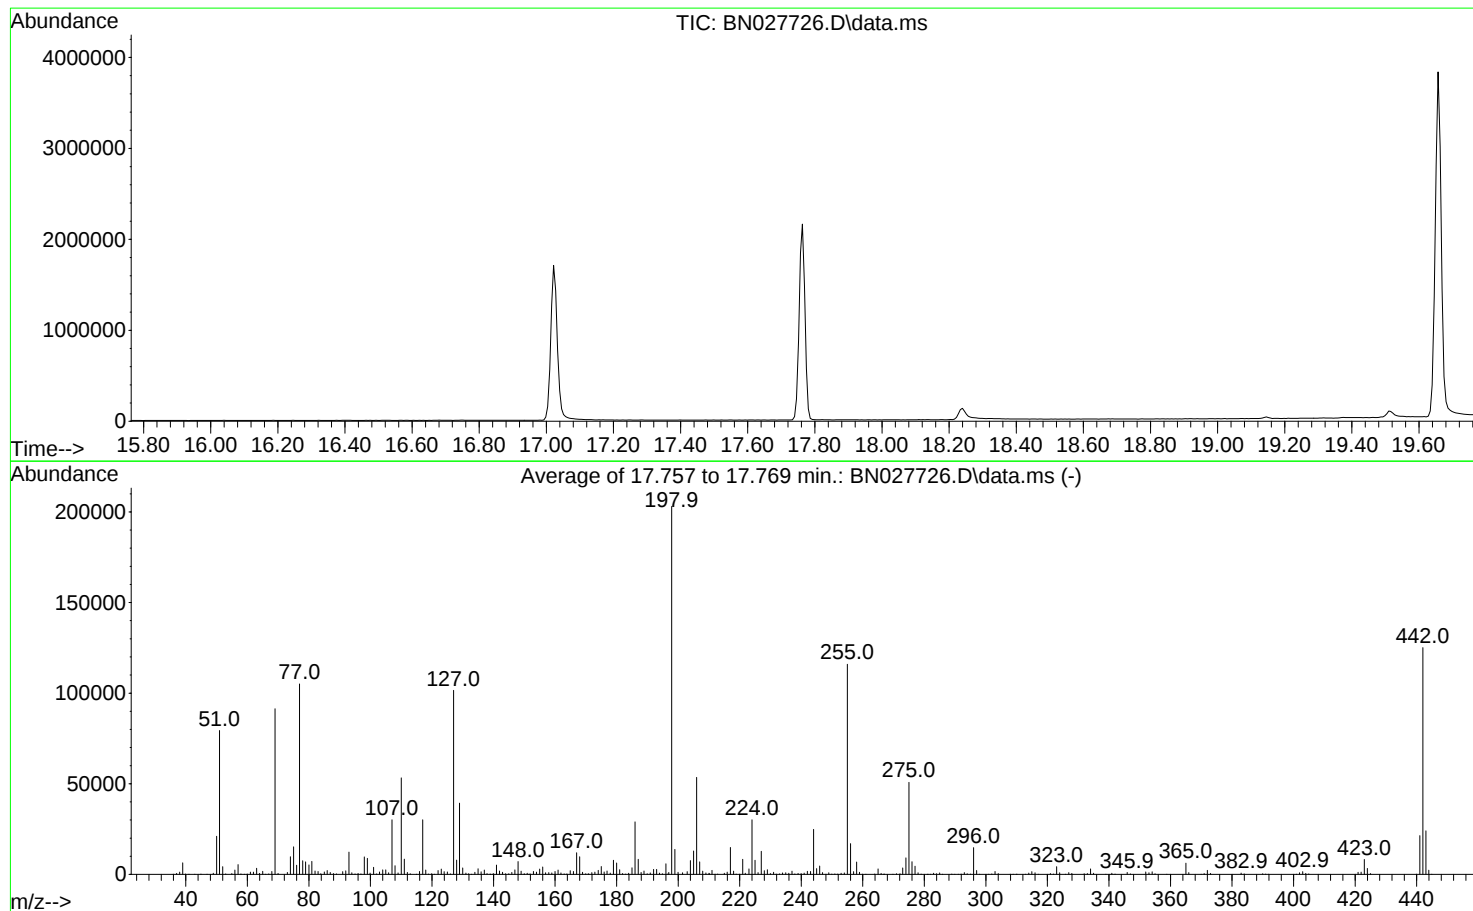




AutoFind: Scans 2528, 2529, 2530; Background Corrected with Scan 2521

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	79383	PASS
68	69	0.00	2	1.8	1603	PASS
69	198	0.00	100	45.0	91397	PASS
70	69	0.00	2	0.6	504	PASS
127	198	10	80	50.0	101523	PASS
197	198	0.00	2	0.5	1042	PASS
198	198	100	100	100.0	203008	PASS
199	198	5	9	6.8	13742	PASS
275	198	10	60	25.0	50795	PASS
365	198	1	100	3.1	6205	PASS
441	198	0.01	100	10.5	21379	PASS
442	442	50	100	100.0	125104	PASS
443	442	15	24	19.2	24053	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091823\
Data File : BN027726.D
Acq On : 18 Sep 2023 09:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 19 04:23:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:23:17 2023
Response via : Initial Calibration

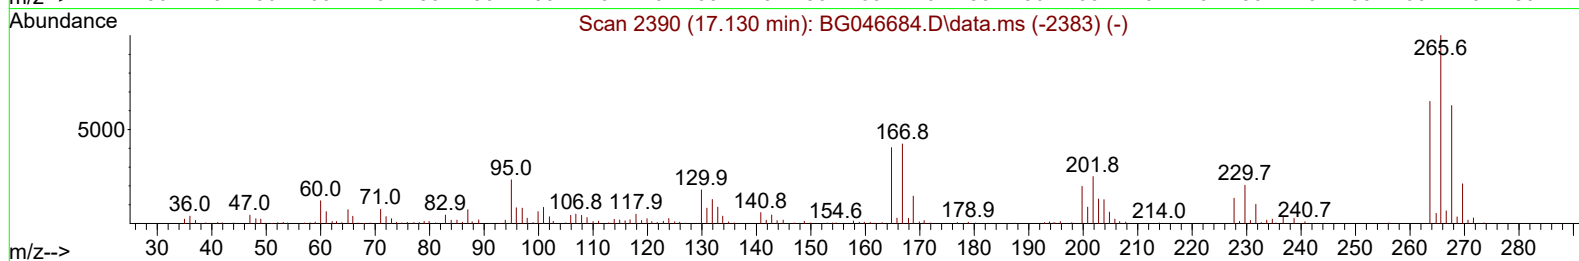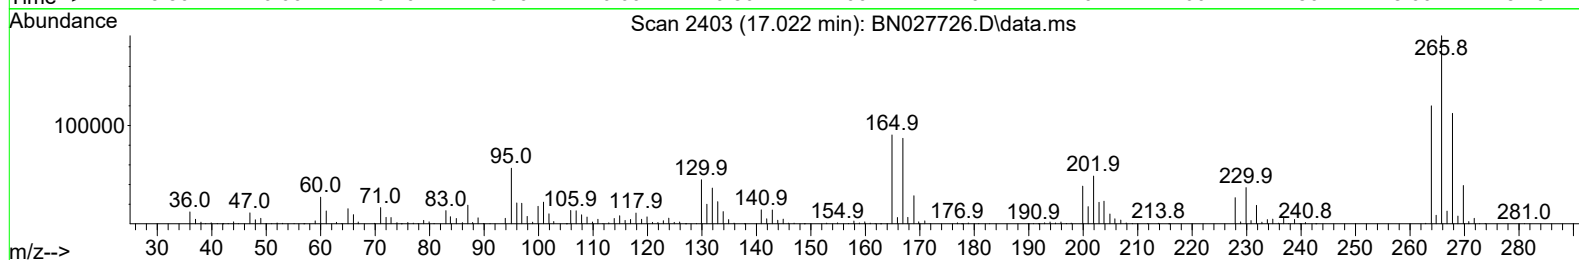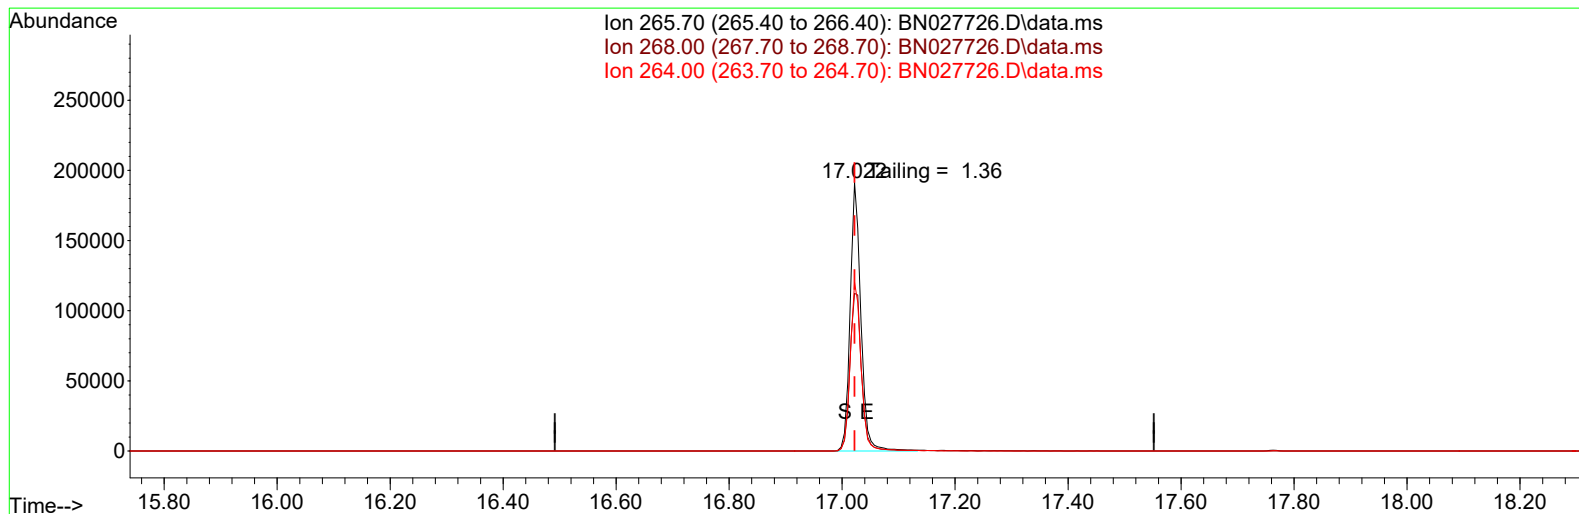

TIC: BN027726.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 20998.28 ng




response 254105

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.74
264.00	61.60	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091823\
Data File : BN027726.D
Acq On : 18 Sep 2023 09:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 19 04:23:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:23:17 2023
Response via : Initial Calibration

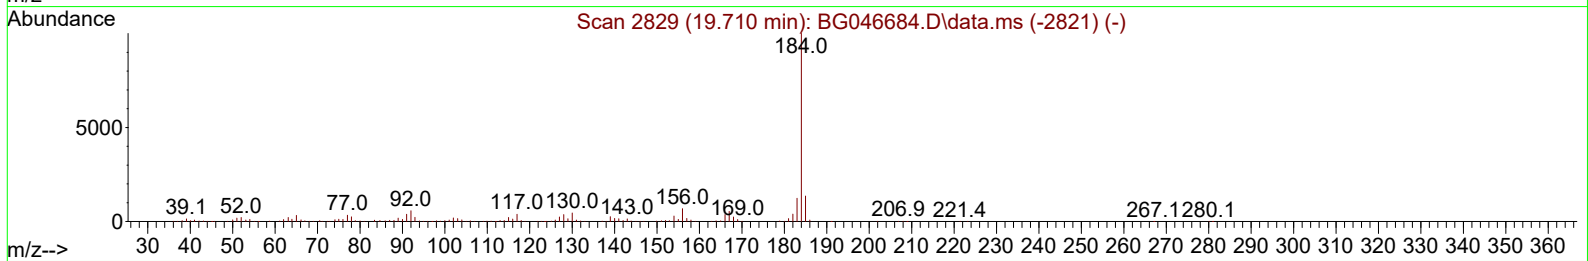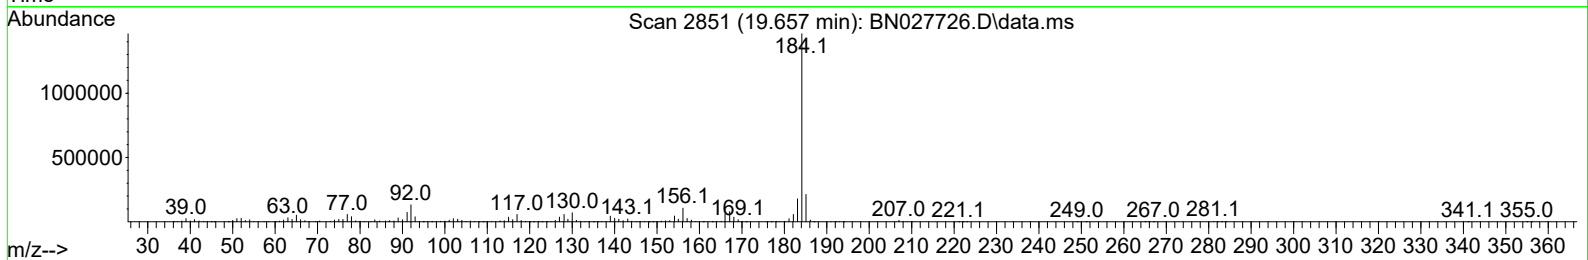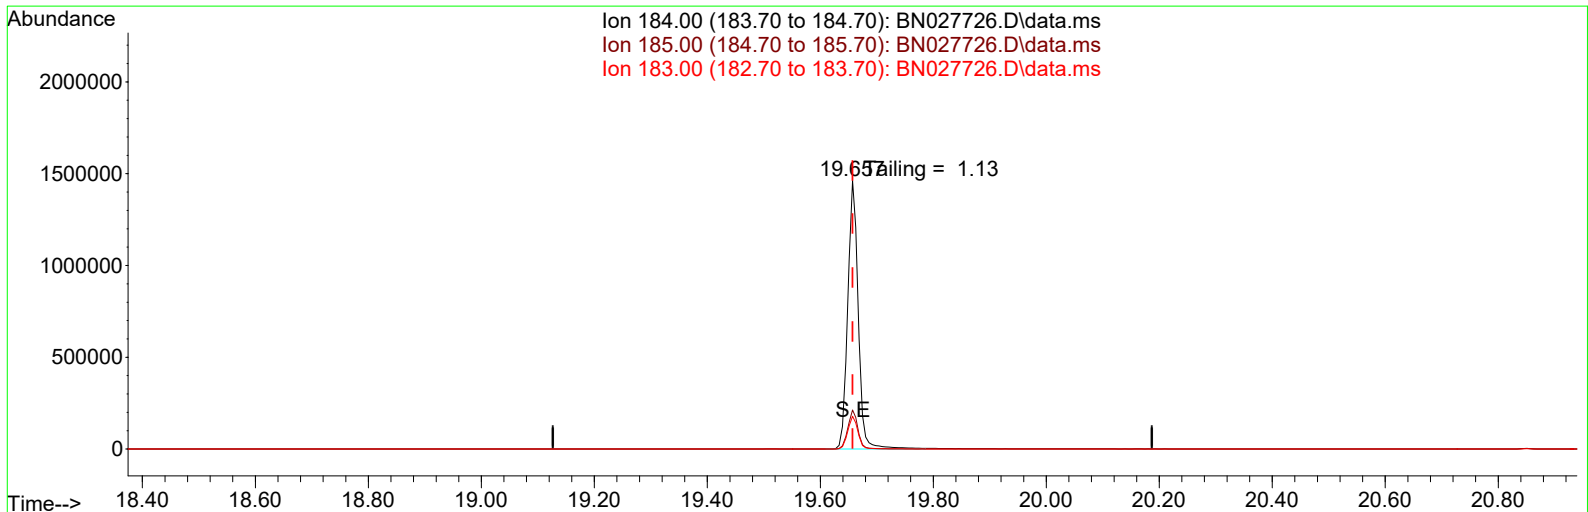

TIC: BN027726.D\data.ms

(77) Benzidine

19.657min (0.000) 0.00 ng

response 1901167

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.60
183.00	13.20	12.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2023	BNA_N	<u>BN027726.D</u>
Compound Name	Response	Retention Time
DDT	854014	20.851
DDD	16670	20.41
DDE	991	19.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17661	871675	2.03

Instrument :
BNA_N
ClientSampleId :
DFTPP