

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091919\
 Data File : BN007745.D
 Acq On : 19 Sep 2019 17:35
 Operator : HP/JU
 Sample : PB123223BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB123223BL

Quant Time: Sep 20 01:49:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 18:24:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	6039	0.40	ng	0.00
7) Naphthalene-d8	10.47	136	22515	0.40	ng	0.00
13) Acenaphthene-d10	14.32	164	12670	0.40	ng	0.00
19) Phenanthrene-d10	17.07	188	28847	0.40	ng	0.00
27) Chrysene-d12	21.27	240	29262	0.40	ng	0.00
34) Perylene-d12	23.48	264	18457	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.32	112	4797	0.23	ng	0.00
5) Phenol-d6	6.88	99	5883	0.22	ng	0.00
8) Nitrobenzene-d5	8.85	82	4905	0.25	ng	0.01
11) 2-Methylnaphthalene-d10	12.06	152	10889	0.29	ng	0.00
14) 2,4,6-Tribromophenol	15.82	330	1204	0.17	ng	0.00
15) 2-Fluorobiphenyl	12.94	172	15481	0.30	ng	0.00
25) Fluoranthene-d10	19.10	212	27577	0.28	ng	0.00
29) Terphenyl-d14	19.71	244	23325	0.32	ng	0.00
Target Compounds						
3) n-Nitrosodimethylamine	3.01	42	7818	2.536	ng	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091919\
Data File : BN007745.D
Acq On : 19 Sep 2019 17:35
Operator : HP/JU
Sample : PB123223BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB123223BL

Quant Time: Sep 20 01:49:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

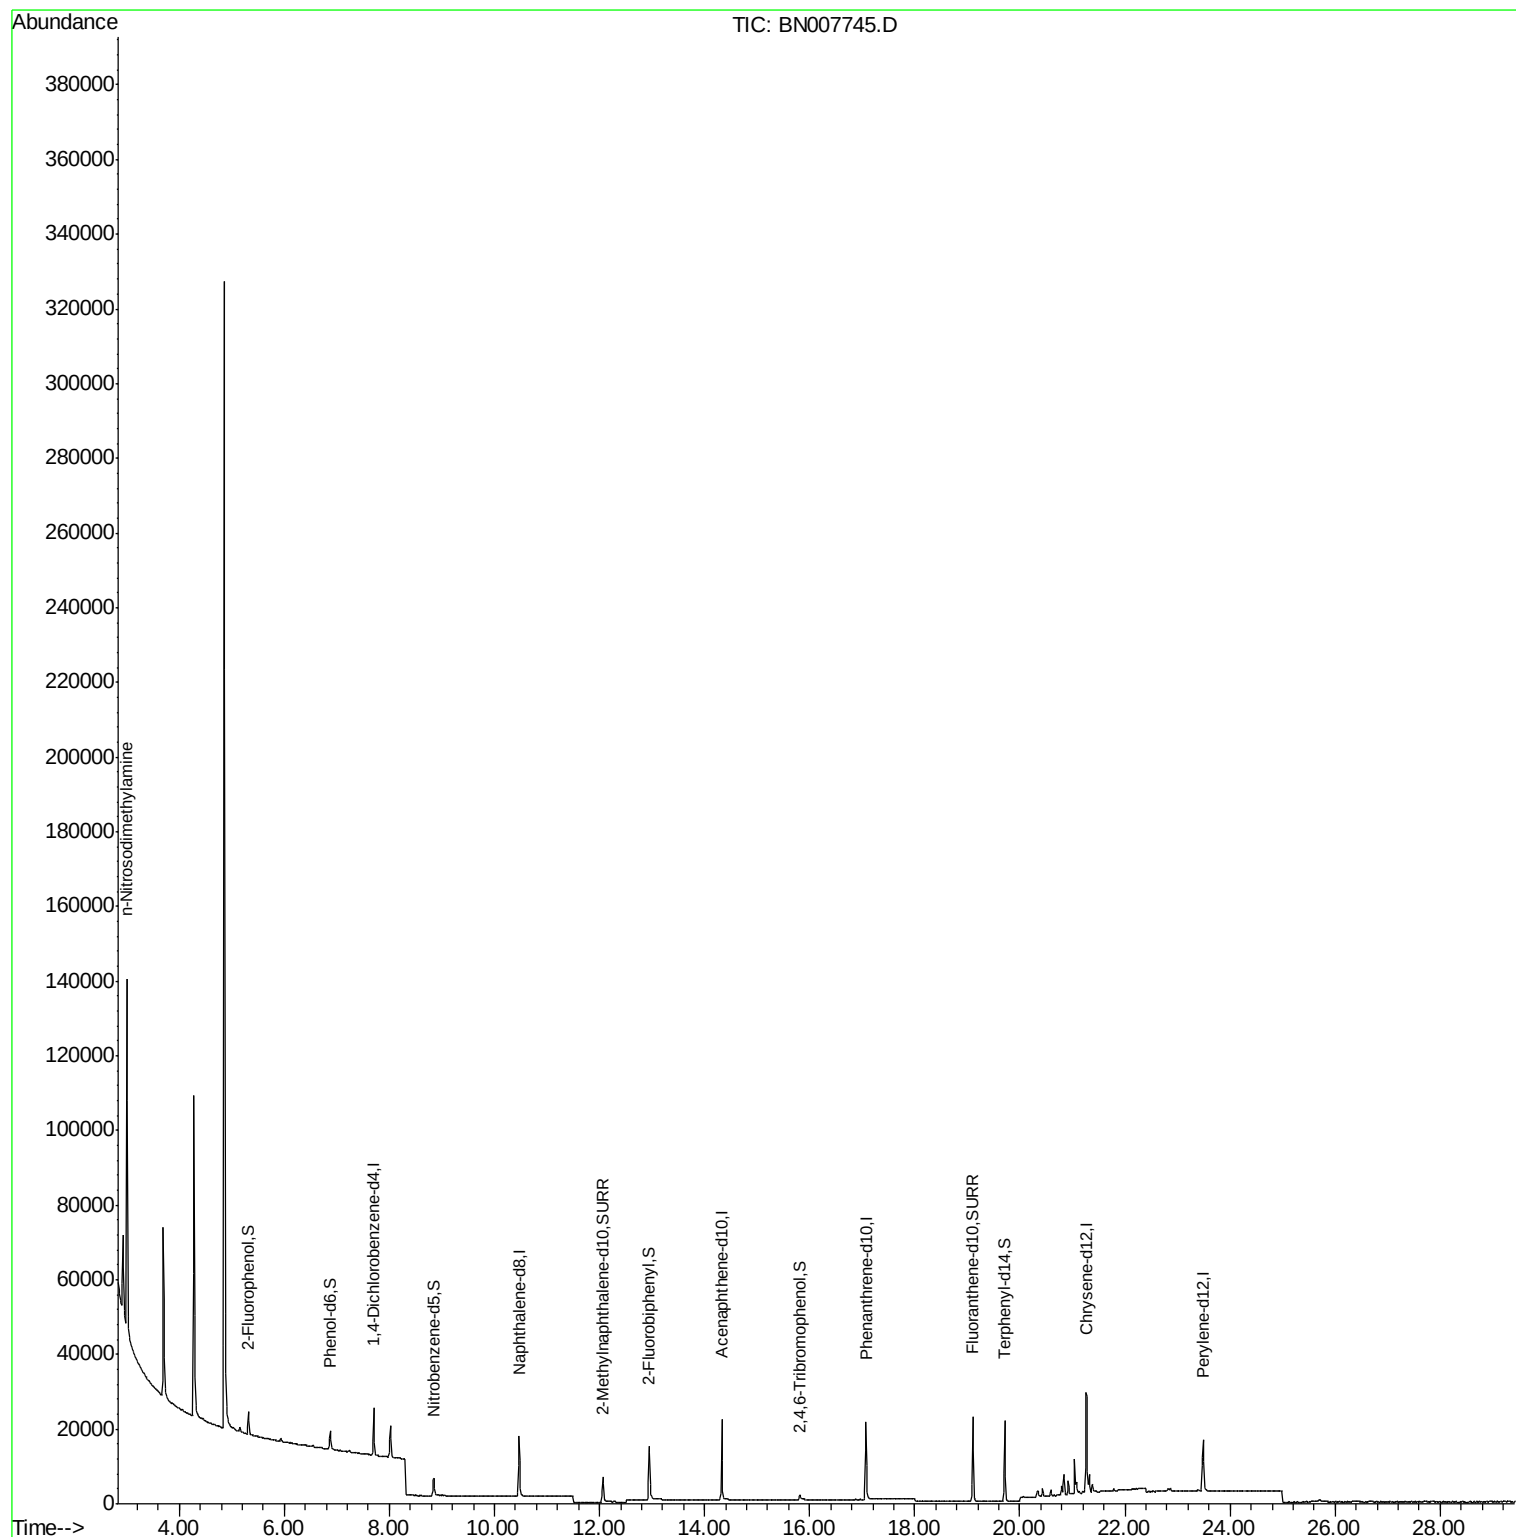

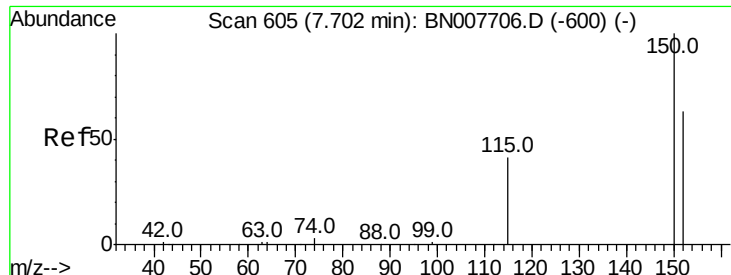

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.70 min Scan# 605

Delta R.T. 0.00 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35

Instrument :

BNA_N

ClientSampleId :

PB123223BL


Tot Ion:152 Resp: 6039

Ion Ratio Lower Upper

152 100

150 156.1 125.6 188.4




115 63.6 53.3 79.9

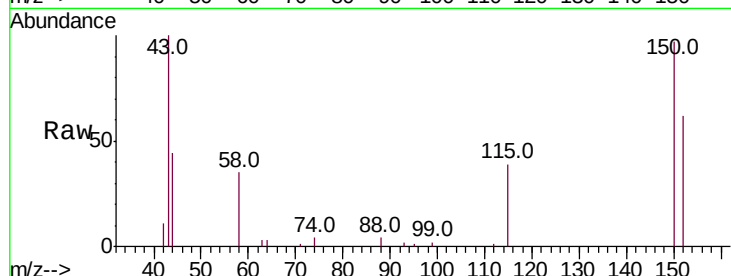

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

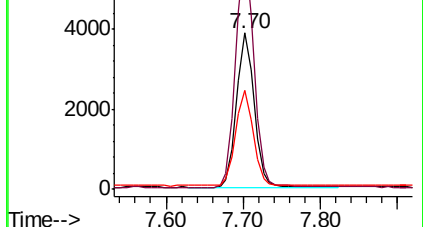

#3

n-Nitrosodimethylamine

Concen: 2.536 ng

RT: 3.01 min Scan# 22

Delta R.T. 0.00 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35


Tgt Ion: 42 Resp: 7818

Ion Ratio Lower Upper

42 100

74 127.7 87.9 131.9



44 30.5 29.4 44.0




Abundance Ion 42.00 (41.70 to 42.70): BNC

Ion 74.00 (73.70 to 74.70): BNC

Ion 44.00 (43.70 to 44.70): BNC

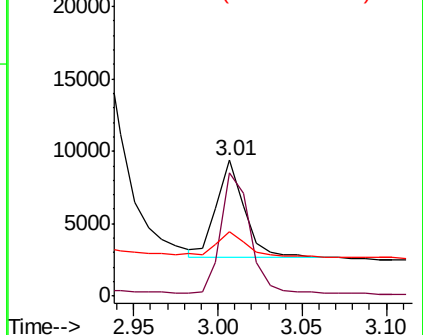

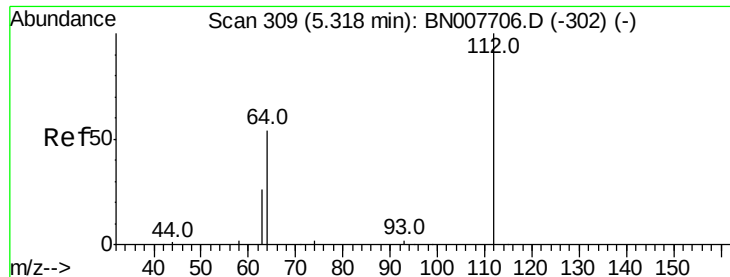

#4

2-Fluorophenol

Concen: 0.231 ng

RT: 5.32 min Scan# 309

Delta R.T. 0.00 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35

Instrument :

BNA_N

ClientSampleId :

PB123223BL


Tot Ion:112 Resp: 4797

Ion Ratio Lower Upper

112 100

64 59.6 46.6 70.0




63 30.3 23.1 34.7

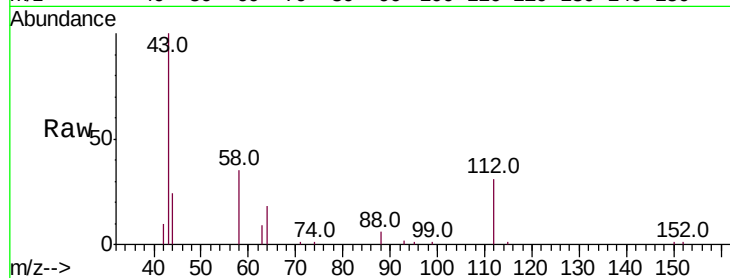

Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

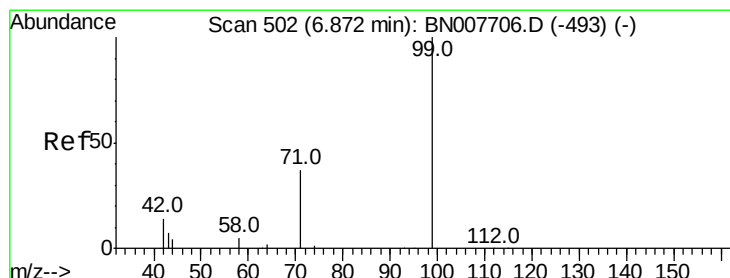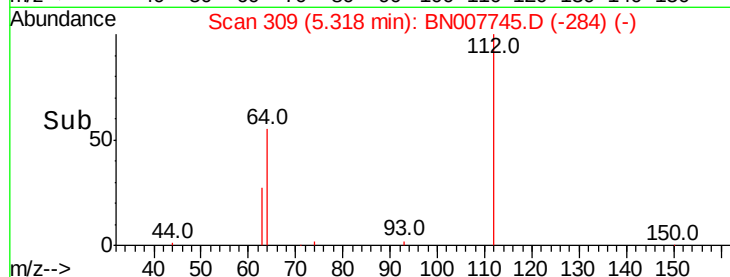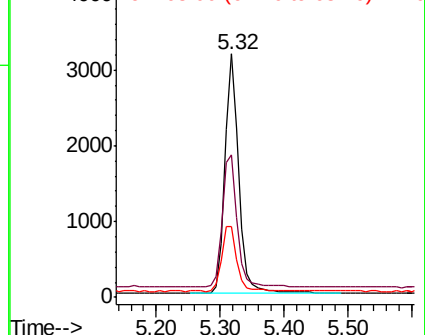

#5

Phenol-d6

Concen: 0.224 ng

RT: 6.88 min Scan# 503

Delta R.T. 0.01 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35


Tgt Ion: 99 Resp: 5883

Ion Ratio Lower Upper

99 100

42 14.3 12.8 19.2



71 34.5 27.6 41.4

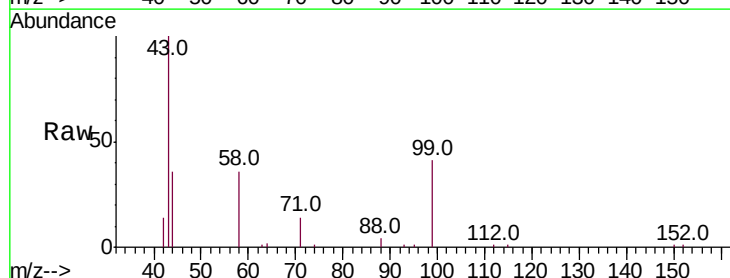


Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

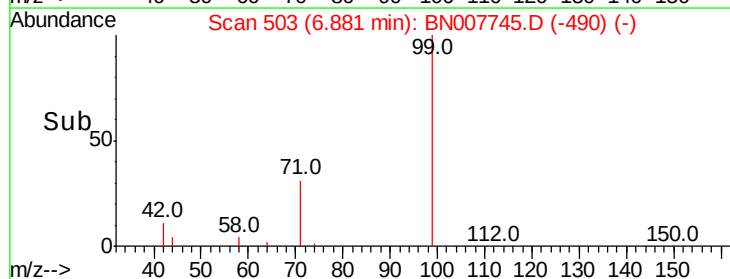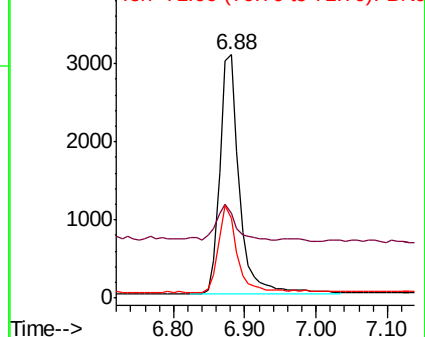



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.47 min Scan# 851

Delta R.T. 0.00 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35

Instrument :

BNA_N

ClientSampleId :

PB123223BL

Tot Ion:136 Resp: 22515


Ion Ratio Lower Upper

136 100

137 11.2 9.2 13.8

54 6.7 5.8 8.8

68 7.3 6.5 9.7






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

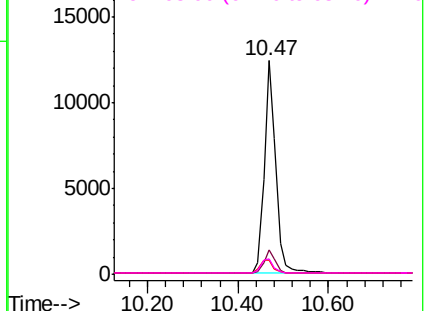

#8

Nitrobenzene-d5

Concen: 0.249 ng

RT: 8.85 min Scan# 723

Delta R.T. 0.01 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35


Tgt Ion: 82 Resp: 4905

Ion Ratio Lower Upper

82 100

128 42.4 24.5 36.7#



54 38.5 35.2 52.8




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC



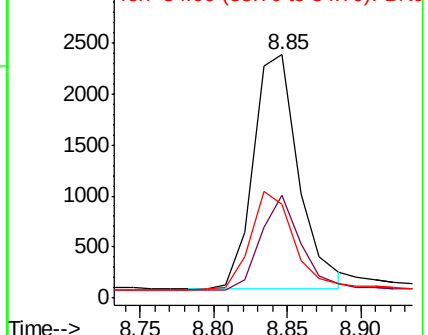



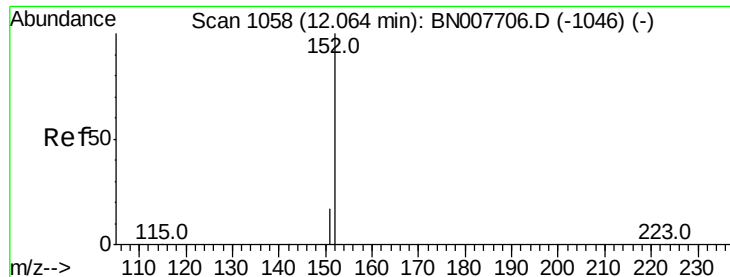

#11
2-Methylnaphthalene-d10
Concen: 0.287 ng
RT: 12.06 min Scan# 1058
Delta R.T. 0.00 min
Lab File: BN007745.D
Acq: 19 Sep 2019 17:35




Instrument :
BNA_N
ClientSampleId :
PB123223BL


Tot Ion:152 Resp: 10889
Ion Ratio Lower Upper
152 100
151 18.8 15.4 23.2

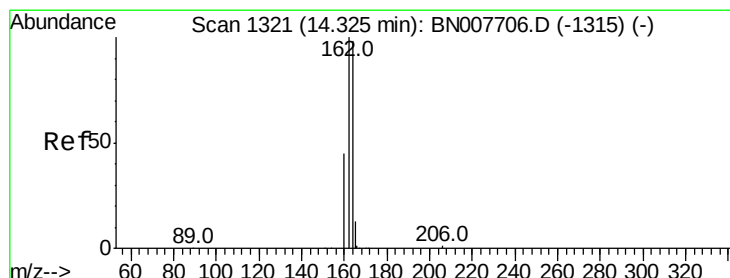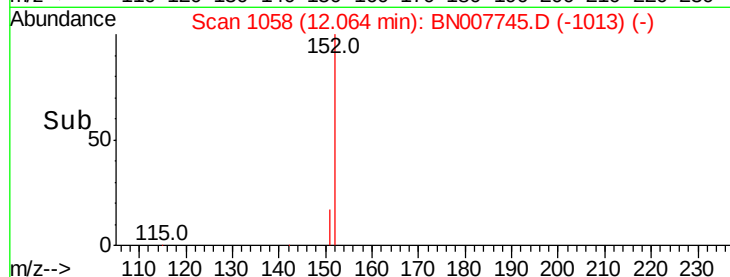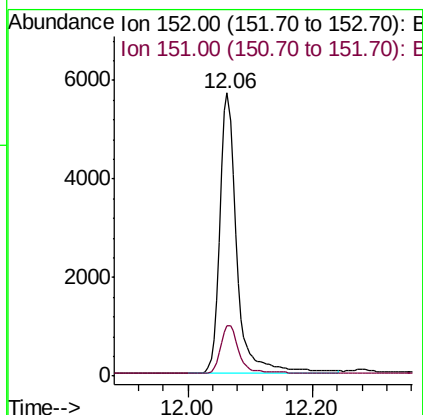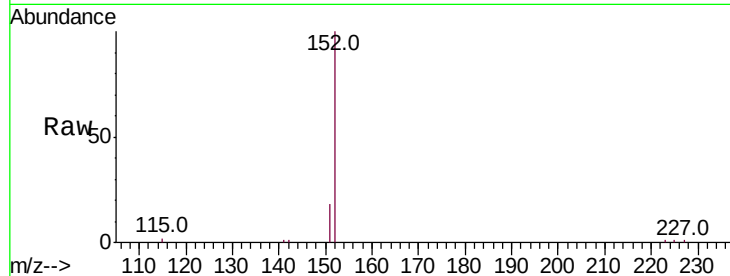

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.32 min Scan# 1321
Delta R.T. 0.00 min
Lab File: BN007745.D
Acq: 19 Sep 2019 17:35

Tgt Ion:164 Resp: 12670
Ion Ratio Lower Upper
164 100
162 100.7 81.7 122.5
160 46.4 37.0 55.4

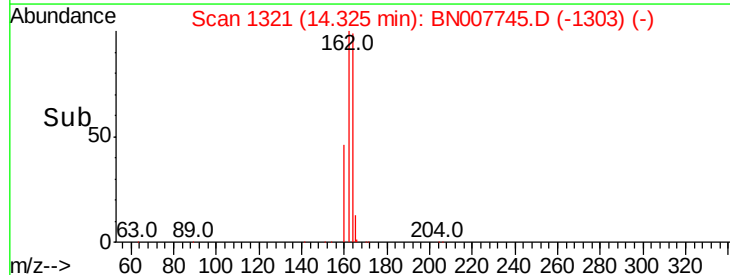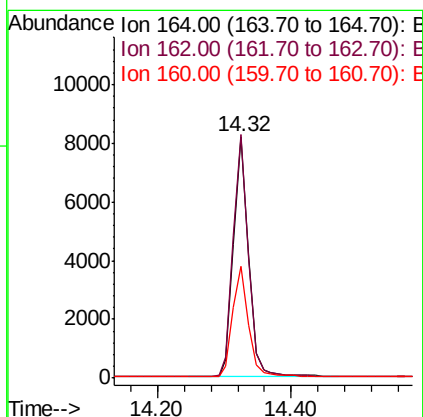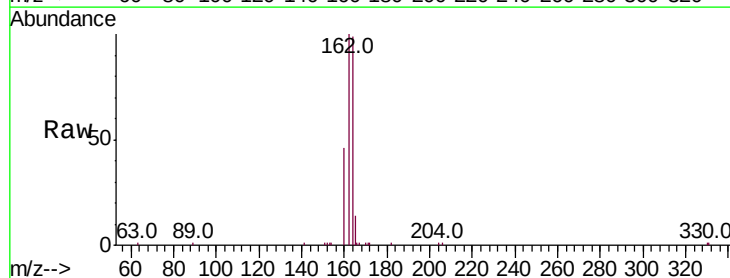







#14
 2,4,6-Tribromophenol
 Concen: 0.174 ng
 RT: 15.82 min Scan# 1455
 Delta R.T. 0.00 min
 Lab File: BN007745.D
 Acq: 19 Sep 2019 17:35

Instrument :
 BNA_N
 ClientSampleId :
 PB123223BL

Tot Ion:330 Resp: 1204
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 33.0 28.7 43.1

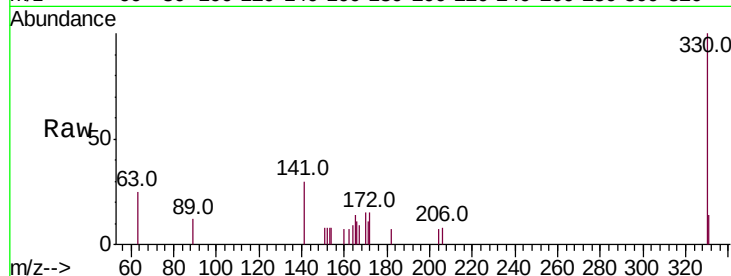


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


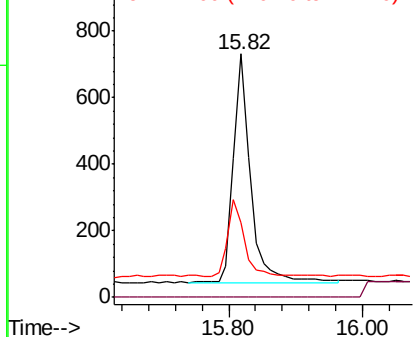



#15
 2-Fluorobiphenyl
 Concen: 0.297 ng
 RT: 12.94 min Scan# 1197
 Delta R.T. 0.00 min
 Lab File: BN007745.D
 Acq: 19 Sep 2019 17:35

Tgt Ion:172 Resp: 15481
 Ion Ratio Lower Upper
 172 100
 171 36.2 28.8 43.2
 170 24.3 19.5 29.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

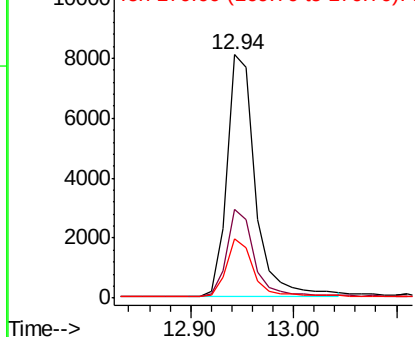



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.07 min Scan# 1572

Delta R.T. 0.00 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35

Instrument :

BNA_N

ClientSampleId :

PB123223BL


Tot Ion:188 Resp: 28847

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 9.6 7.4 11.2

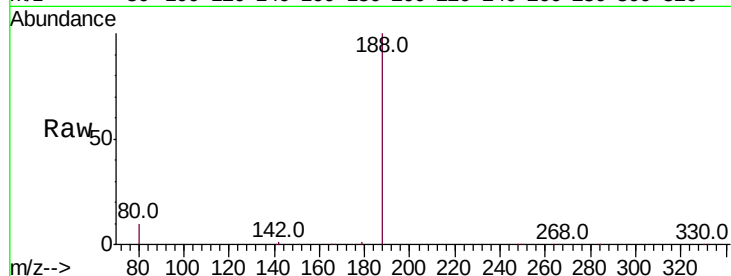

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNO

Ion 80.00 (79.70 to 80.70): BNO

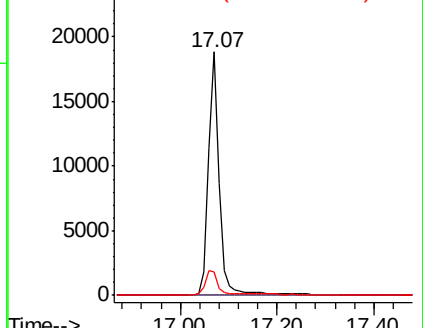

#25

Fluoranthene-d10

Concen: 0.284 ng

RT: 19.10 min Scan# 1881

Delta R.T. -0.00 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35


Tgt Ion:212 Resp: 27577

Ion Ratio Lower Upper

212 100

106 11.6 9.4 14.0



104 6.6 5.3 7.9




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

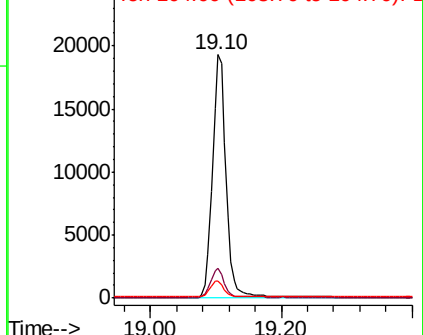



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.27 min Scan# 2182

Delta R.T. 0.00 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35

Instrument :

BNA_N

ClientSampleId :

PB123223BL


Tot Ion:240 Resp: 29262

Ion Ratio Lower Upper

240 100

120 5.4 5.4 8.2#




236 26.0 21.0 31.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

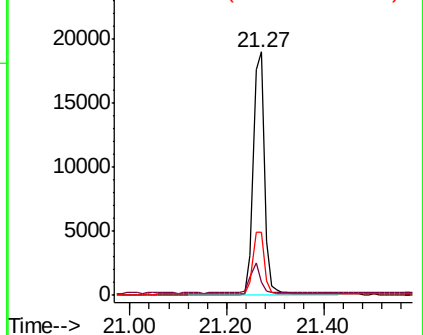

#29

Terphenyl-d14

Concen: 0.325 ng

RT: 19.71 min Scan# 2004

Delta R.T. 0.00 min

Lab File: BN007745.D

Acq: 19 Sep 2019 17:35


Tgt Ion:244 Resp: 23325

Ion Ratio Lower Upper

244 100

212 7.1 5.9 8.9



122 8.9 7.4 11.2






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

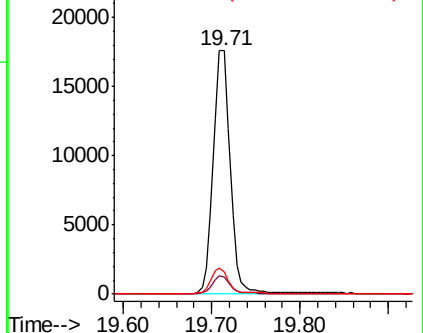

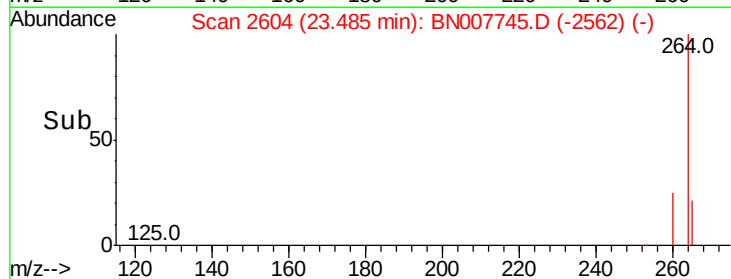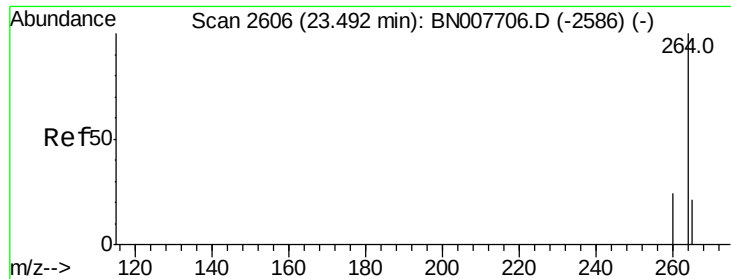

#34
 Pervlene-d12
 Concen: 0.400 ng
 RT: 23.48 min Scan# 2604
 Delta R.T. -0.01 min
 Lab File: BN007745.D
 Acq: 19 Sep 2019 17:35

Instrument :
 BNA_N
 ClientSampleId :
 PB123223BL

Tot Ion: 264 Resp: 18457
 Ion Ratio Lower Upper
 264 100
 260 25.2 19.3 28.9
 265 43.5 26.9 40.3#

