

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091919\
 Data File : BN007754.D
 Acq On : 19 Sep 2019 22:57
 Operator : HP/JU
 Sample : K4858-16 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 20 01:50:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 18:24:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	6351	0.40	ng	0.00
7) Naphthalene-d8	10.47	136	24182	0.40	ng	0.00
13) Acenaphthene-d10	14.32	164	14758	0.40	ng	0.00
19) Phenanthrene-d10	17.07	188	34202	0.40	ng	0.00
27) Chrysene-d12	21.26	240	37385	0.40	ng	-0.01
34) Perylene-d12	23.48	264	39107	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.32	112	676	0.03	ng	0.00
5) Phenol-d6	6.88	99	617	0.02	ng	0.00
8) Nitrobenzene-d5	8.85	82	1339	0.06	ng	0.01
11) 2-Methylnaphthalene-d10	12.06	152	3028	0.07	ng	0.00
14) 2,4,6-Tribromophenol	15.82	330	403	0.05	ng	0.00
15) 2-Fluorobiphenyl	12.94	172	5079	0.08	ng	0.00
25) Fluoranthene-d10	19.10	212	9196	0.08	ng	0.00
29) Terphenyl-d14	19.71	244	9203	0.10	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.30	88	10345	1.461	ng	# 90
3) n-Nitrosodimethylamine	3.01	42	26596	8.203	ng	# 74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN091919\
Data File : BN007754.D
Acq On : 19 Sep 2019 22:57
Operator : HP/JU
Sample : K4858-16 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 20 01:50:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

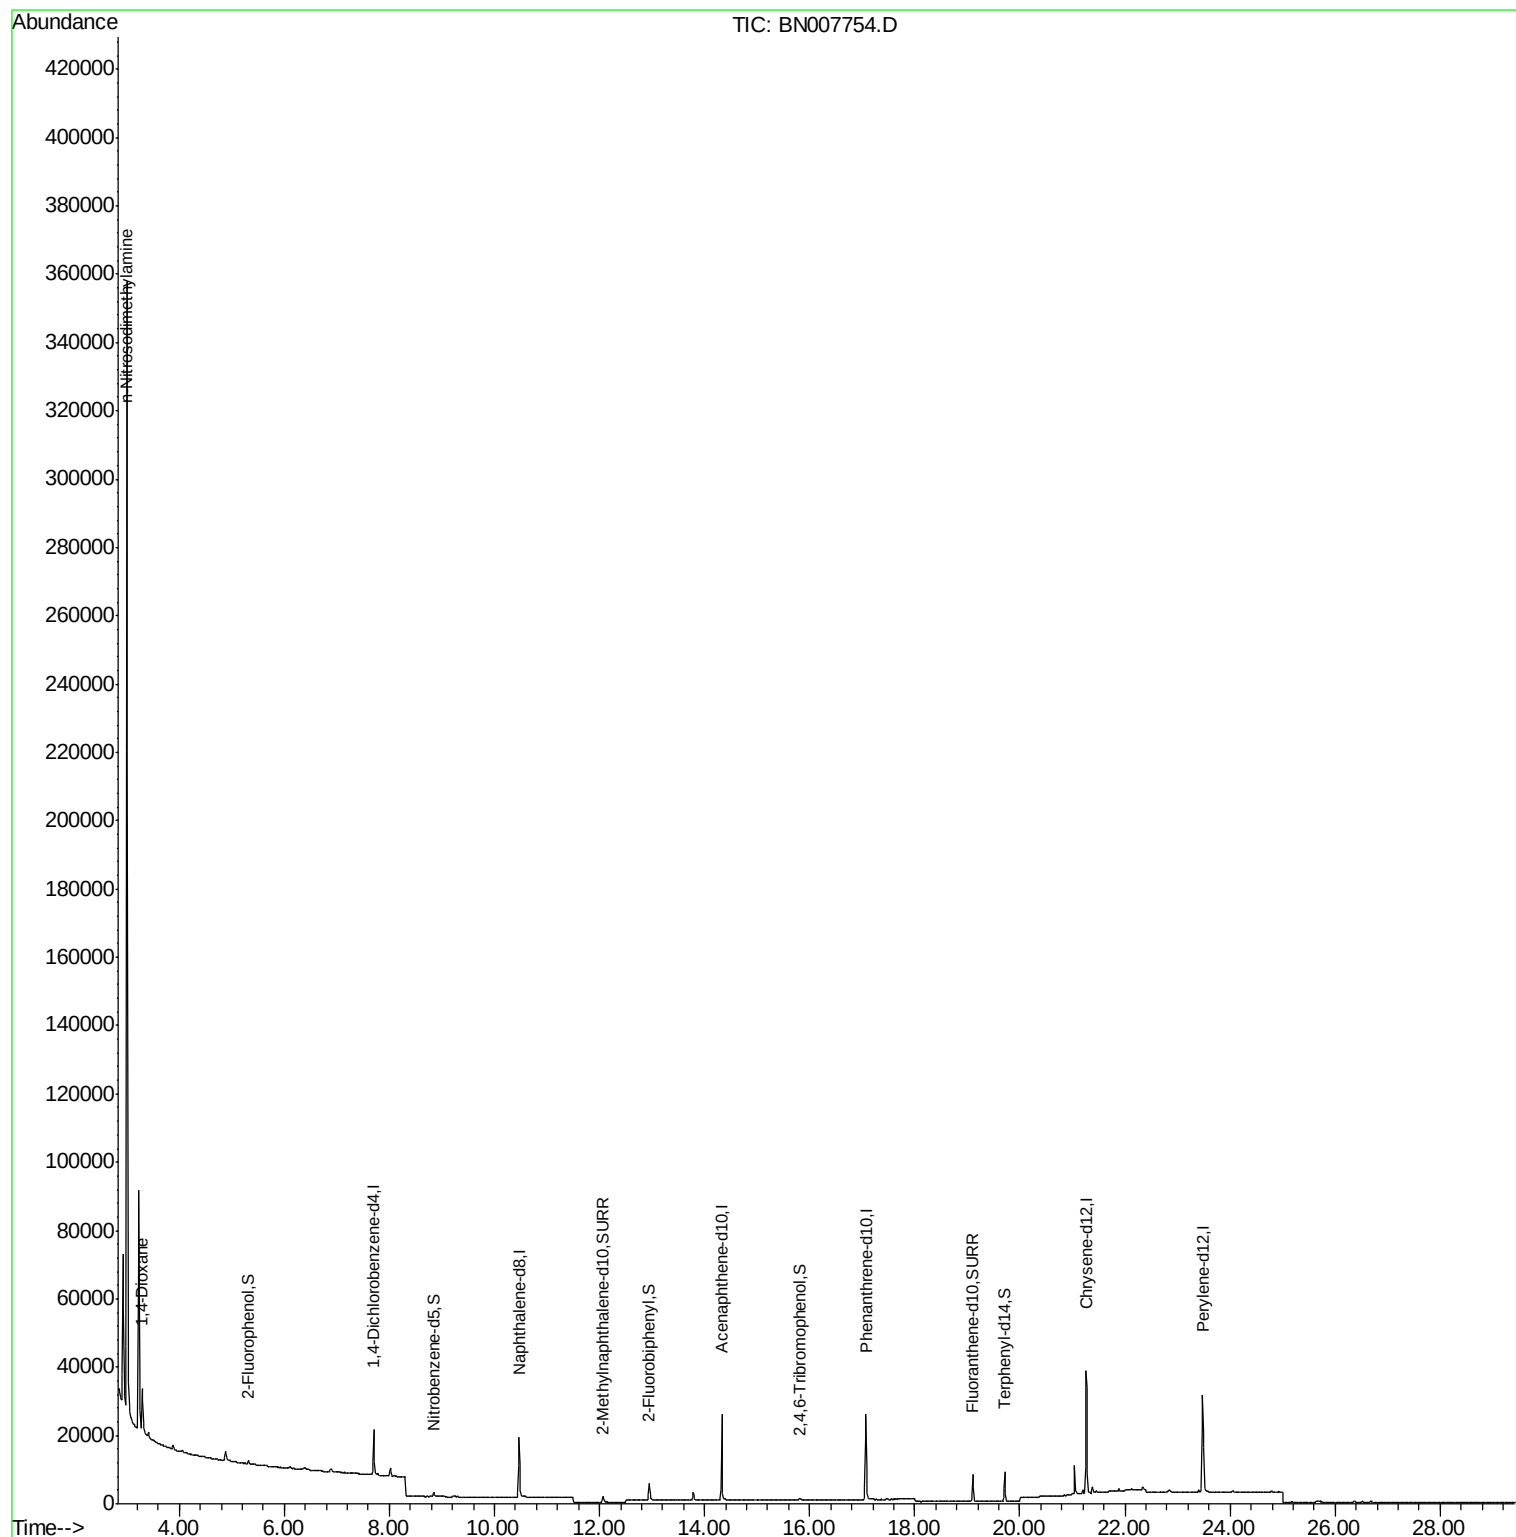

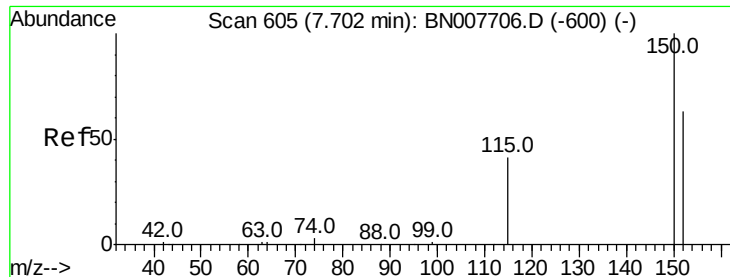


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.70 min Scan# 605
Delta R.T. -0.00 min
Lab File: BN007754.D
Acq: 19 Sep 2019 22:57

Instrument :
BNA_N
ClientSampleId :

Tot Ion:152 Resp: 6351
Ion Ratio Lower Upper
152 100
150 155.6 125.6 188.4
115 63.3 53.3 79.9

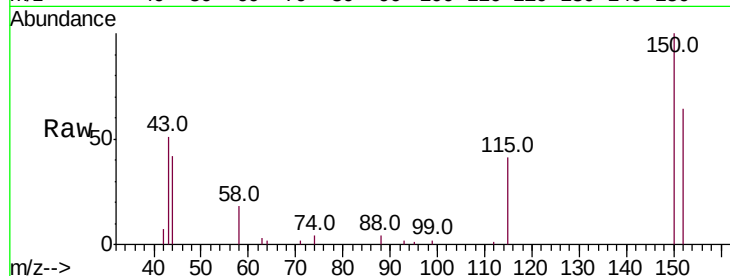


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

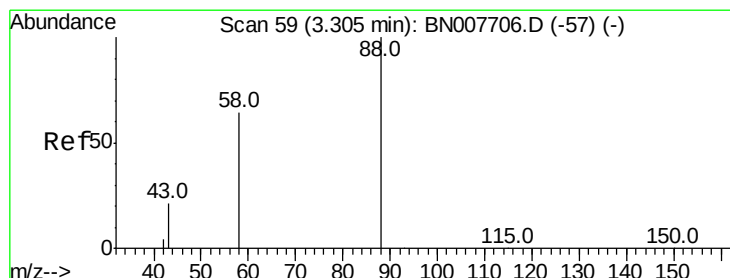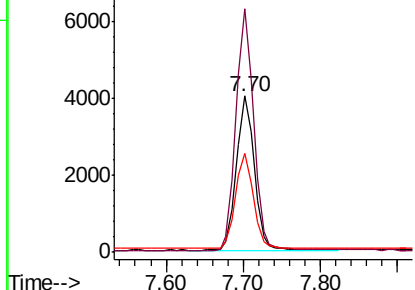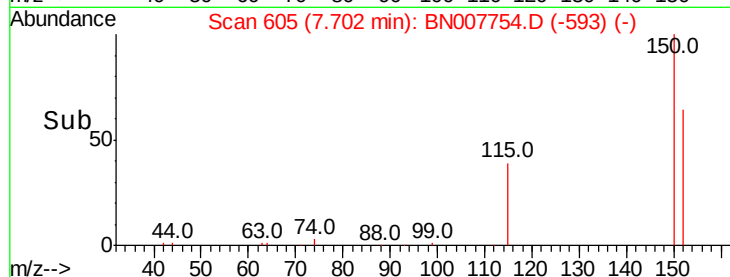



#2


1,4-Dioxane
Concen: 1.461 ng
RT: 3.30 min Scan# 58
Delta R.T. -0.01 min
Lab File: BN007754.D
Acq: 19 Sep 2019 22:57

Tgt Ion: 88 Resp: 10345
Ion Ratio Lower Upper
88 100
58 59.8 44.6 66.8
43 28.4 14.4 21.6#

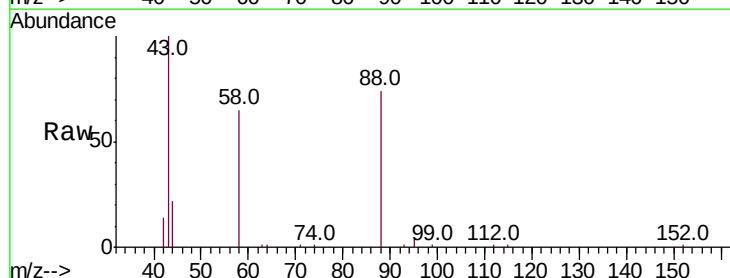

Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC

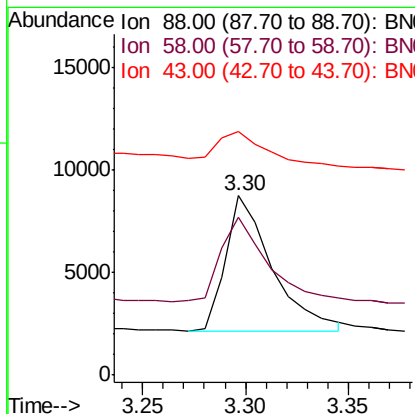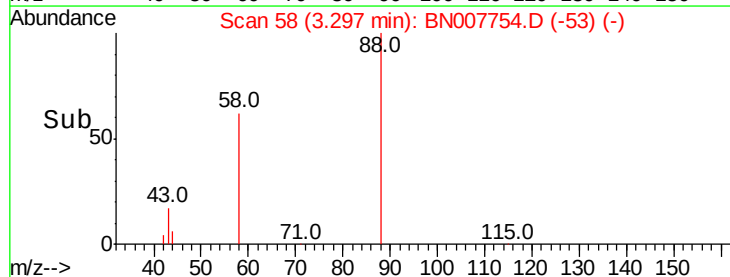

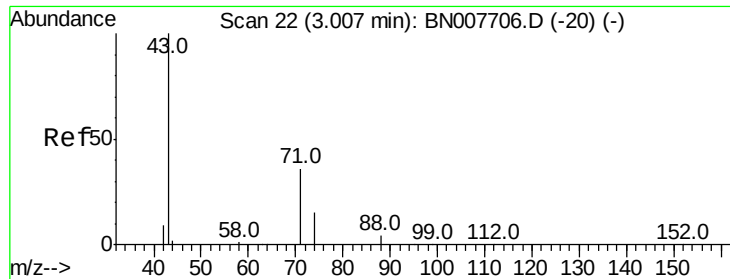

#3

n-Nitrosodimethylamine

Concen: 8.203 ng

RT: 3.01 min Scan# 22

Delta R.T. -0.00 min





Lab File: BN007754.D

Acq: 19 Sep 2019 22:57

Instrument :
BNA_N
ClientSampleId :

Tot Ion: 42 Resp: 26596

Ion	Ratio	Lower	Upper
42	100		
74	141.4	87.9	131.9#
44	27.0	29.4	44.0#

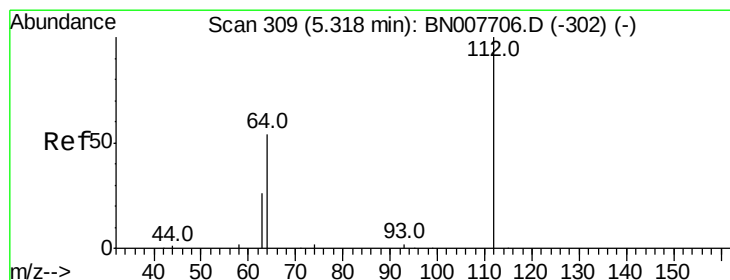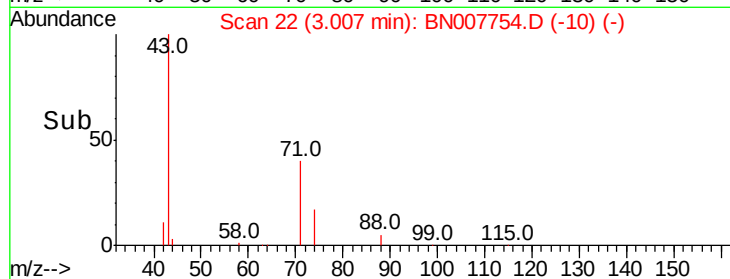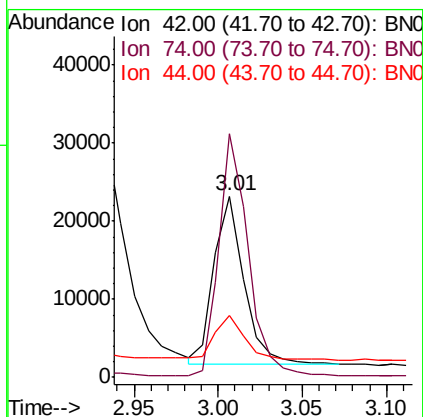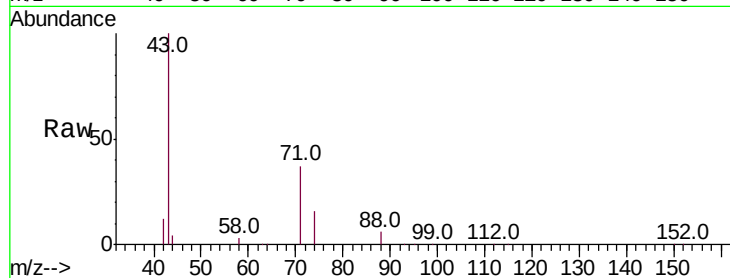

#4

2-Fluorophenol

Concen: 0.031 ng

RT: 5.32 min Scan# 309




Delta R.T. -0.00 min


Lab File: BN007754.D

Acq: 19 Sep 2019 22:57

Tgt Ion: 112 Resp: 676

Ion	Ratio	Lower	Upper
112	100		
64	62.4	46.6	70.0
63	32.8	23.1	34.7

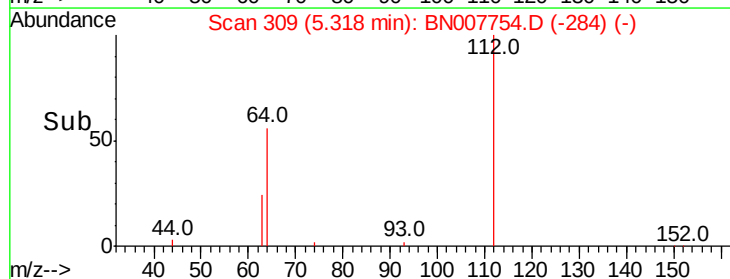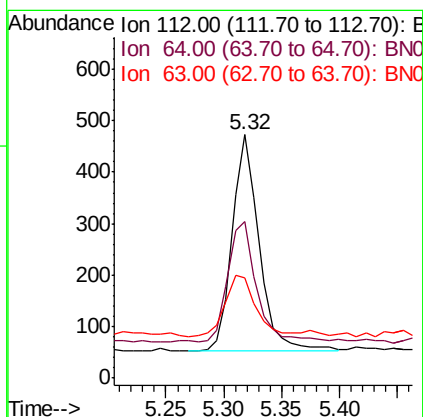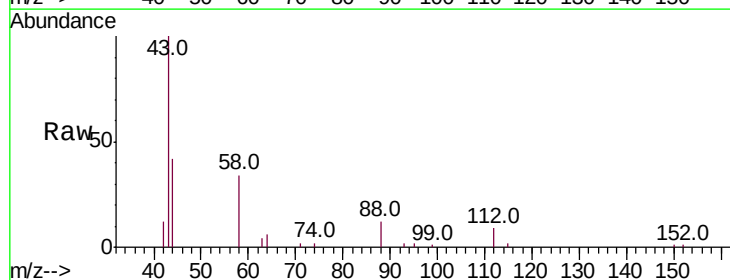



#5

Phenol-d6

Concen: 0.017 ng

RT: 6.88 min Scan# 503

Delta R.T. 0.01 min

Lab File: BN007754.D

Acq: 19 Sep 2019 22:57


Instrument :

BNA_N




ClientSampleId :

Tot Ion: 99 Resp: 617

Ion	Ratio	Lower	Upper
99	100		
42	36.8	12.8	19.2#
71	40.2	27.6	41.4

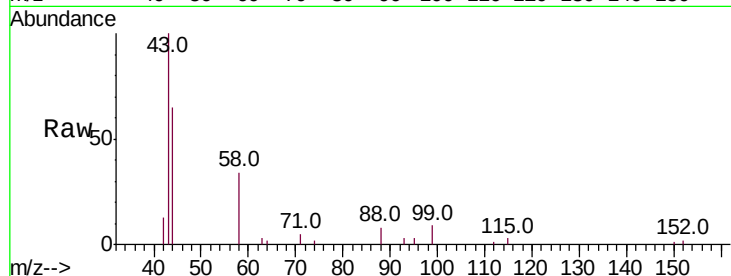

Abundance Ion 99.00 (98.70 to 99.70): BN007706.D (-493) (-)

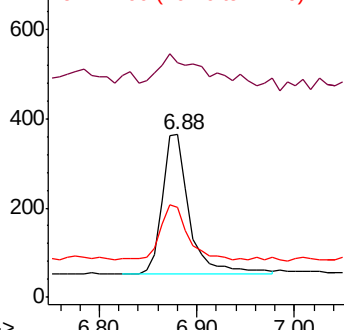

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.47 min Scan# 851


Delta R.T. -0.00 min

Lab File: BN007754.D



Acq: 19 Sep 2019 22:57


Tgt Ion: 136 Resp: 24182

Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.2	13.8
54	6.6	5.8	8.8
68	6.9	6.5	9.7



Abundance Ion 136.00 (135.70 to 136.70): BN007706.D (-846) (-)

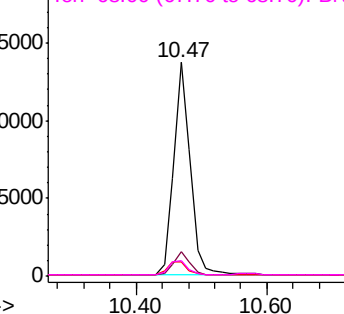



#8

Nitrobenzene-d5

Concen: 0.063 ng

RT: 8.85 min Scan# 723

Delta R.T. 0.01 min

Lab File: BN007754.D

Acq: 19 Sep 2019 22:57

Instrument :

BNA_N

ClientSampleId :


Tot Ion: 82 Resp: 1339

Ion Ratio Lower Upper

82 100

128 41.9 24.5 36.7#


54 41.6 35.2 52.8

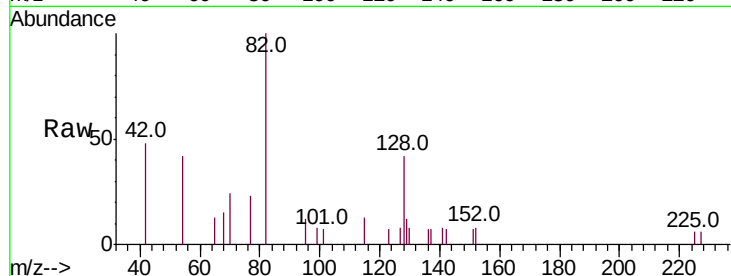



Abundance Ion 82.00 (81.70 to 82.70): BN007706.D (-719) (-)

Ion 128.00 (127.70 to 128.70): BN007706.D (-719) (-)

Ion 54.00 (53.70 to 54.70): BN007706.D (-719) (-)

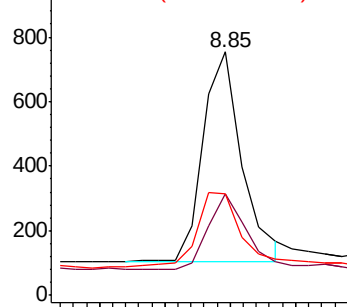

Time-->



#11

2-Methylnaphthalene-d10

Concen: 0.074 ng

RT: 12.06 min Scan# 1058

Delta R.T. -0.00 min

Lab File: BN007754.D


Acq: 19 Sep 2019 22:57

Tgt Ion: 152 Resp: 3028

Ion Ratio Lower Upper


152 100

151 19.7 15.4 23.2





Abundance Ion 152.00 (151.70 to 152.70): BN007706.D (-1046) (-)

Ion 151.00 (150.70 to 151.70): BN007706.D (-1046) (-)

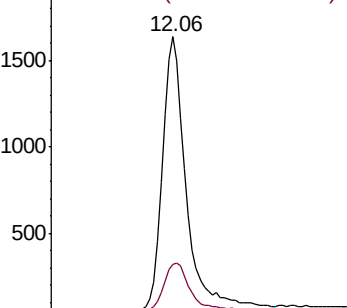

Time-->







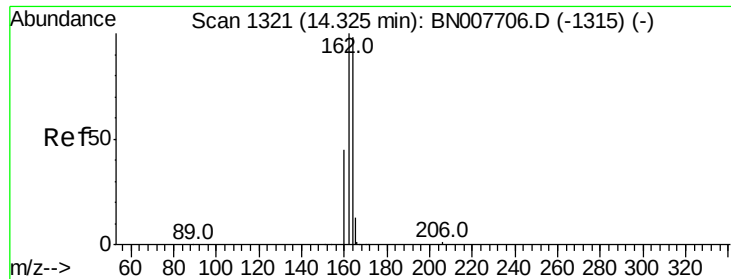

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.32 min Scan# 1321
Delta R.T. -0.00 min
Lab File: BN007754.D
Acq: 19 Sep 2019 22:57




Instrument :
BNA_N
ClientSampleId :


Tot Ion:164 Resp: 14758
Ion Ratio Lower Upper
164 100
162 102.2 81.7 122.5
160 46.0 37.0 55.4

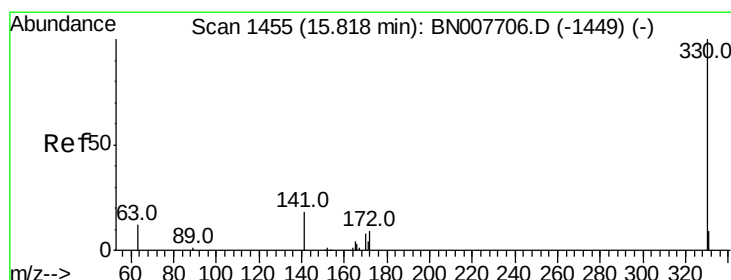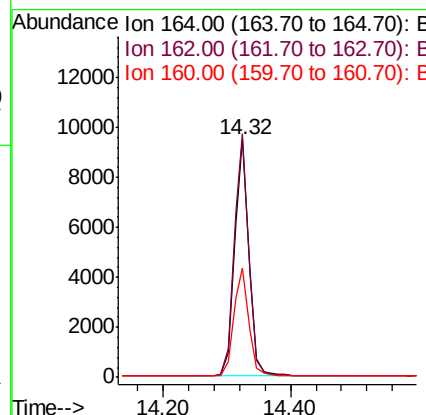

#14
2,4,6-Tribromophenol
Concen: 0.050 ng
RT: 15.82 min Scan# 1455
Delta R.T. -0.00 min
Lab File: BN007754.D
Acq: 19 Sep 2019 22:57

Tgt Ion:330 Resp: 403
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 41.7 28.7 43.1


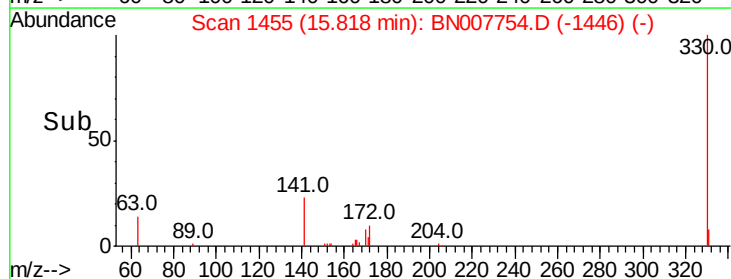
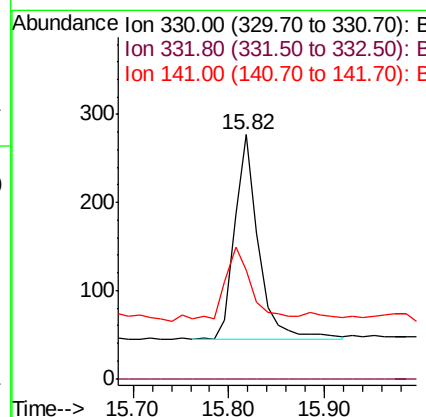
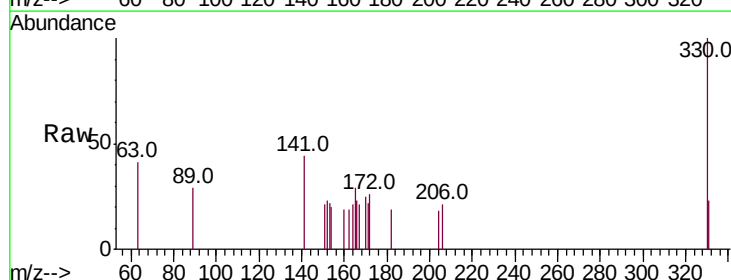


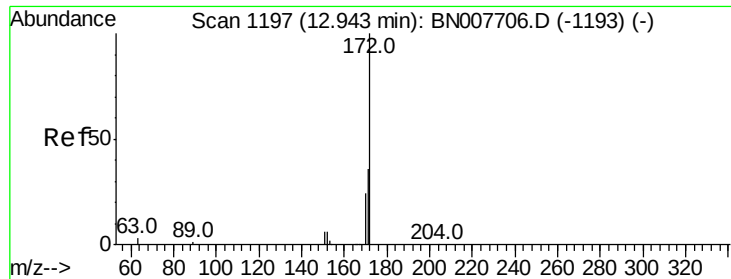

#15
2-Fluorobiphenyl
Concen: 0.084 ng
RT: 12.94 min Scan# 1197
Delta R.T. -0.00 min
Lab File: BN007754.D
Acq: 19 Sep 2019 22:57




Instrument :
BNA_N
ClientSampleId :


Tot Ion:172 Resp: 5079
Ion Ratio Lower Upper
172 100
171 36.5 28.8 43.2
170 25.2 19.5 29.3

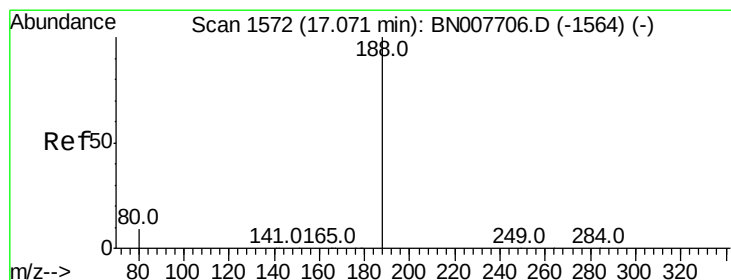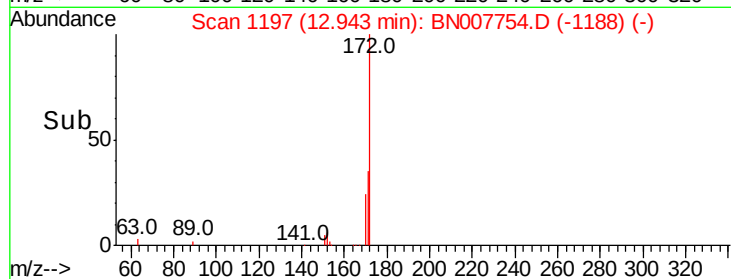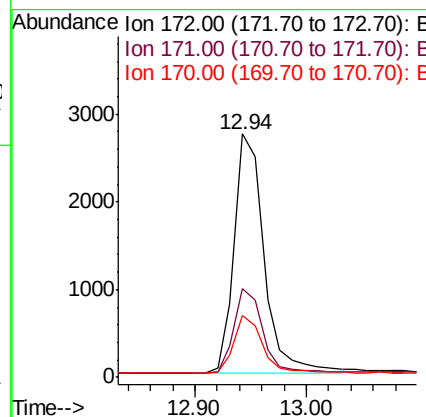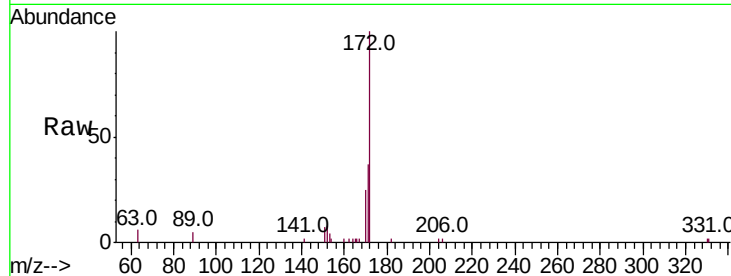

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.07 min Scan# 1572
Delta R.T. -0.00 min
Lab File: BN007754.D
Acq: 19 Sep 2019 22:57

Tgt Ion:188 Resp: 34202
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.4 7.4 11.2

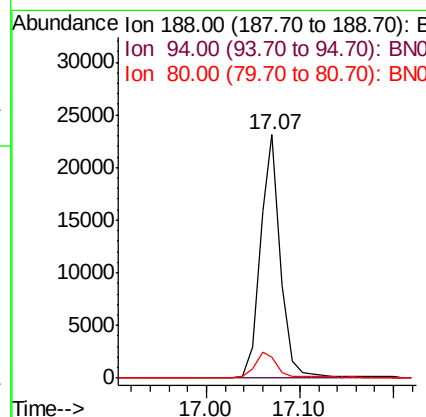



#25

Fluoranthene-d10

Concen: 0.080 ng

RT: 19.10 min Scan# 1881

Delta R.T. -0.01 min

Lab File: BN007754.D

Acq: 19 Sep 2019 22:57

Instrument :

BNA_N

ClientSampleId :


Tot Ion:212 Resp: 9196

Ion Ratio Lower Upper

212 100

106 12.4 9.4 14.0




104 6.8 5.3 7.9

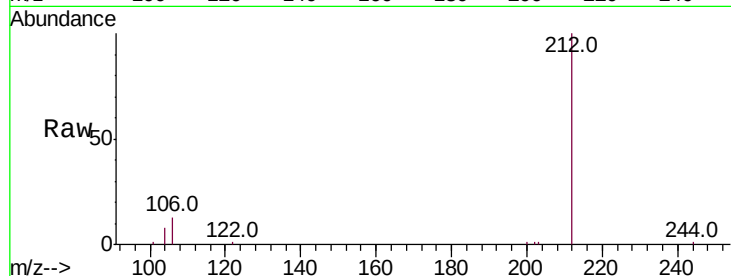

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

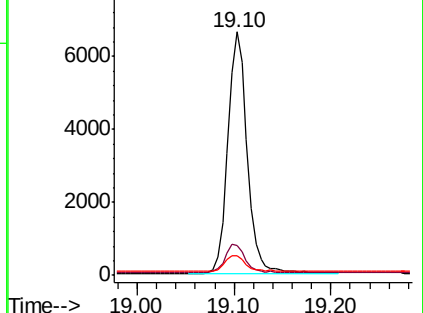

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.26 min Scan# 2181

Delta R.T. -0.01 min

Lab File: BN007754.D

Acq: 19 Sep 2019 22:57


Tgt Ion:240 Resp: 37385

Ion Ratio Lower Upper

240 100

120 12.5 5.4 8.2#



236 27.0 21.0 31.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

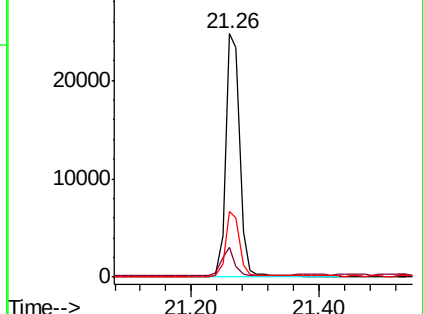



#29

Terphenyl-d14

Concen: 0.100 ng

RT: 19.71 min Scan# 2003

Delta R.T. -0.01 min

Lab File: BN007754.D

Acq: 19 Sep 2019 22:57

Instrument :

BNA_N

ClientSampleId :


Tot Ion:244 Resp: 9203

Ion Ratio Lower Upper

244 100

212 7.8 5.9 8.9




122 11.0 7.4 11.2

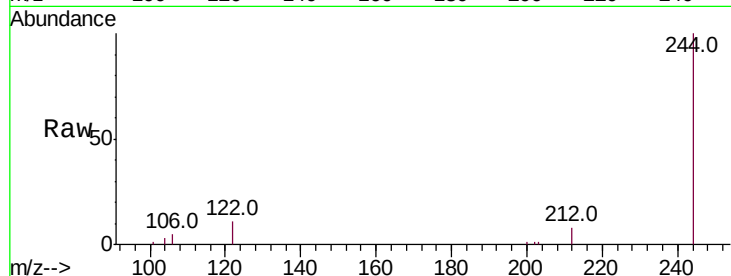

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

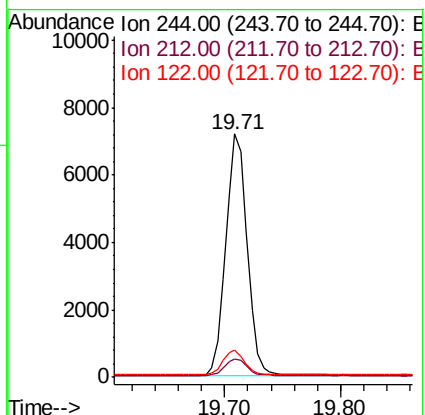

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.48 min Scan# 2603

Delta R.T. -0.01 min

Lab File: BN007754.D

Acq: 19 Sep 2019 22:57


Tgt Ion:264 Resp: 39107

Ion Ratio Lower Upper

264 100

260 24.1 19.3 28.9

265 31.8 26.9 40.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

