


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN091919\
 Data File : BN007740.D
 Acq On : 19 Sep 2019 14:36
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 18 18:24:40 2019

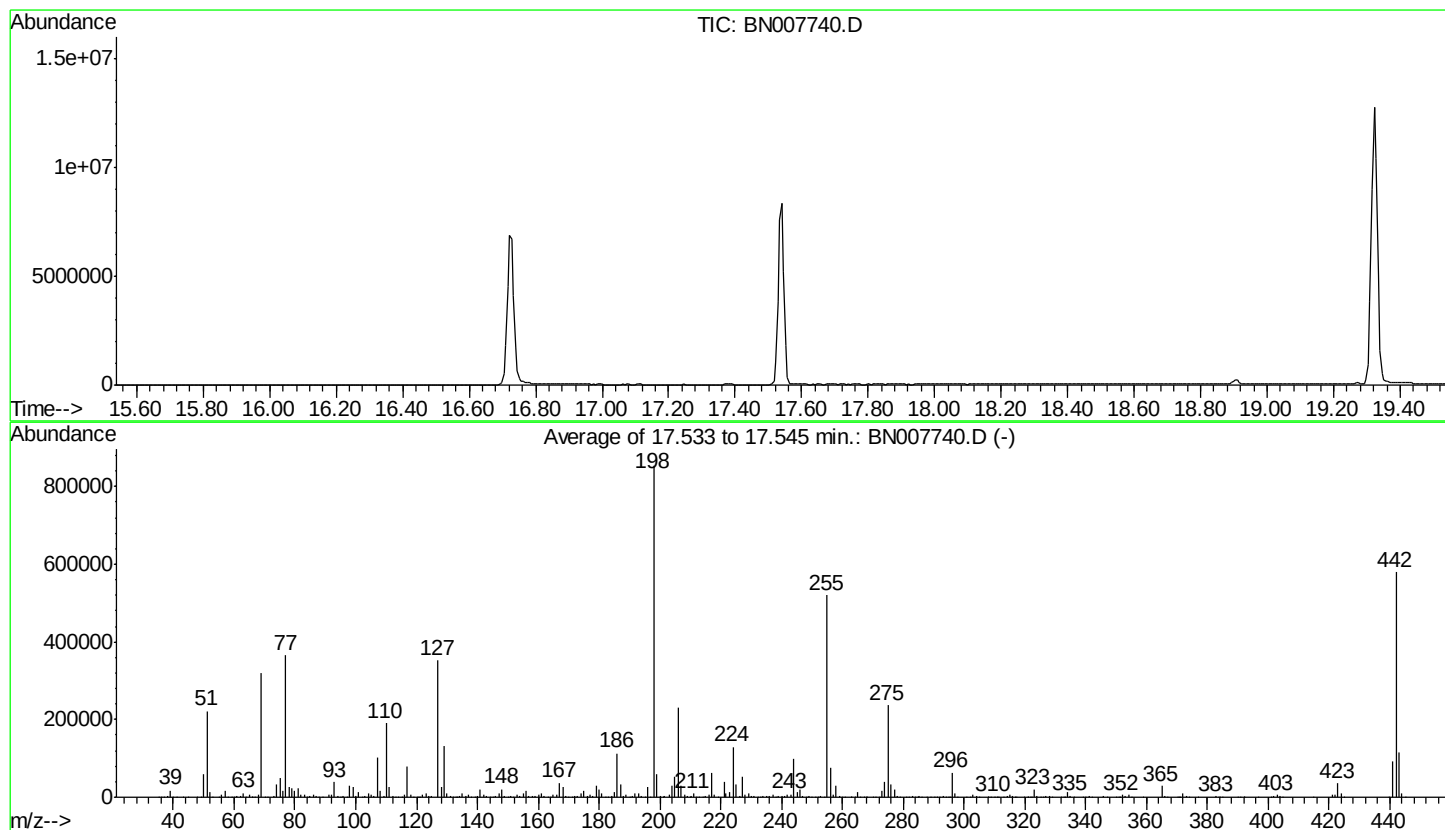

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.0	221573	PASS
68	69	0.00	2	1.8	5847	PASS
69	198	0.00	100	37.3	318613	PASS
70	69	0.00	2	0.5	1741	PASS
127	198	10	80	41.2	351402	PASS
197	198	0.00	2	0.1	1170	PASS
198	198	100	100	100.0	853802	PASS
199	198	5	9	6.9	58600	PASS
275	198	10	60	27.8	237184	PASS
365	198	1	100	3.3	28378	PASS
441	198	0.01	100	10.8	91984	PASS
442	198	50	100	67.8	579200	PASS
443	442	15	24	19.8	114746	PASS