
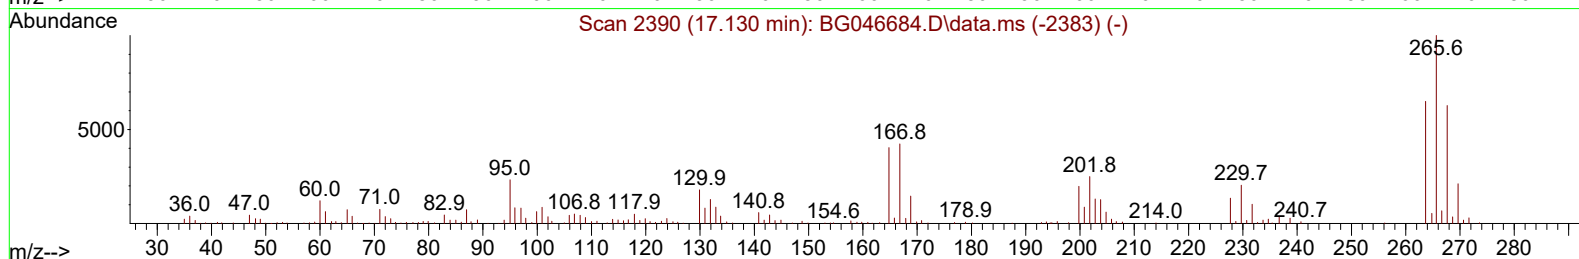
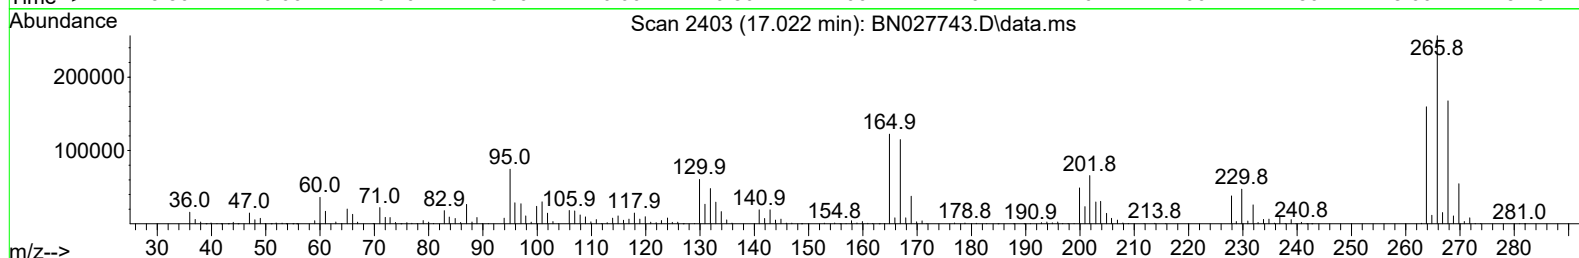


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091923\
Data File : BN027743.D
Acq On : 19 Sep 2023 08:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 01:23:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 01:23:52 2023
Response via : Initial Calibration

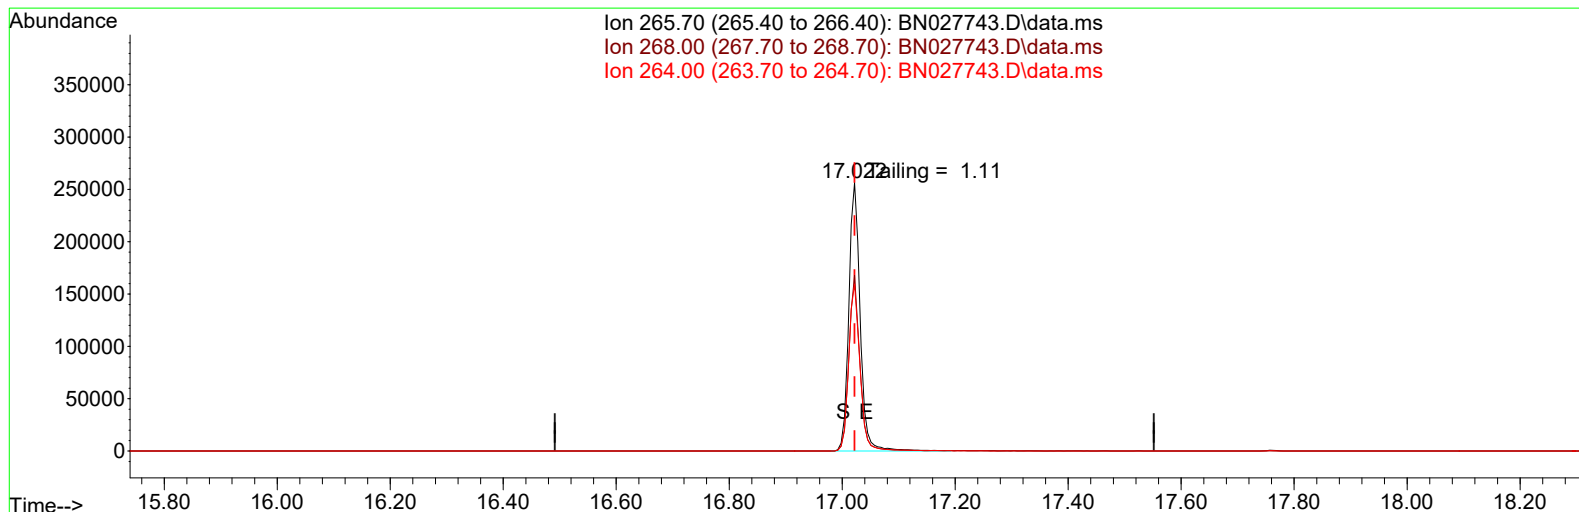

TIC: BN027743.D\data.ms

(70) Pentachlorophenol (C)




17.022min (0.000) 23471.22 ng

response 358630

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.41
264.00	61.60	62.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091923\
Data File : BN027743.D
Acq On : 19 Sep 2023 08:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 01:23:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 01:23:52 2023
Response via : Initial Calibration

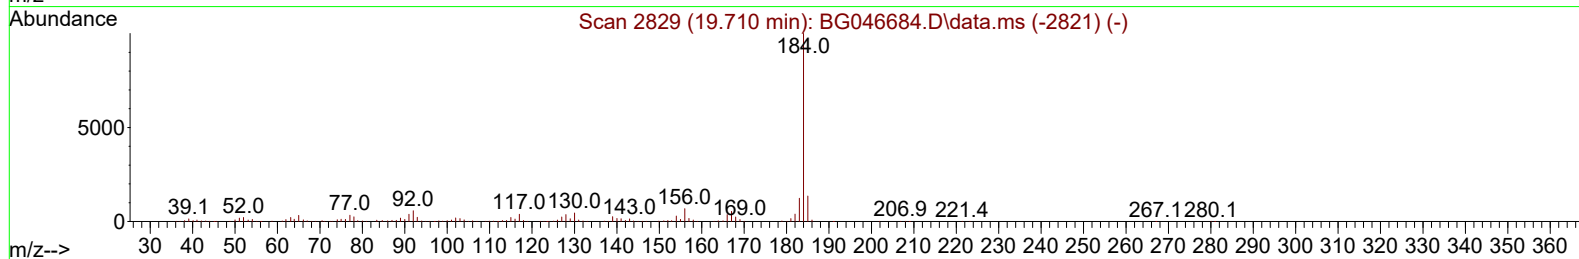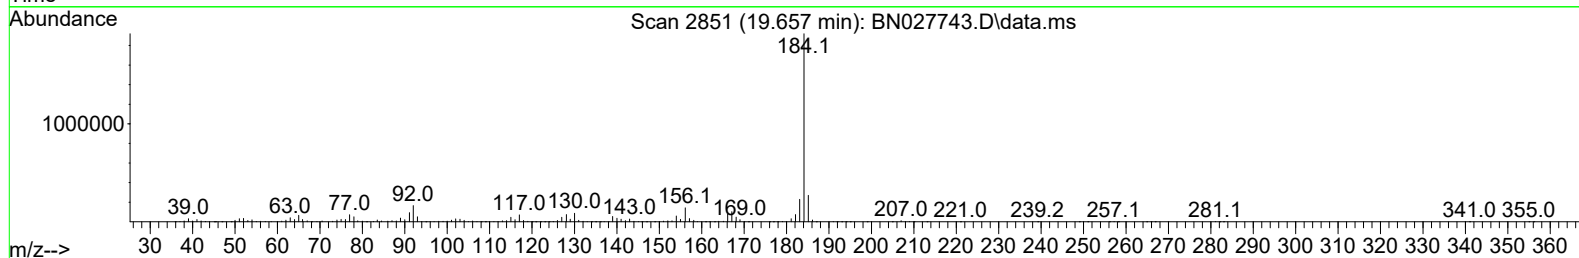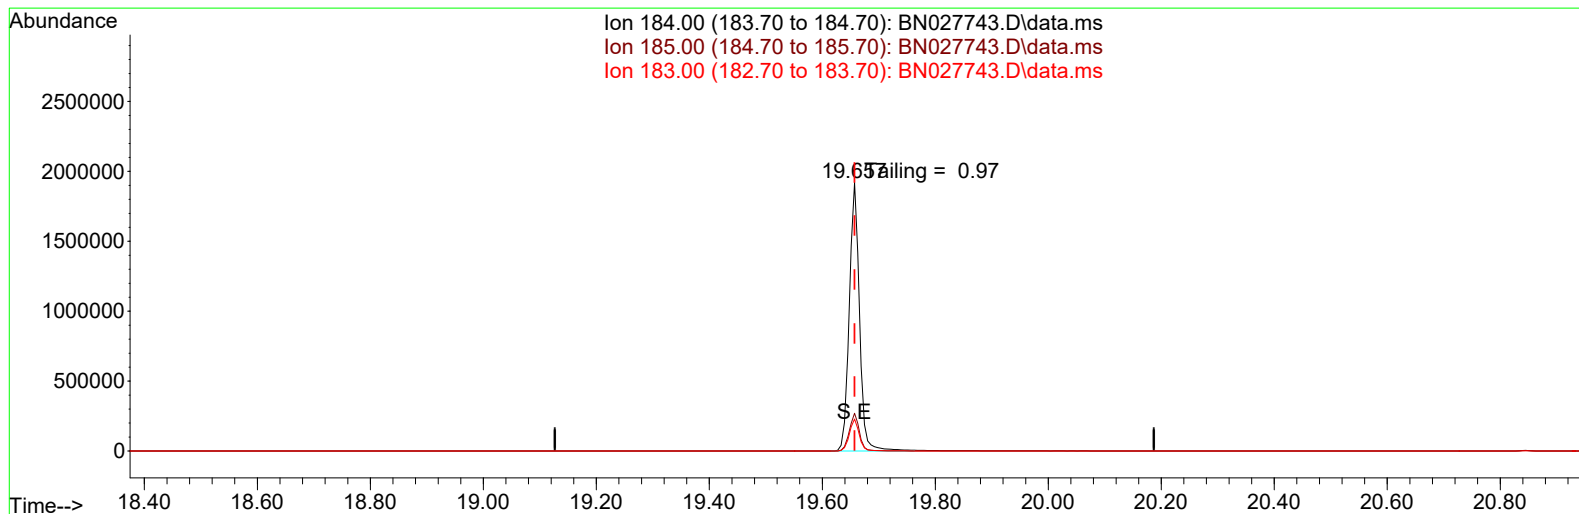

TIC: BN027743.D\data.ms

(77) Benzidine

19.657min (0.000) 0.00 ng

response 2435547

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	11.95
0.00	0.00	0.00