


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091923\
 Data File : BN027743.D
 Acq On : 19 Sep 2023 08:38
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 18 14:40:21 2023

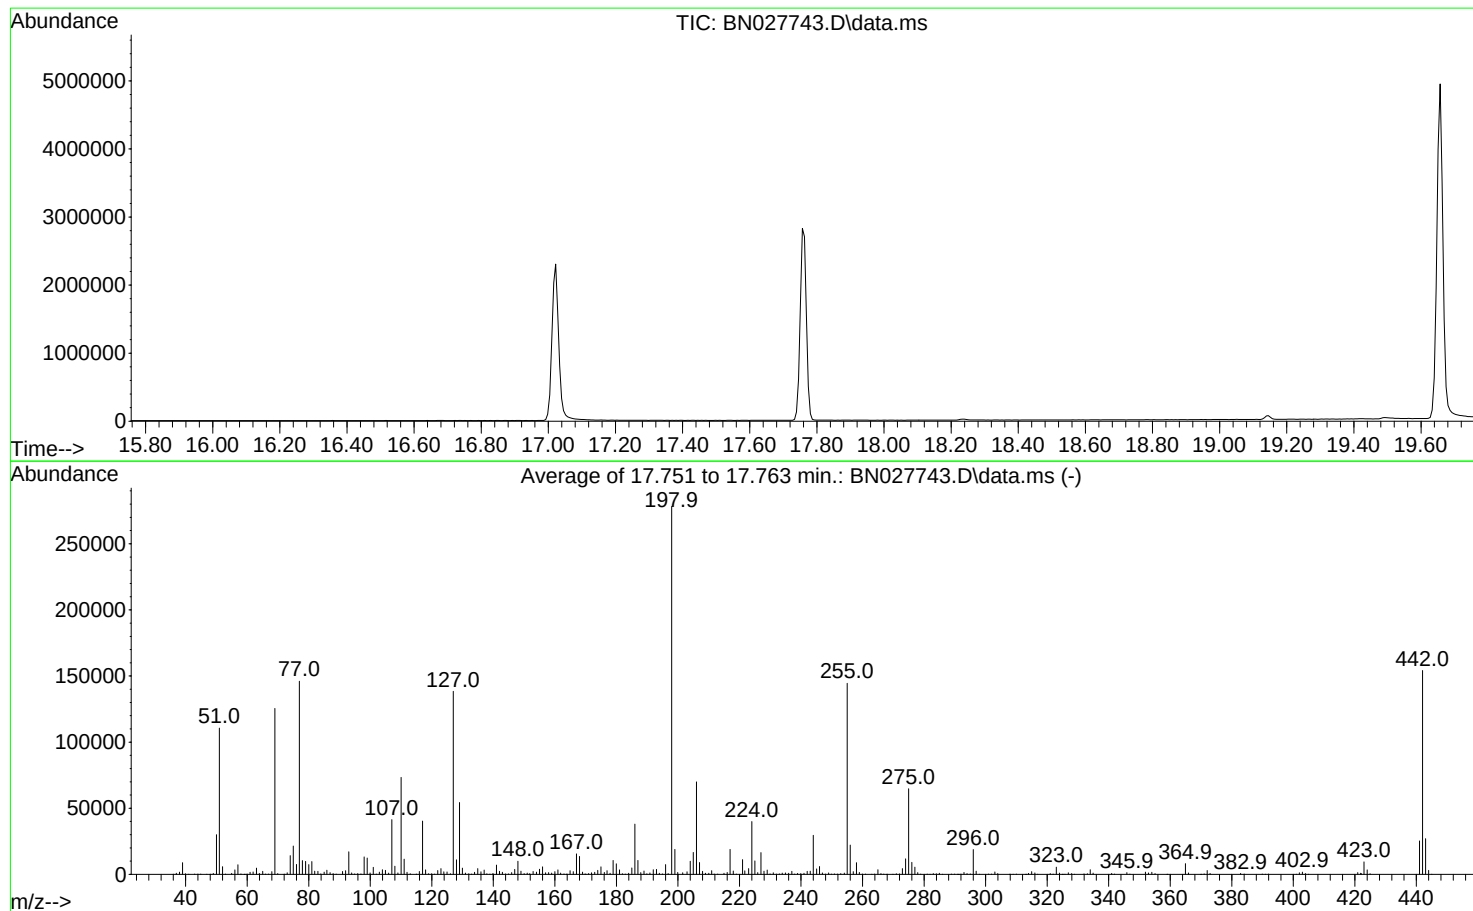




AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2521

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	110578	PASS
68	69	0.00	2	1.7	2111	PASS
69	198	0.00	100	45.1	125512	PASS
70	69	0.00	2	0.5	643	PASS
127	198	10	80	49.7	138400	PASS
197	198	0.00	2	0.2	574	PASS
198	198	100	100	100.0	278208	PASS
199	198	5	9	6.8	18917	PASS
275	198	10	60	23.3	64749	PASS
365	198	1	100	2.9	8172	PASS
441	198	0.01	100	9.1	25343	PASS
442	442	50	100	100.0	154187	PASS
443	442	15	24	17.5	26990	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091923\
Data File : BN027743.D
Acq On : 19 Sep 2023 08:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 20 01:23:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 01:23:52 2023
Response via : Initial Calibration

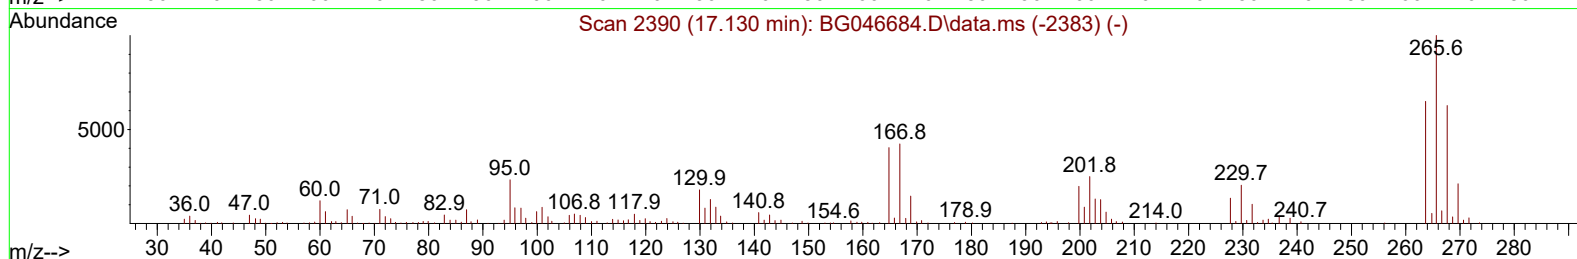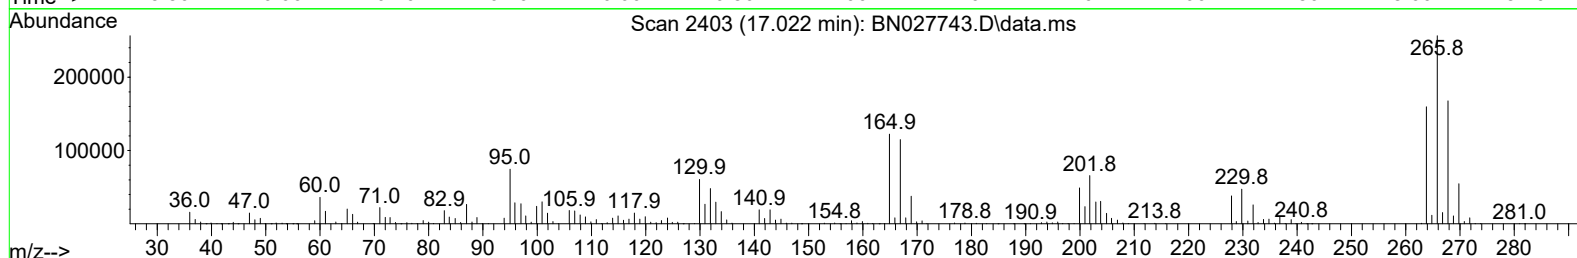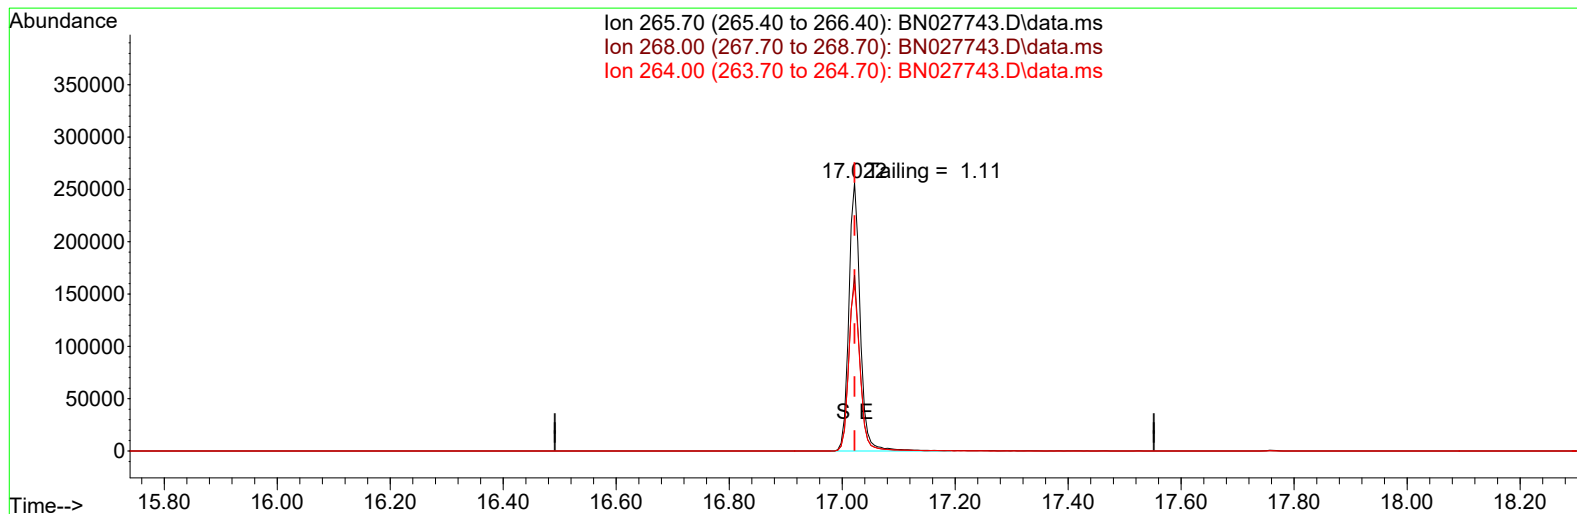

TIC: BN027743.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 23471.22 ng




response 358630

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.41
264.00	61.60	62.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091923\
Data File : BN027743.D
Acq On : 19 Sep 2023 08:38
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 20 01:23:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 20 01:23:52 2023
Response via : Initial Calibration

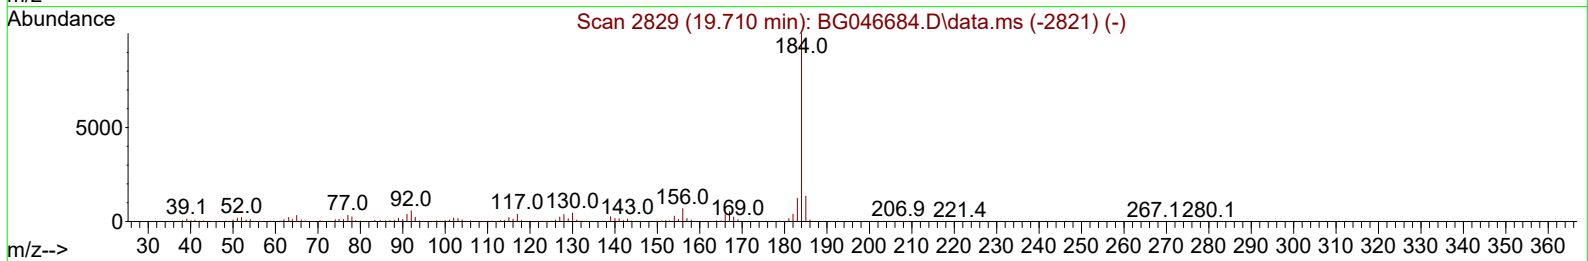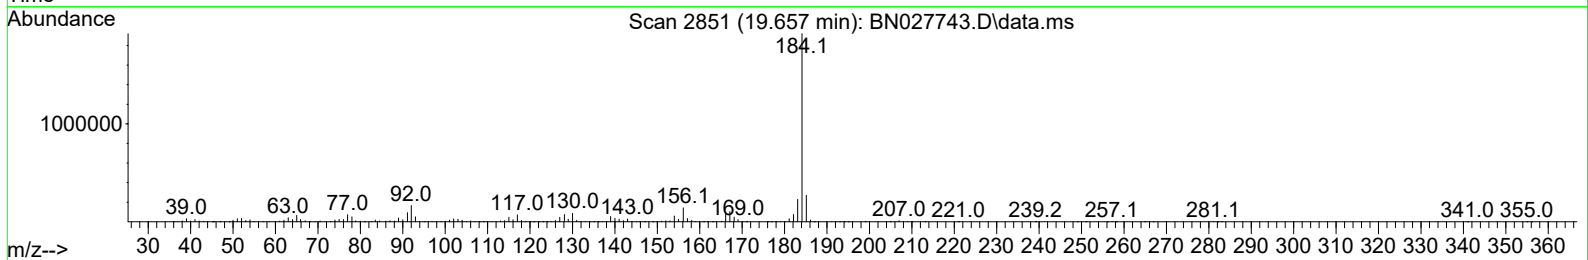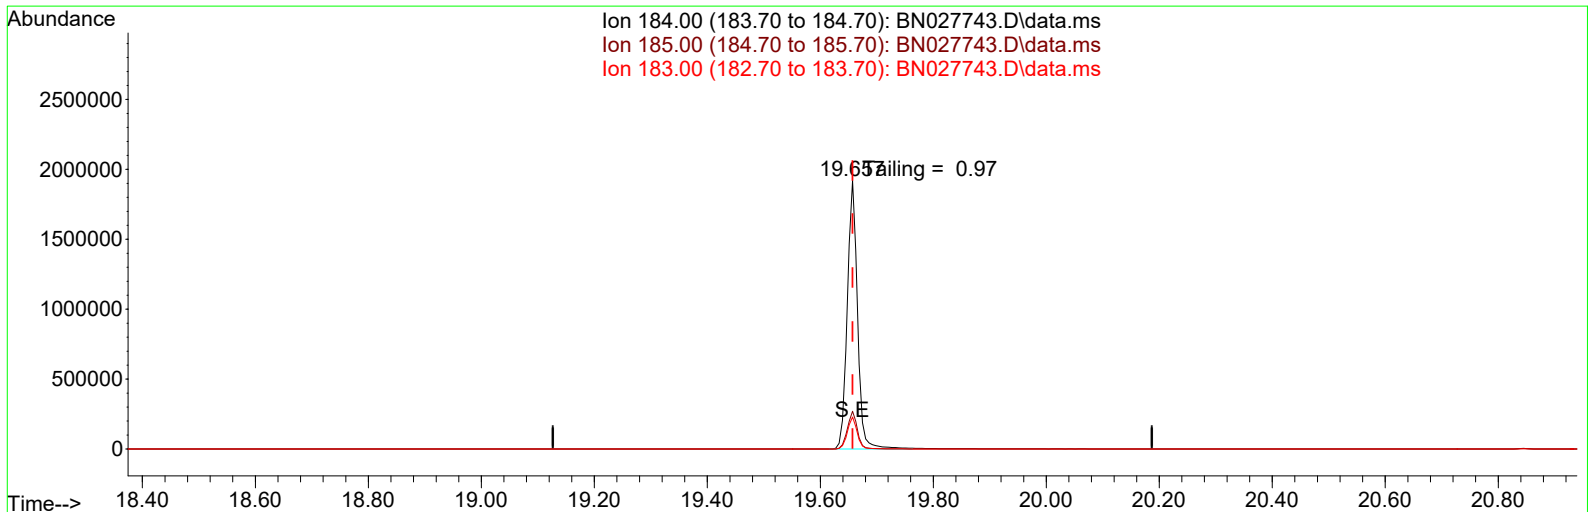

TIC: BN027743.D\data.ms

(77) Benzidine

19.657min (0.000) 0.00 ng

response 2435547

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2023	BNA_N	<u>BN027743.D</u>
Compound Name	Response	Retention Time
DDT	1089772	20.845
DDD	26730	20.41
DDE	1522	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28252	1118024	2.53

Instrument :
BNA_N
ClientSampleId :
DFTPP