
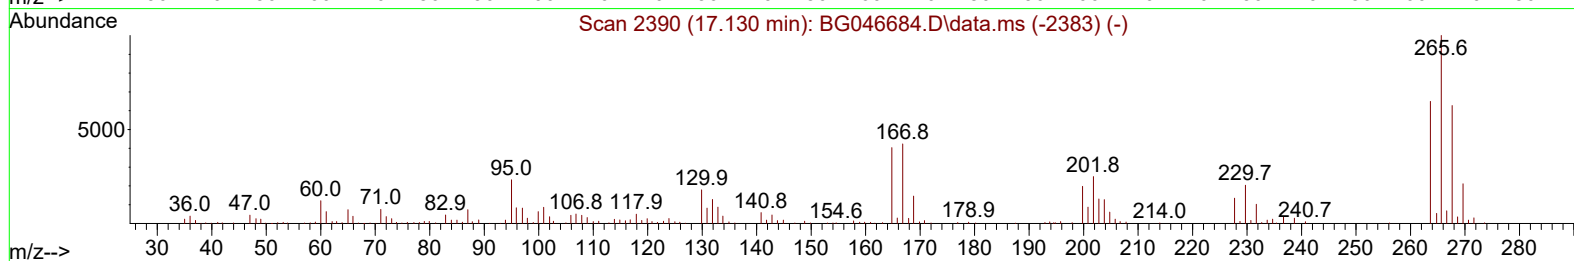
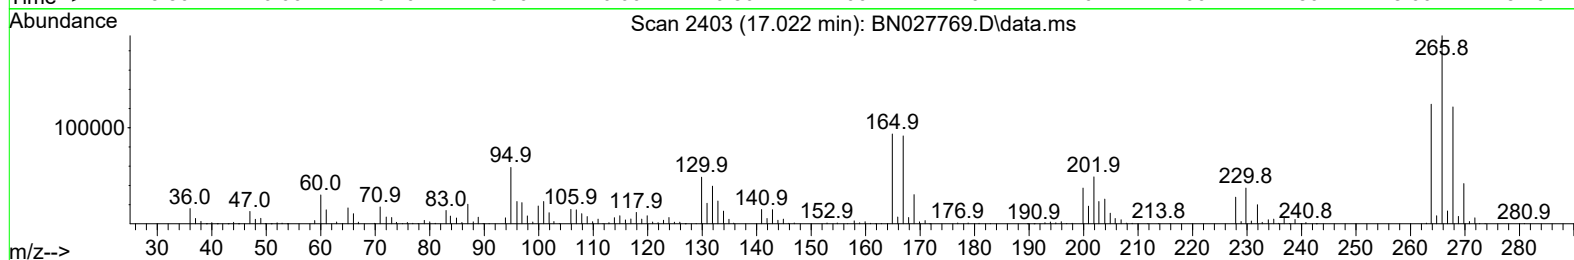


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092023\
Data File : BN027769.D
Acq On : 20 Sep 2023 17:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 05:33:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 21 05:32:06 2023
Response via : Initial Calibration

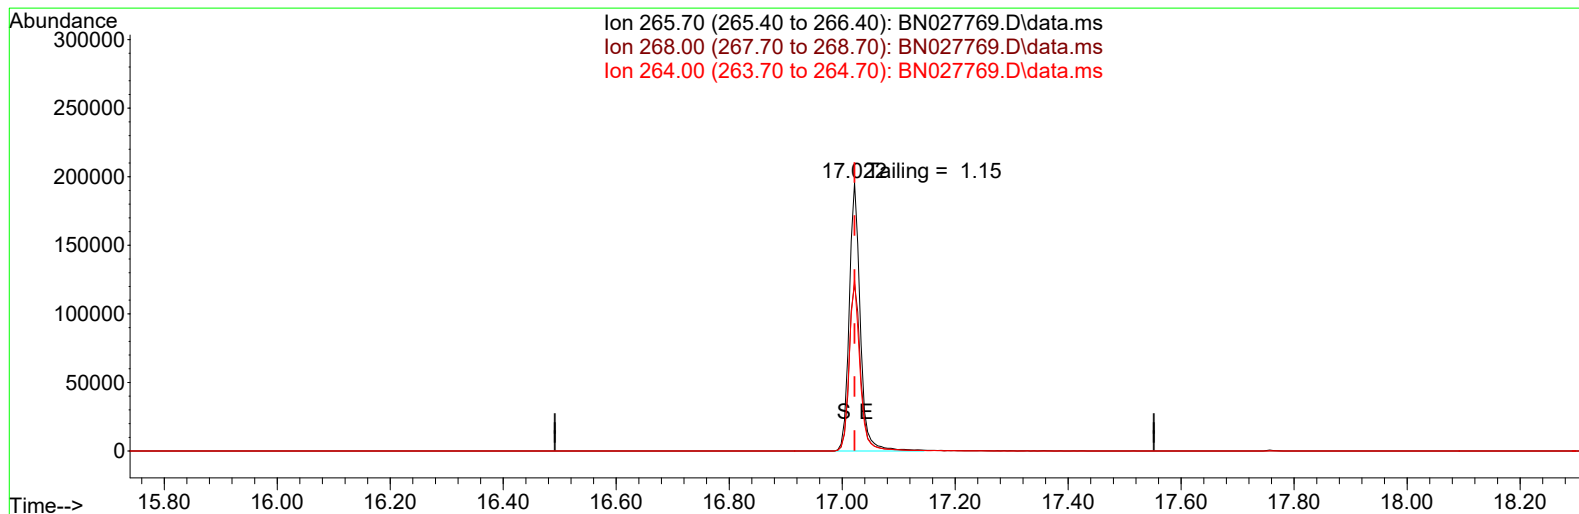

TIC: BN027769.D\data.ms

(70) Pentachlorophenol (C)




17.022min (-0.000) 17801.92 ng

response 267116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.16
264.00	61.60	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092023\
 Data File : BN027769.D
 Acq On : 20 Sep 2023 17:58
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 05:33:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 21 05:32:06 2023
 Response via : Initial Calibration

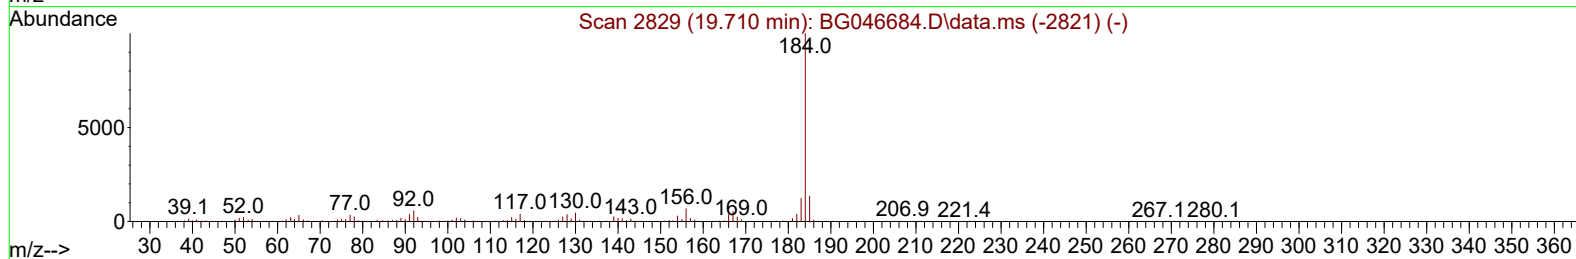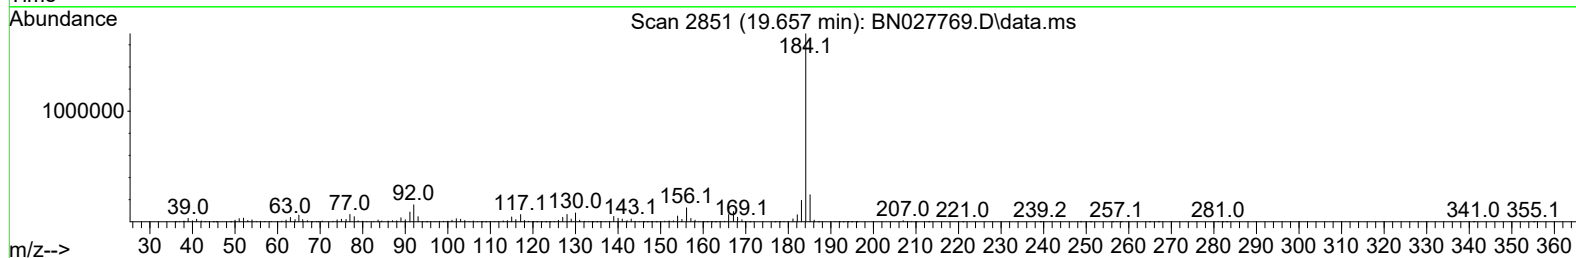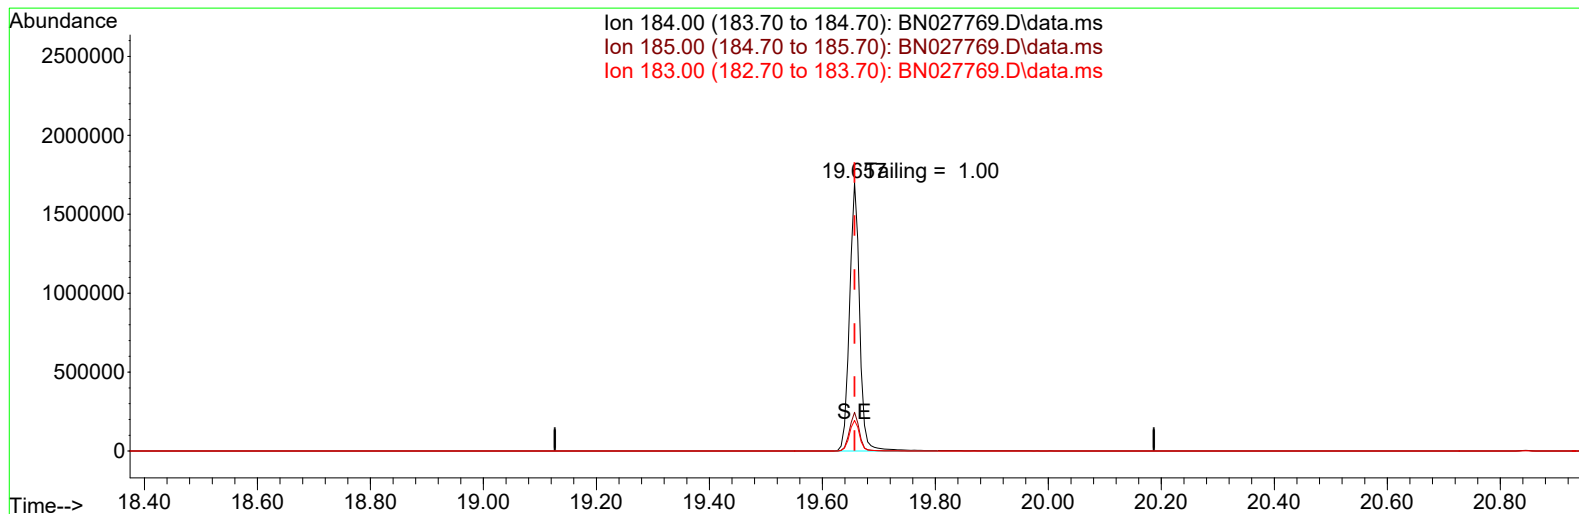

TIC: BN027769.D\data.ms

(77) Benzidine

19.657min (-0.000) 0.00 ng

response 2126800

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	11.39
0.00	0.00	0.00