
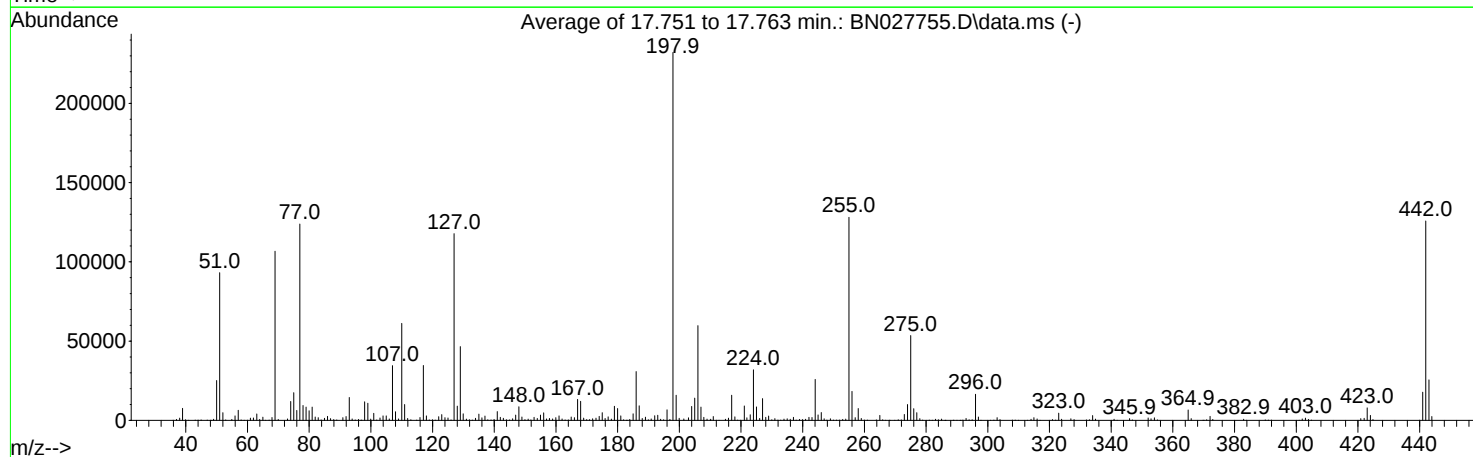


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092023\
Data File : BN027755.D
Acq On : 20 Sep 2023 08:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 20 13:45:42 2023

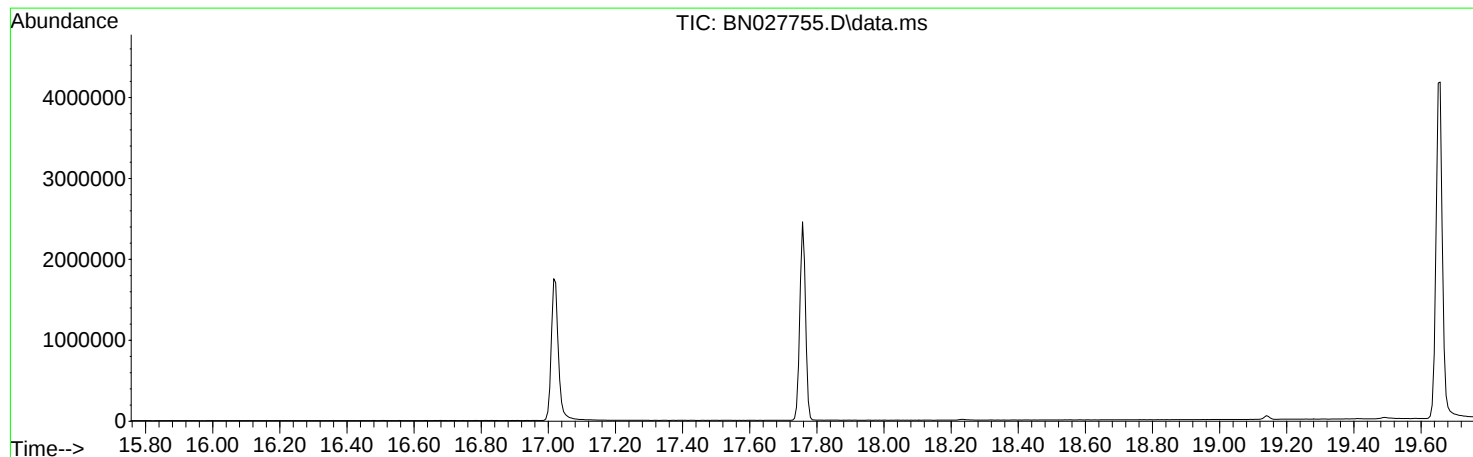




AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	93151	PASS
68	69	0.00	2	1.7	1784	PASS
69	198	0.00	100	46.0	106752	PASS
70	69	0.00	2	0.5	567	PASS
127	198	10	80	50.8	117853	PASS
197	198	0.00	2	0.3	592	PASS
198	198	100	100	100.0	232085	PASS
199	198	5	9	6.8	15832	PASS
275	198	10	60	23.1	53536	PASS
365	198	1	100	2.8	6589	PASS
441	198	0.01	100	7.6	17741	PASS
442	442	50	100	100.0	125787	PASS
443	442	15	24	20.3	25562	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092023\
 Data File : BN027755.D
 Acq On : 20 Sep 2023 08:15
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 21 05:32:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 21 05:32:06 2023
 Response via : Initial Calibration

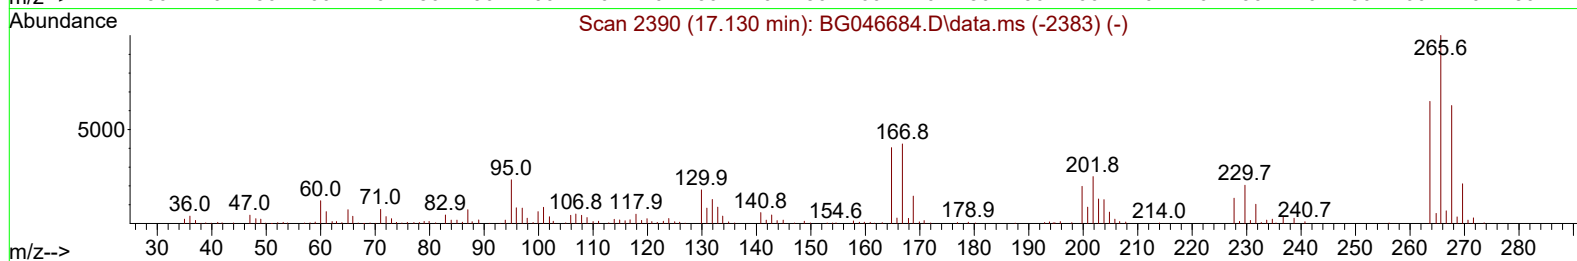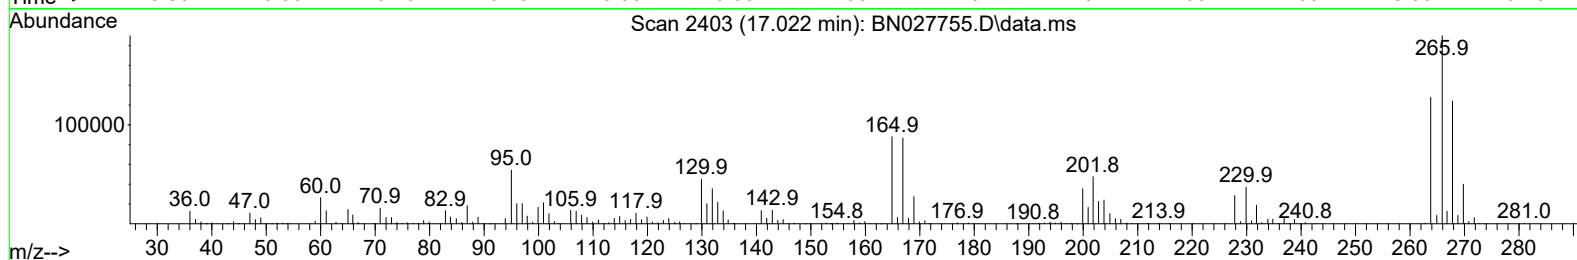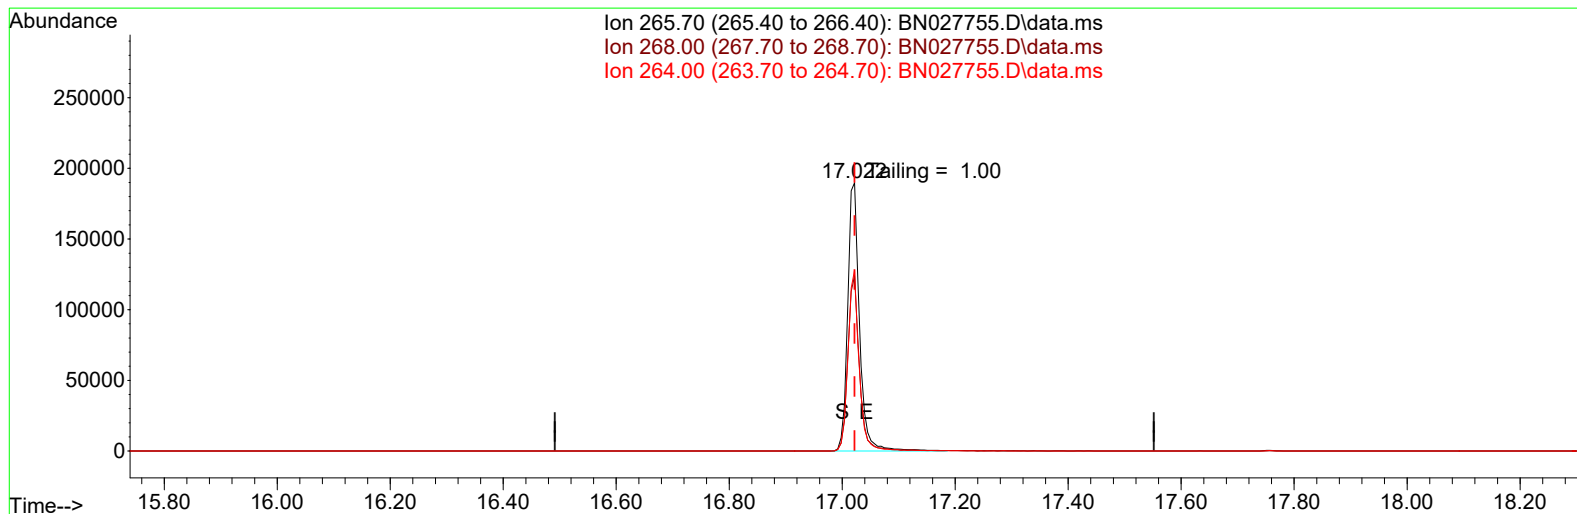

TIC: BN027755.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 21334.23 ng




response 278094

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.31
264.00	61.60	67.35
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092023\  
Data File : BN027755.D  
Acq On    : 20 Sep 2023  08:15  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 21 05:32:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 21 05:32:06 2023
Response via : Initial Calibration

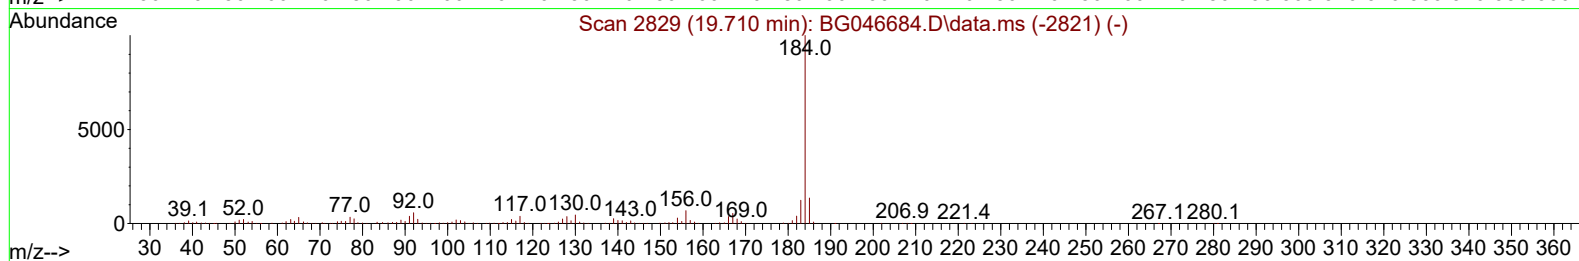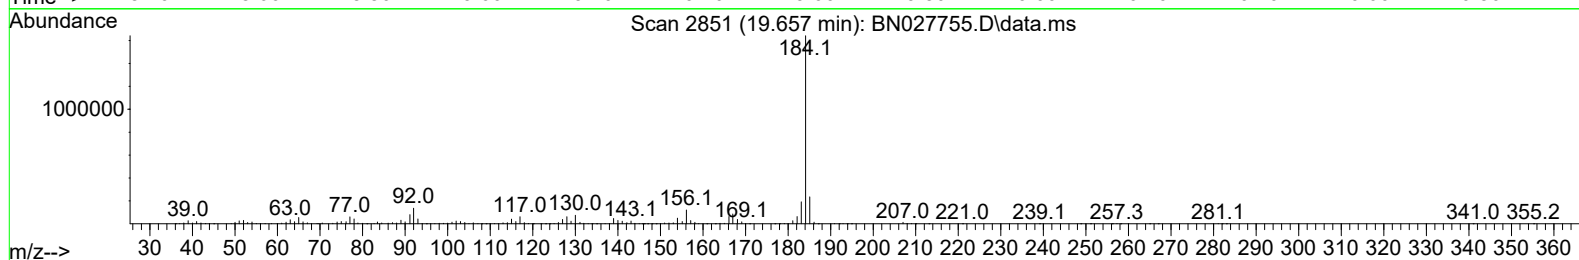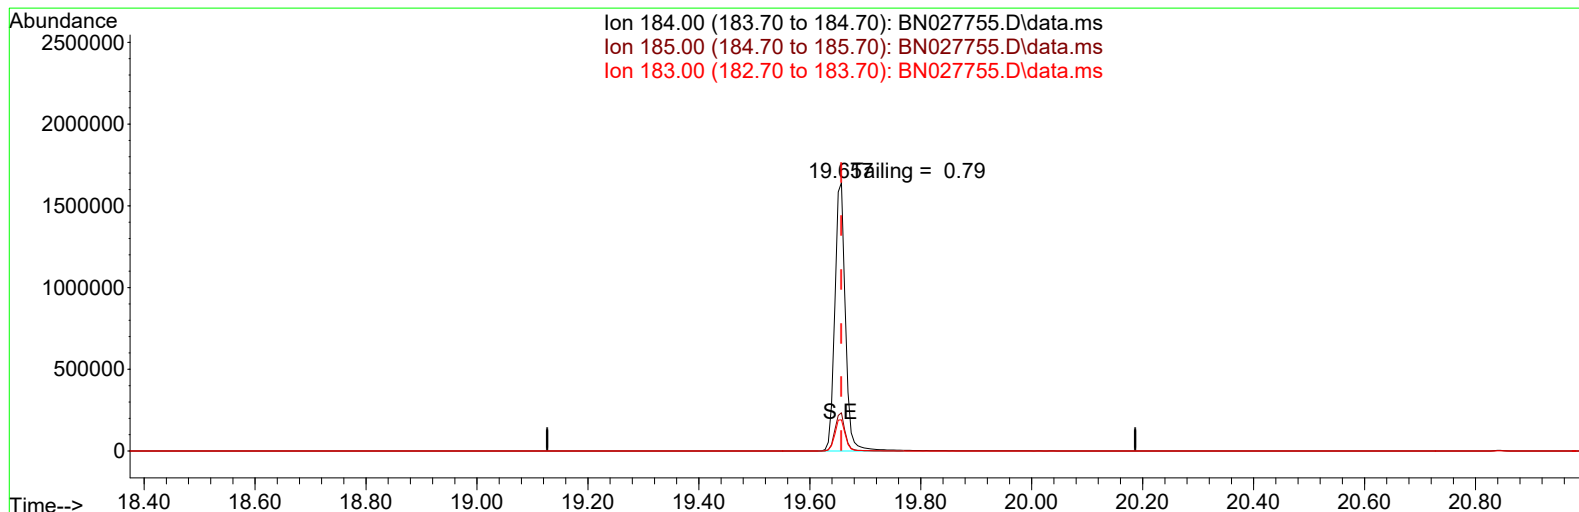

TIC: BN027755.D\data.ms

(77) Benzidine

19.657min (0.000) 0.00 ng

response **2189983**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.27
183.00	13.20	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2023	BNA_N	<u>BN027755.D</u>
Compound Name	Response	Retention Time
DDT	909309	20.845
DDD	19658	20.41
DDE	1326	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20984	930293	2.26

Instrument :
BNA_N
ClientSampleId :
DFTPP