


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092023\
Data File : BN027769.D
Acq On : 20 Sep 2023 17:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 20 13:45:42 2023

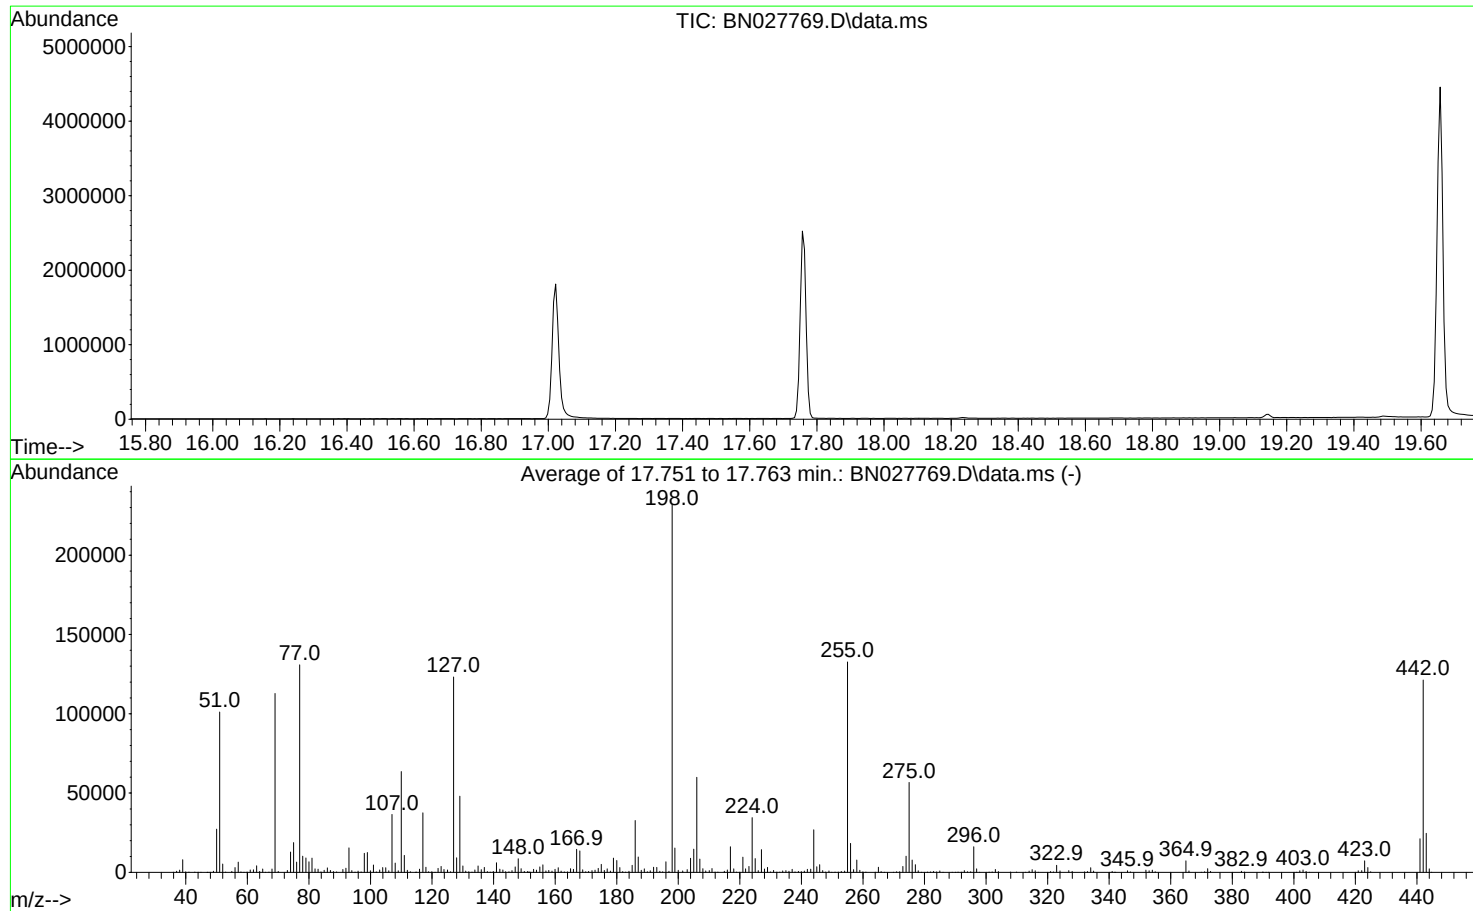




AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2521

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	101091	PASS
68	69	0.00	2	1.9	2136	PASS
69	198	0.00	100	48.6	112787	PASS
70	69	0.00	2	0.6	662	PASS
127	198	10	80	53.1	123171	PASS
197	198	0.00	2	0.3	743	PASS
198	198	100	100	100.0	231936	PASS
199	198	5	9	6.6	15312	PASS
275	198	10	60	24.4	56691	PASS
365	198	1	100	3.1	7269	PASS
441	198	0.01	100	9.1	21157	PASS
442	442	50	100	100.0	121216	PASS
443	442	15	24	20.4	24670	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092023\
 Data File : BN027769.D
 Acq On : 20 Sep 2023 17:58
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 21 05:33:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 21 05:32:06 2023
 Response via : Initial Calibration

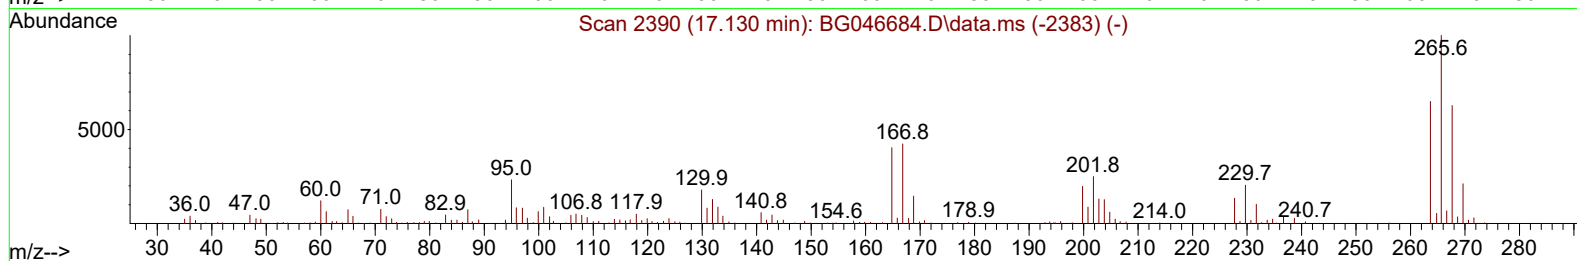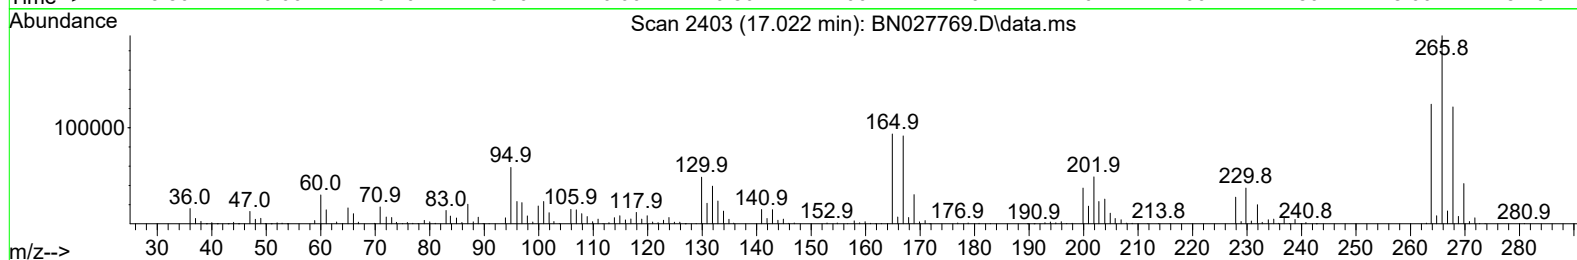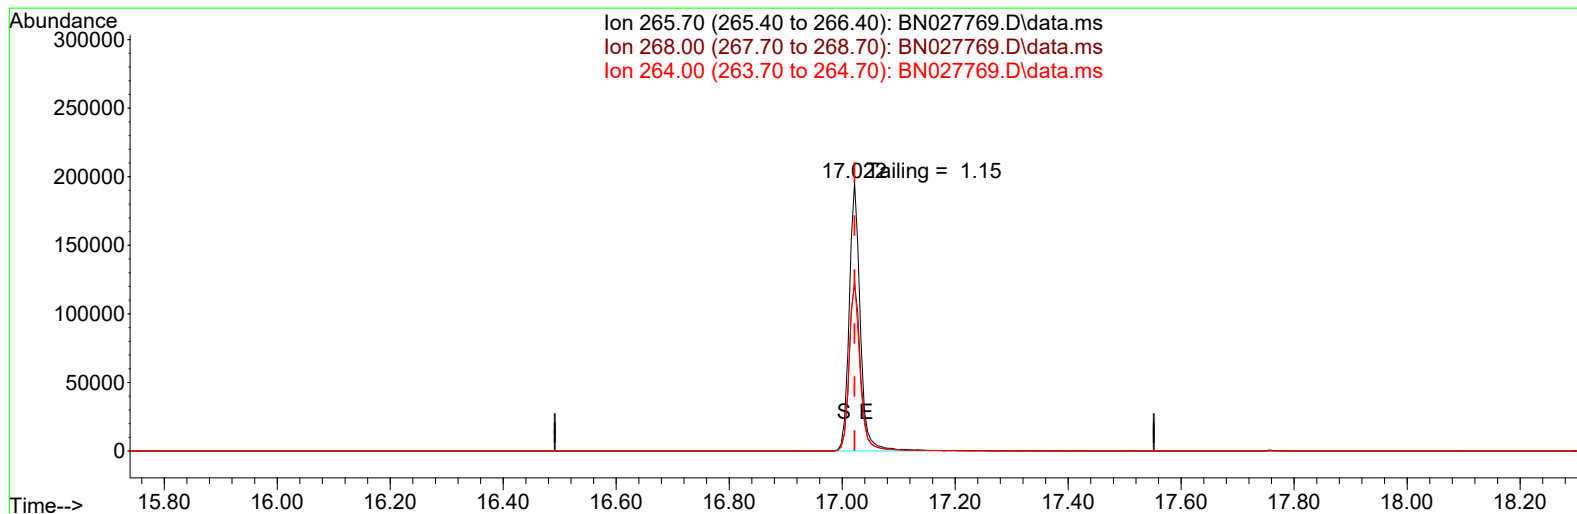

TIC: BN027769.D\data.ms

(70) Pentachlorophenol (C)

17.022min (-0.000) 17801.92 ng




response 267116

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.16
264.00	61.60	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092023\
Data File : BN027769.D
Acq On : 20 Sep 2023 17:58
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 21 05:33:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 21 05:32:06 2023
Response via : Initial Calibration

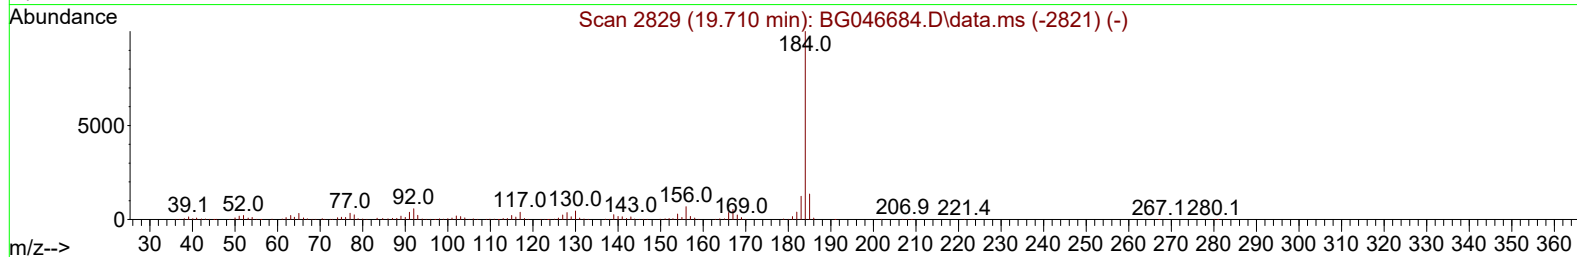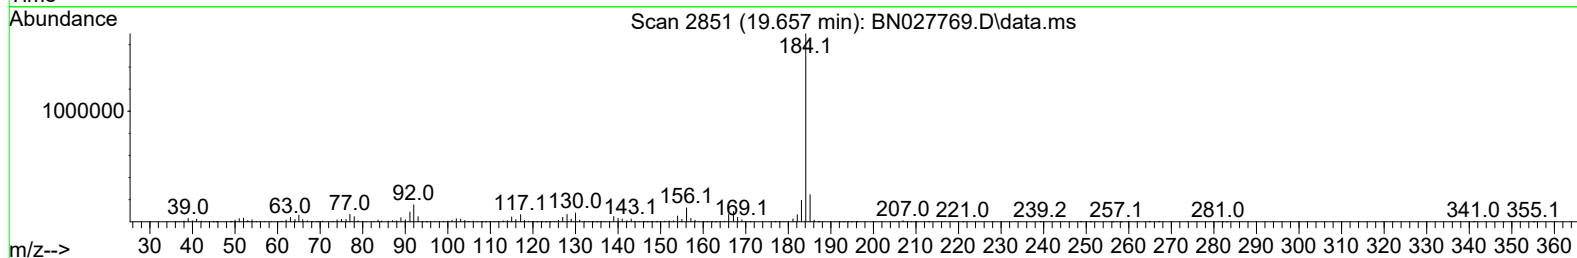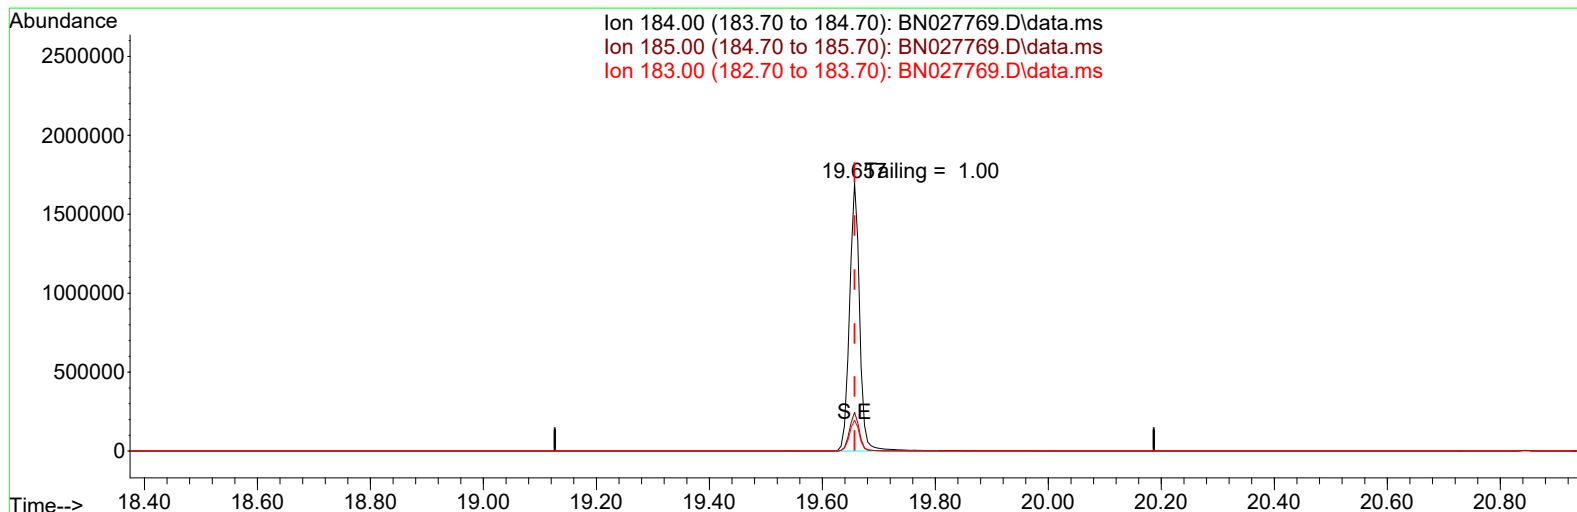

TIC: BN027769.D\data.ms

(77) Benzidine

19.657min (-0.000) 0.00 ng

response 2126800

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	11.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2023	BNA_N	<u>BN027769.D</u>
Compound Name	Response	Retention Time
DDT	952437	20.845
DDD	15369	20.41
DDE	1014	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16383	968820	1.69

Instrument :
BNA_N
ClientSampleId :
DFTPP