
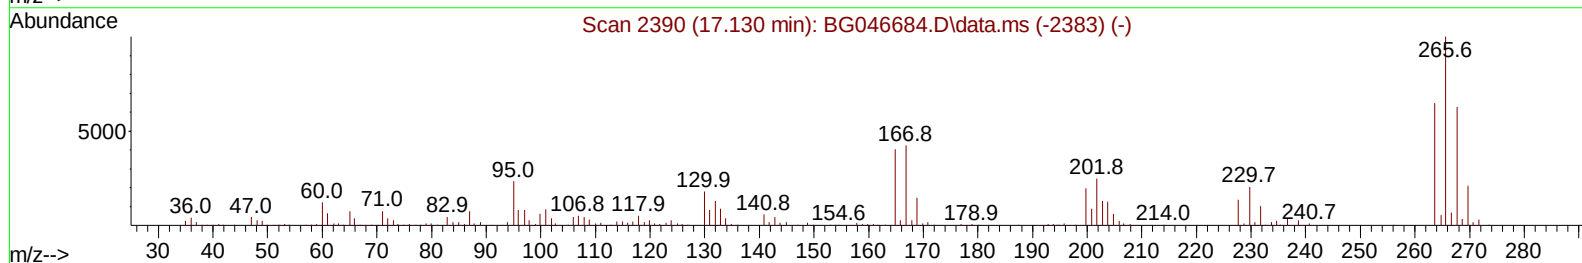
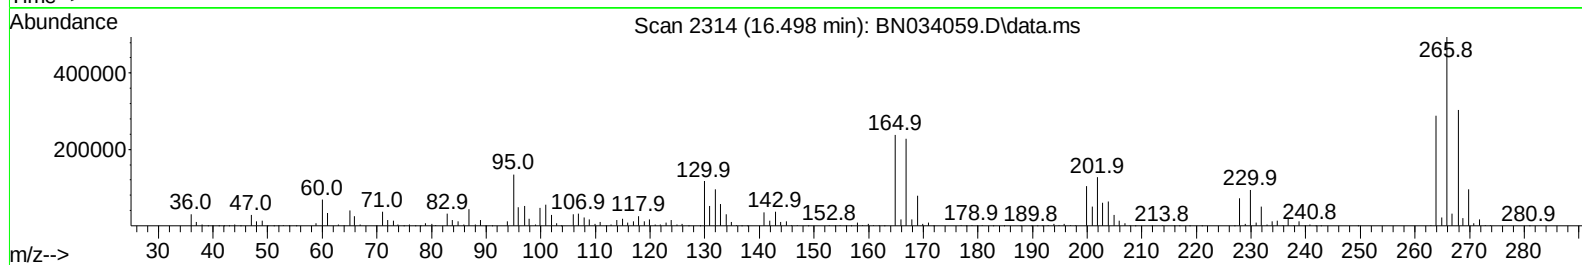


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092024\
Data File : BN034059.D
Acq On : 19 Sep 2024 21:20
Operator : JU/RC
Sample : DFTTP
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Sep 20 04:54:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 04:53:44 2024
Response via : Initial Calibration

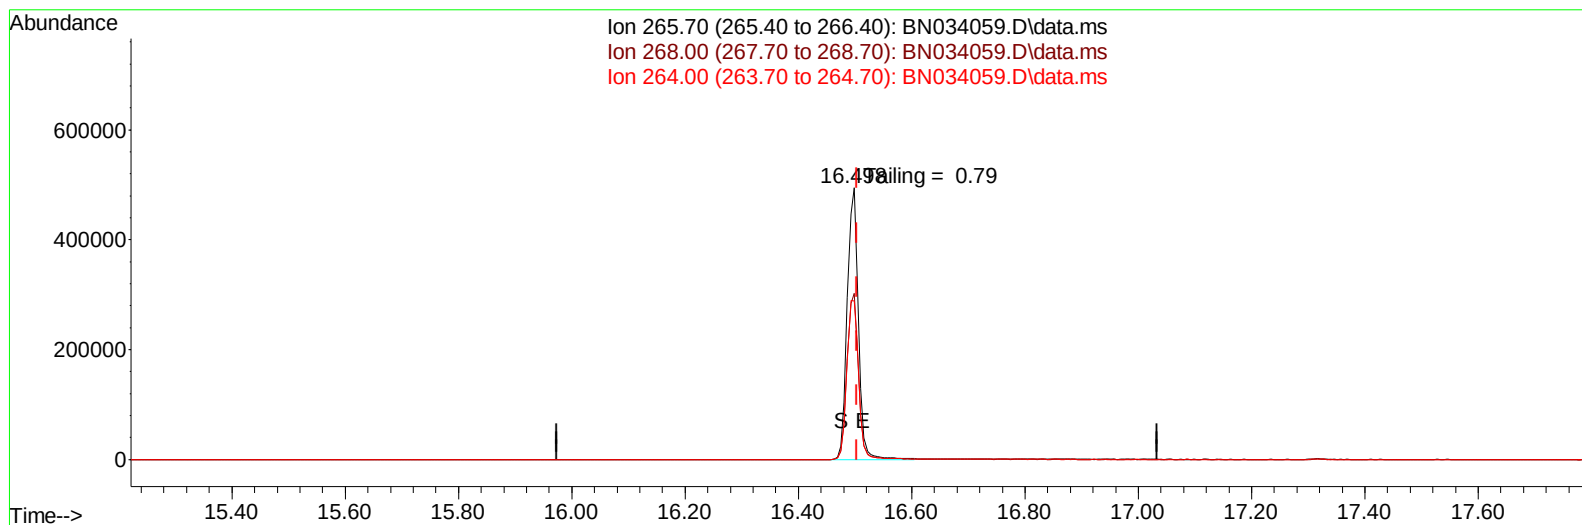

TIC: BN034059.D\data.ms

(70) Pentachlorophenol (C)




16.498min (-0.006) 23990.92 ng

response 679860

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.27
264.00	61.60	58.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092024\
Data File : BN034059.D
Acq On : 19 Sep 2024 21:20
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Sep 20 04:54:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 04:53:44 2024
Response via : Initial Calibration

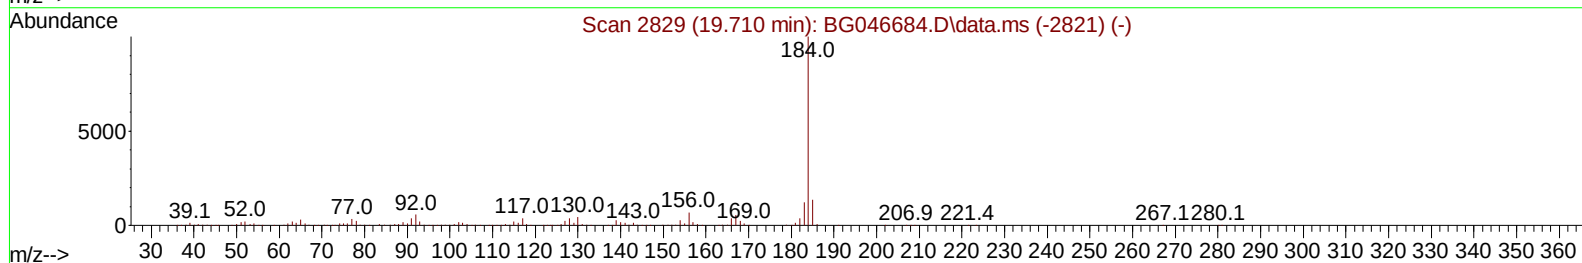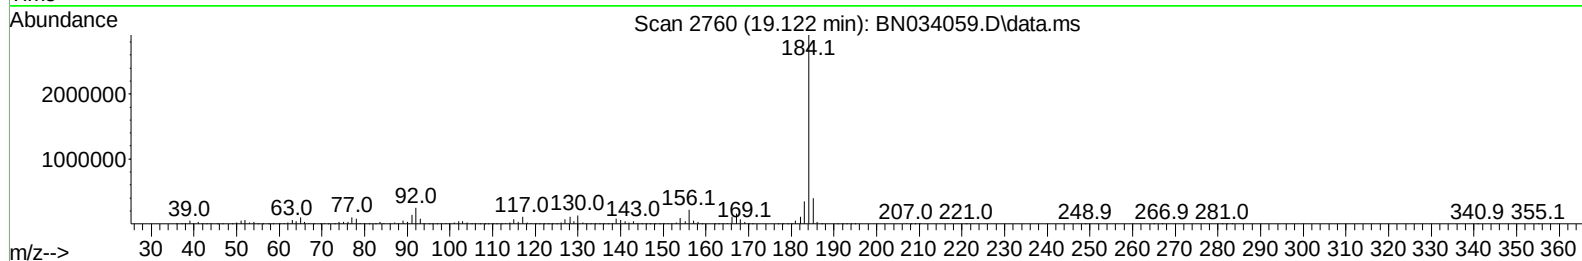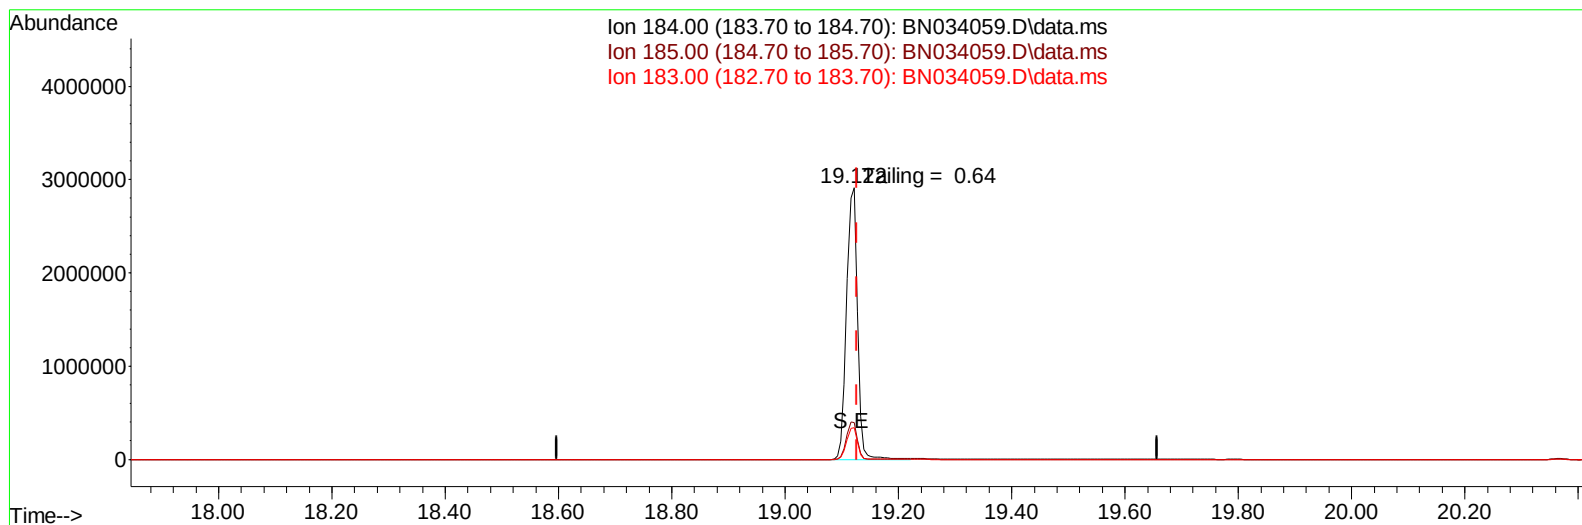

TIC: BN034059.D\data.ms

(77) Benzidine**19.122min (-0.006) 0.00 ng****response 3954728**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.66
183.00	13.20	11.76
0.00	0.00	0.00