
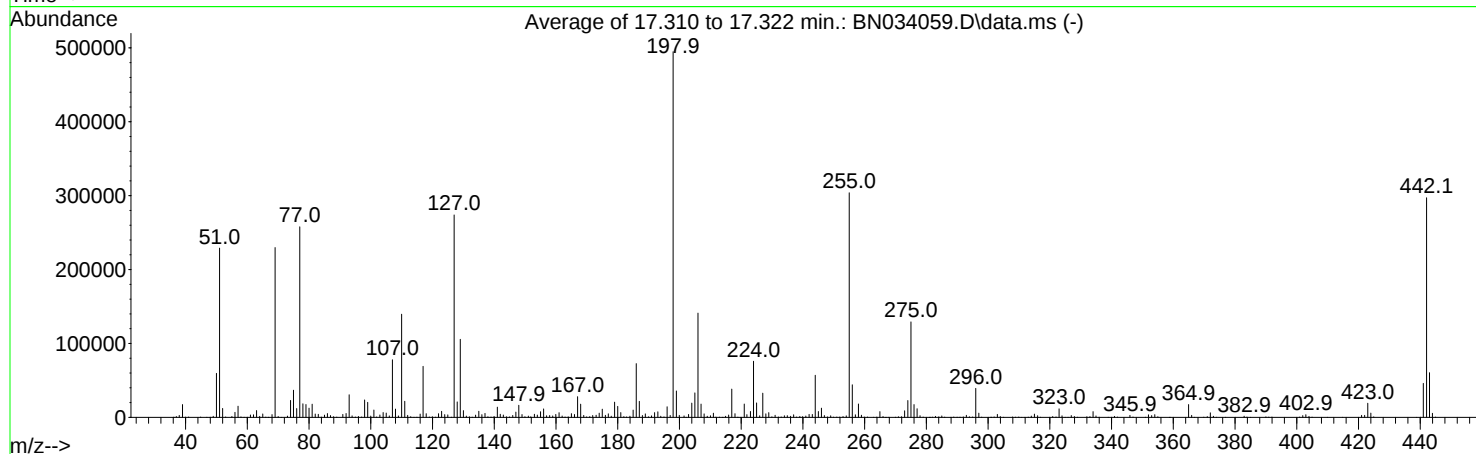


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092024\
Data File : BN034059.D
Acq On : 19 Sep 2024 21:20
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 18 16:09:28 2024

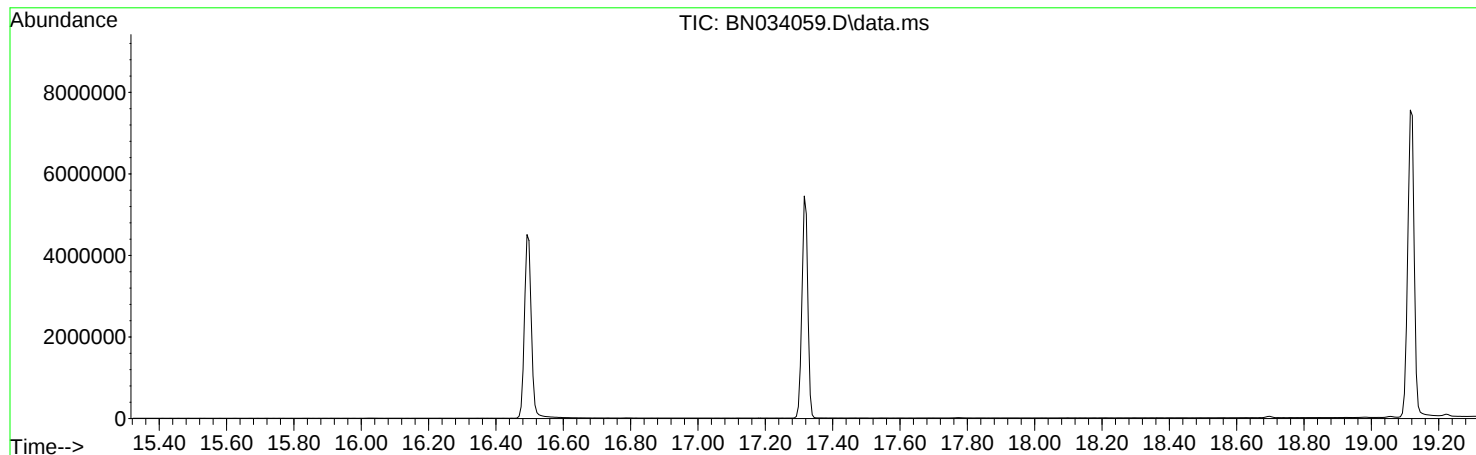




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	229025	PASS
68	69	0.00	2	1.6	3753	PASS
69	198	0.00	100	46.4	229803	PASS
70	69	0.00	2	0.5	1180	PASS
127	198	10	80	55.4	273899	PASS
197	198	0.00	2	0.5	2617	PASS
198	198	100	100	100.0	494805	PASS
199	198	5	9	7.2	35739	PASS
275	198	10	60	26.1	129195	PASS
365	198	1	100	3.5	17371	PASS
441	198	0.01	100	9.3	46013	PASS
442	442	50	100	100.0	297173	PASS
443	442	15	24	20.3	60448	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092024\
Data File : BN034059.D
Acq On : 19 Sep 2024 21:20
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 20 04:54:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 04:53:44 2024
Response via : Initial Calibration

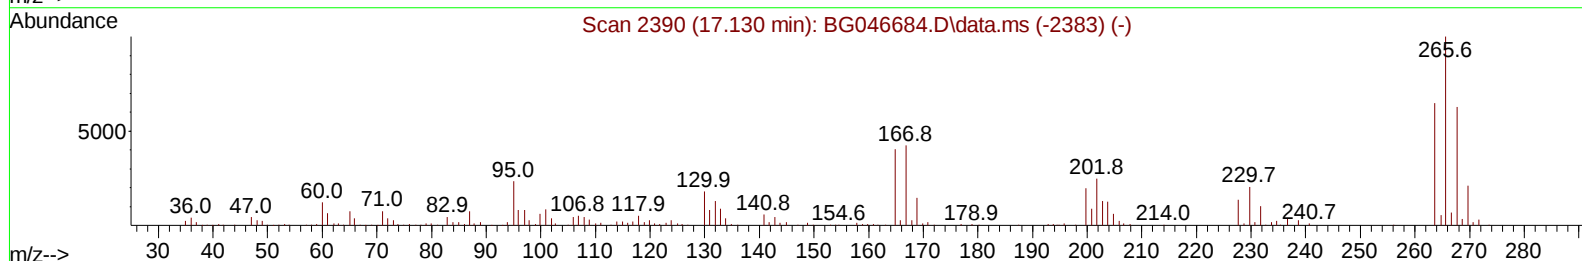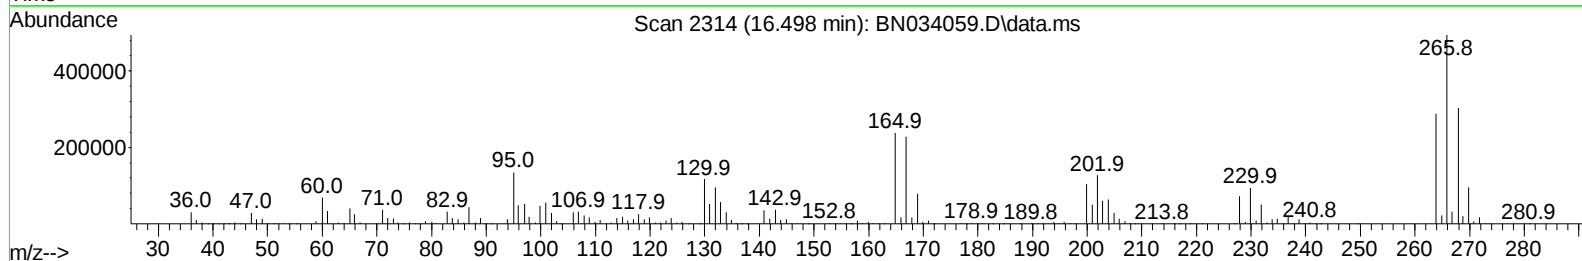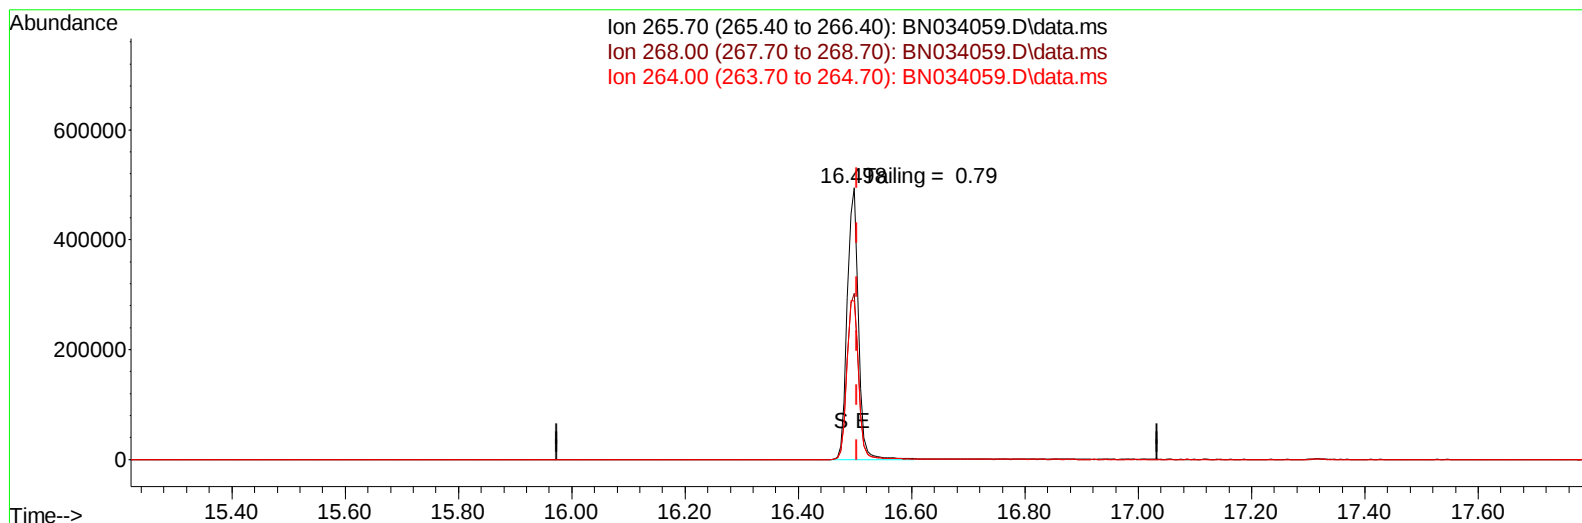

TIC: BN034059.D\data.ms

(70) Pentachlorophenol (C)

16.498min (-0.006) 23990.92 ng




response 679860

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.27
264.00	61.60	58.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092024\
Data File : BN034059.D
Acq On : 19 Sep 2024 21:20
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 20 04:54:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 04:53:44 2024
Response via : Initial Calibration

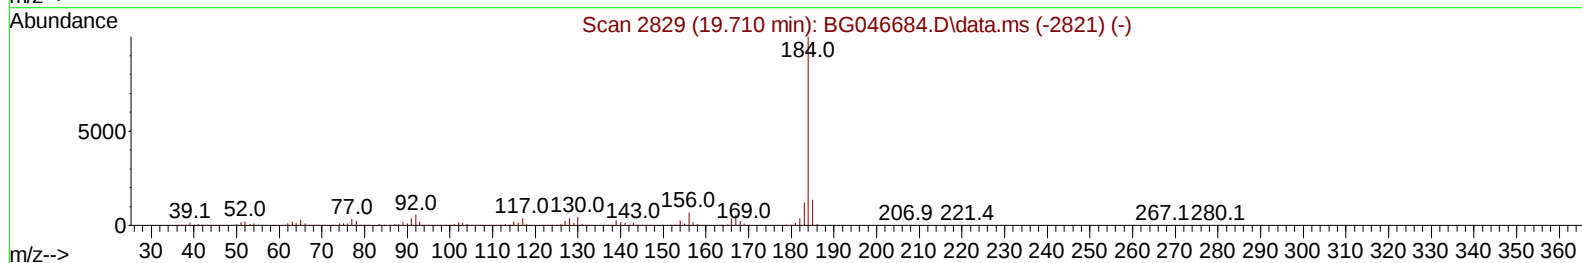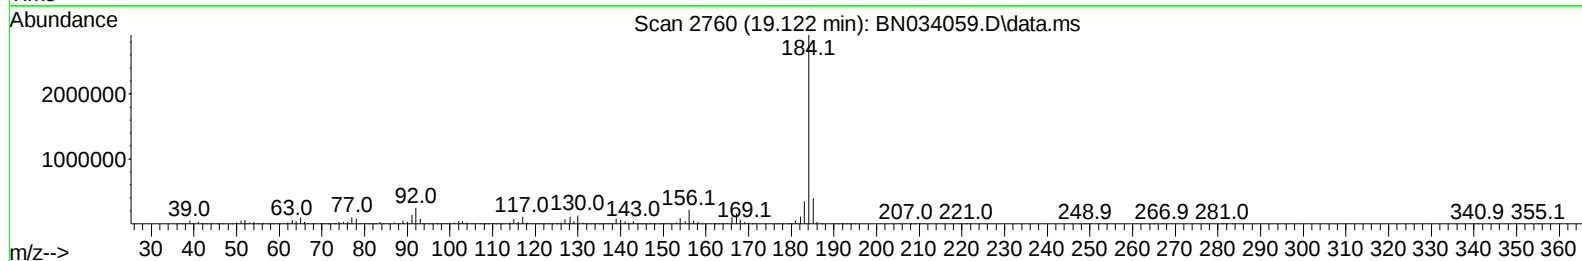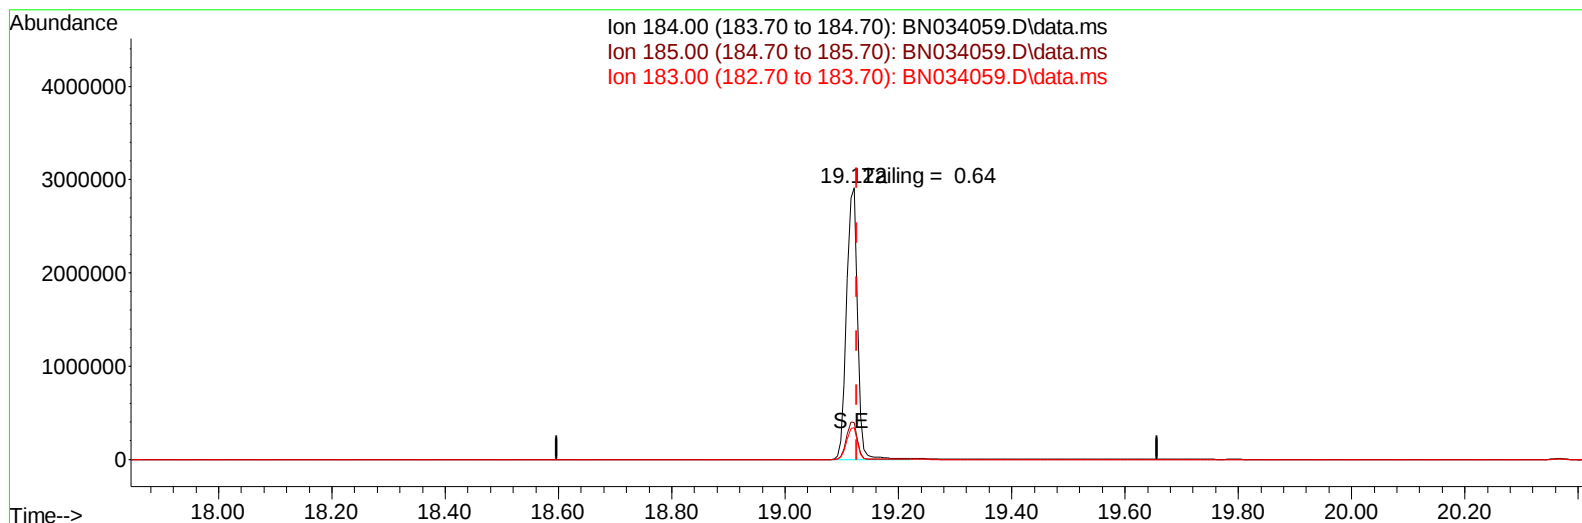

TIC: BN034059.D\data.ms

(77) Benzidine

19.122min (-0.006) 0.00 ng

response 3954728

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.66
183.00	13.20	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2024	BNA_N	<u>BN034059.D</u>
Compound Name	Response	Retention Time
DDT	1931147	20.369
DDD	16380	19.975
DDE	182	19.41
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16562	1947709	0.85

Instrument :
BNA_N
ClientSampleId :
DFTPP