
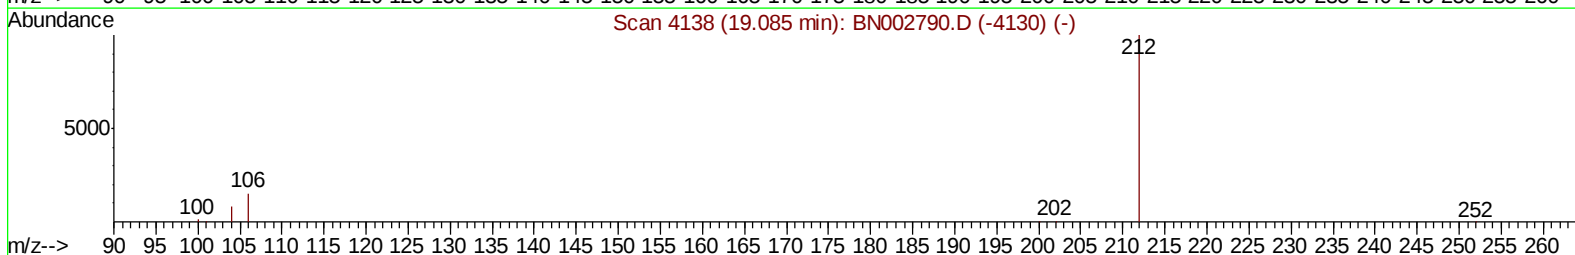
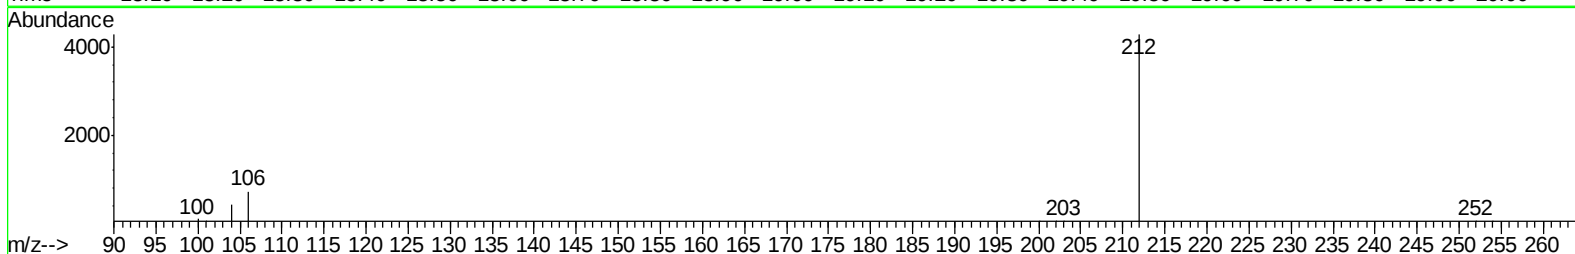


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
Data File : BN002806.D
Acq On : 21 Sep 2018 02:43
Operator : JU/SJ
Sample : PB112889BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Sep 21 05:29:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 04:00:39 2018
Response via : Initial Calibration

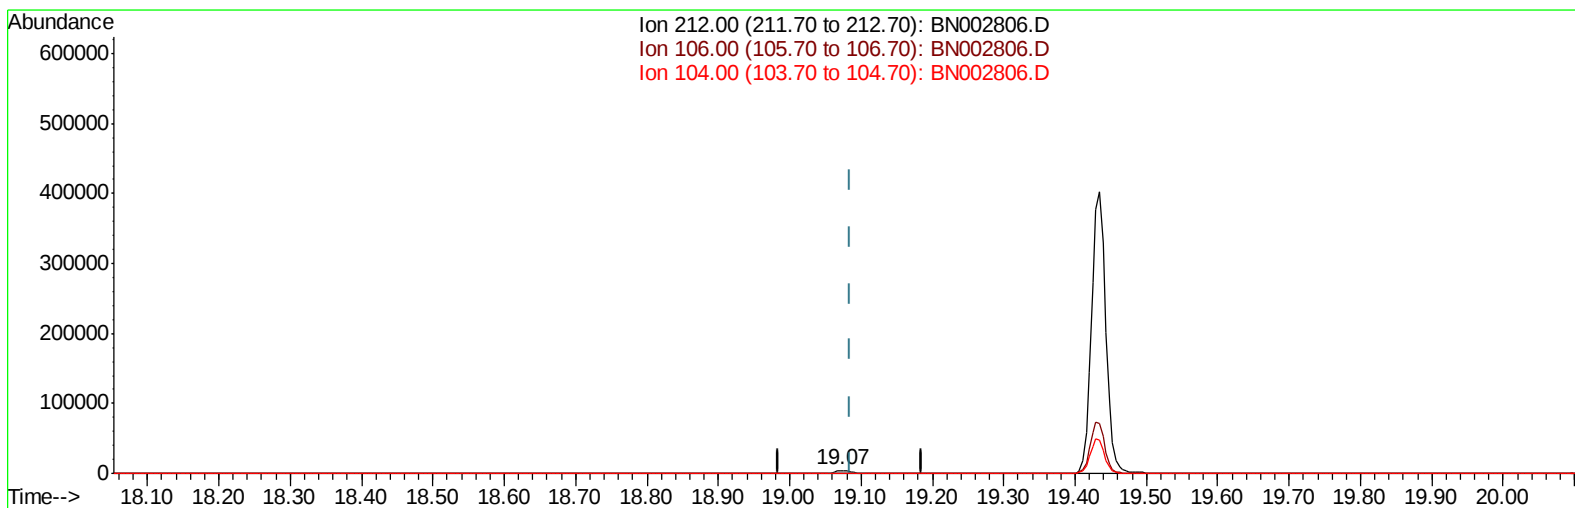

TIC: BN002806.D

(14) Fluoranthene-d10 (SURR)

19.072min (-0.014) 0.37ng/ul m

response 6136

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00