

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
 Data File : BN002806.D
 Acq On : 21 Sep 2018 02:43
 Operator : JU/SJ
 Sample : PB112889BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK89

Quant Time: Sep 21 05:27:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 04:00:39 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	1650	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.42	136	6346	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	3336	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.13	188	545292	0.40	ng/ul	0.08
16) Chrysene-d12	21.26	240	3987	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	6407	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	3579	0.39	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.43	202	795	0.061	ng/ul#	1
23) Benzo(a)pyrene	23.31	252	1847	0.091	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
Data File : BN002806.D
Acq On : 21 Sep 2018 02:43
Operator : JU/SJ
Sample : PB112889BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK89

Quant Time: Sep 21 05:27:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 04:00:39 2018
Response via : Initial Calibration




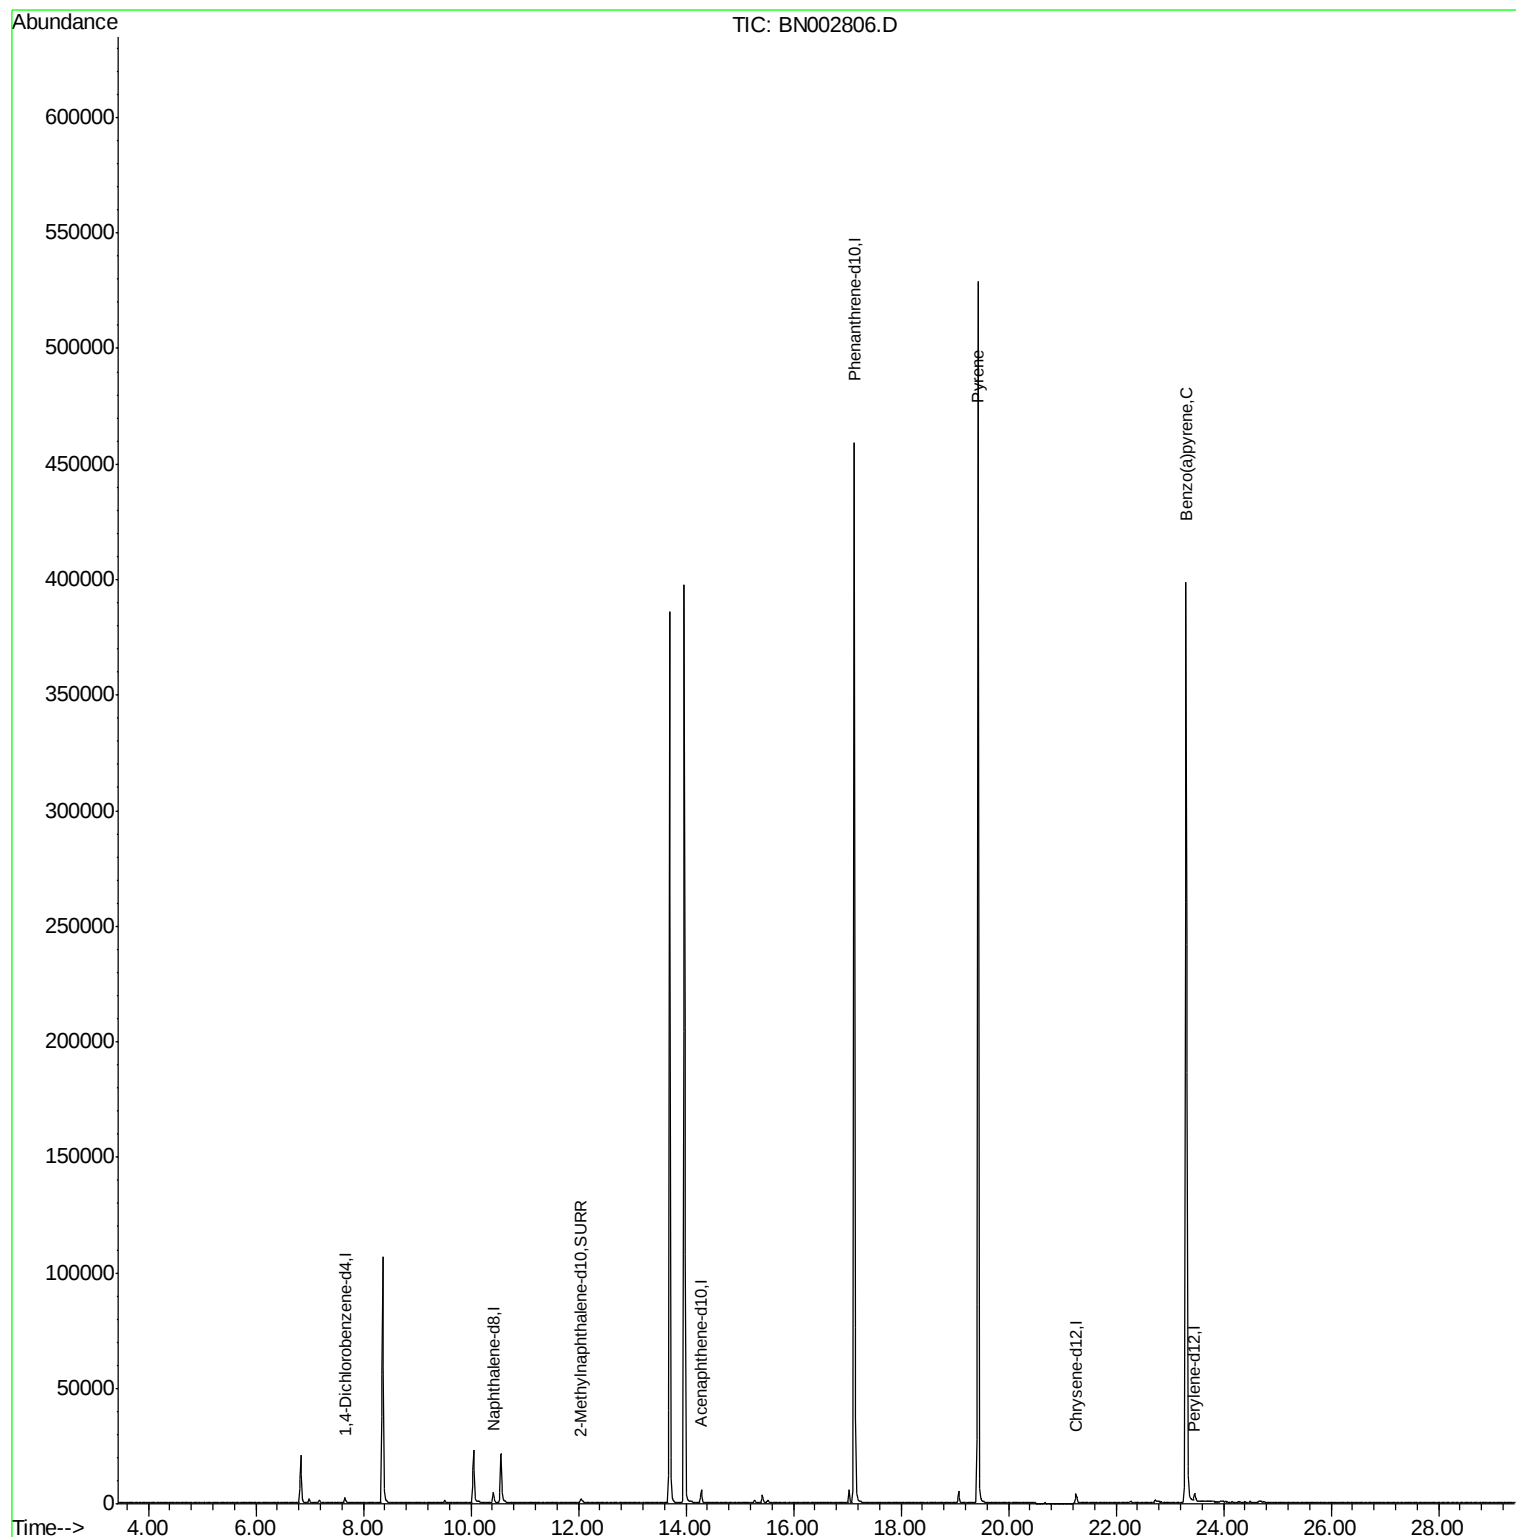


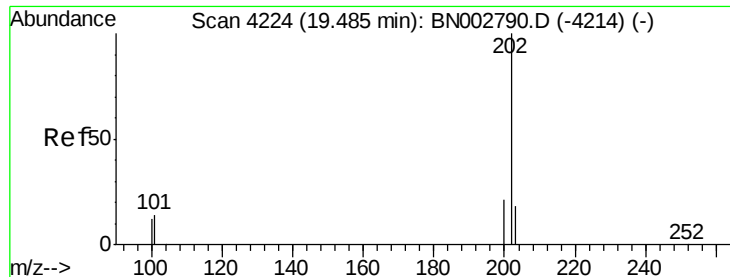

#17
Pyrene
Concen: 0.061 ng/ul
RT: 19.43 min Scan# 4213
Delta R.T. -0.05 min
Lab File: BN002806.D
Acq: 21 Sep 2018 02:43

Instrument :
BNA_N
ClientSampleId :
SBLK89

Tgt Ion:202 Resp: 795
Ion Ratio Lower Upper
202 100
101 138.2 12.0 18.0#
100 878.4 8.0 12.0#

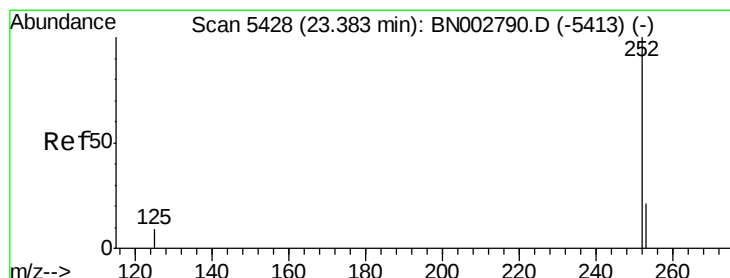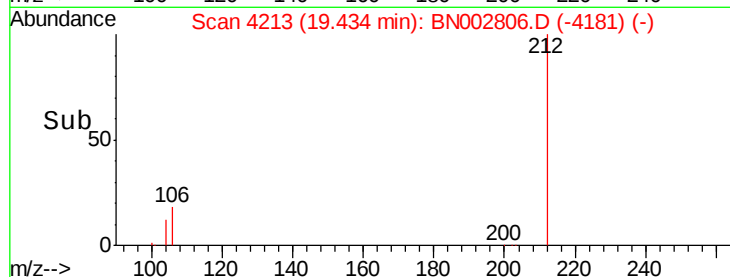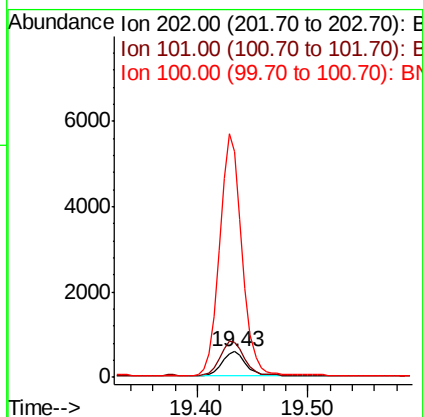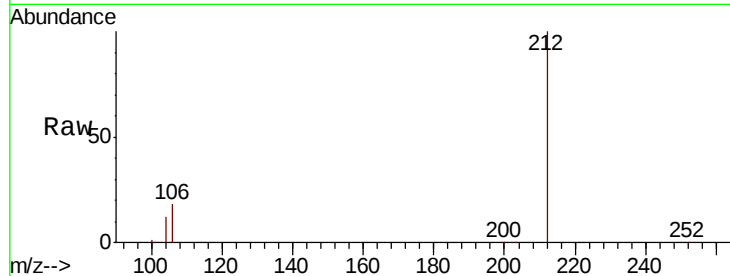

#23
Benzo(a)pyrene
Concen: 0.091 ng/ul
RT: 23.31 min Scan# 5402
Delta R.T. -0.08 min
Lab File: BN002806.D
Acq: 21 Sep 2018 02:43

Tgt Ion:252 Resp: 1847
Ion Ratio Lower Upper
252 100
253 40.1 16.0 24.0#
125 34.6 12.0 18.0#

