


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
Data File : BN002791.D
Acq On : 20 Sep 2018 17:58
Operator : JU/SJ
Sample : PB112991BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK91

Manual Integrations
APPROVED

Sohil
9/21/2018 2:06:04 PM

Quant Time: Sep 21 04:14:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 04:00:39 2018
Response via : Initial Calibration

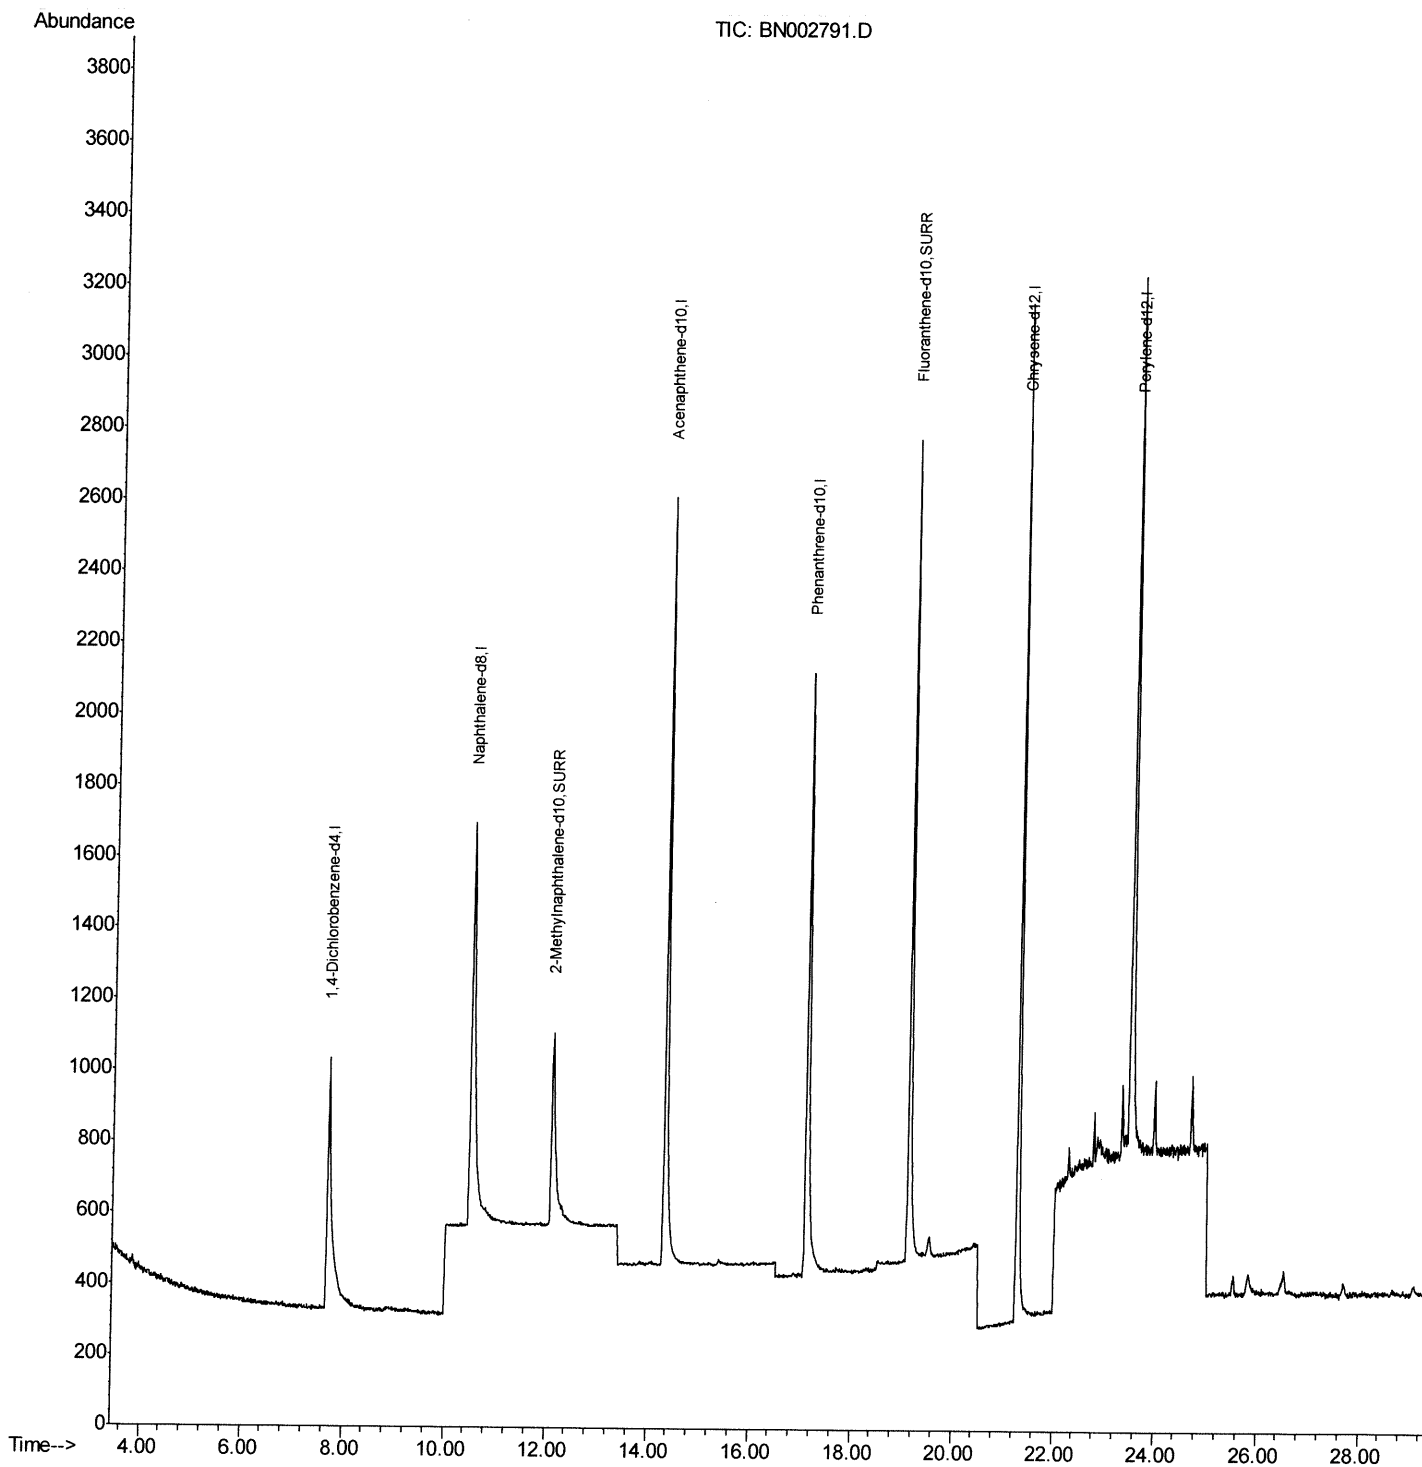

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
Data File : BN002791.D
Acq On : 20 Sep 2018 17:58
Operator : JU/SJ
Sample : PB112991BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK91

Manual Integrations
APPROVED

Sohil
9/21/2018 2:06:04 PM

Quant Time: Sep 21 04:00:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 04:00:39 2018
Response via : Initial Calibration

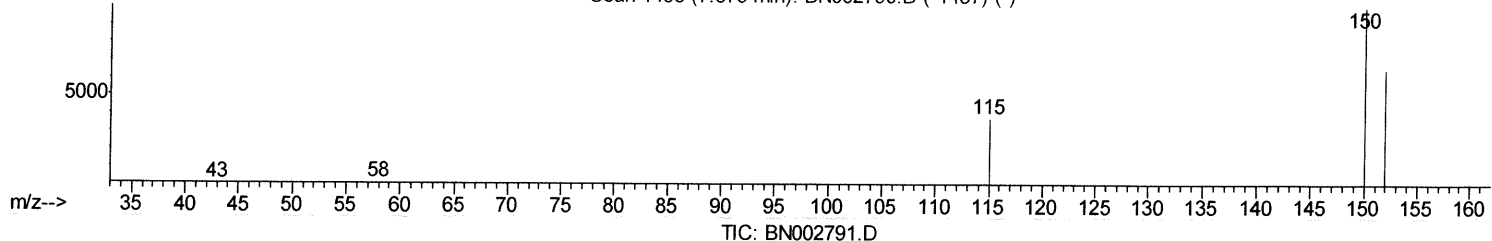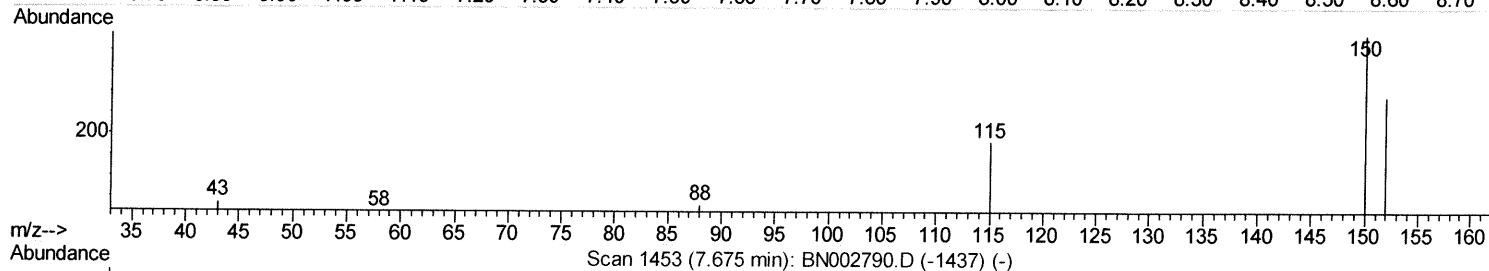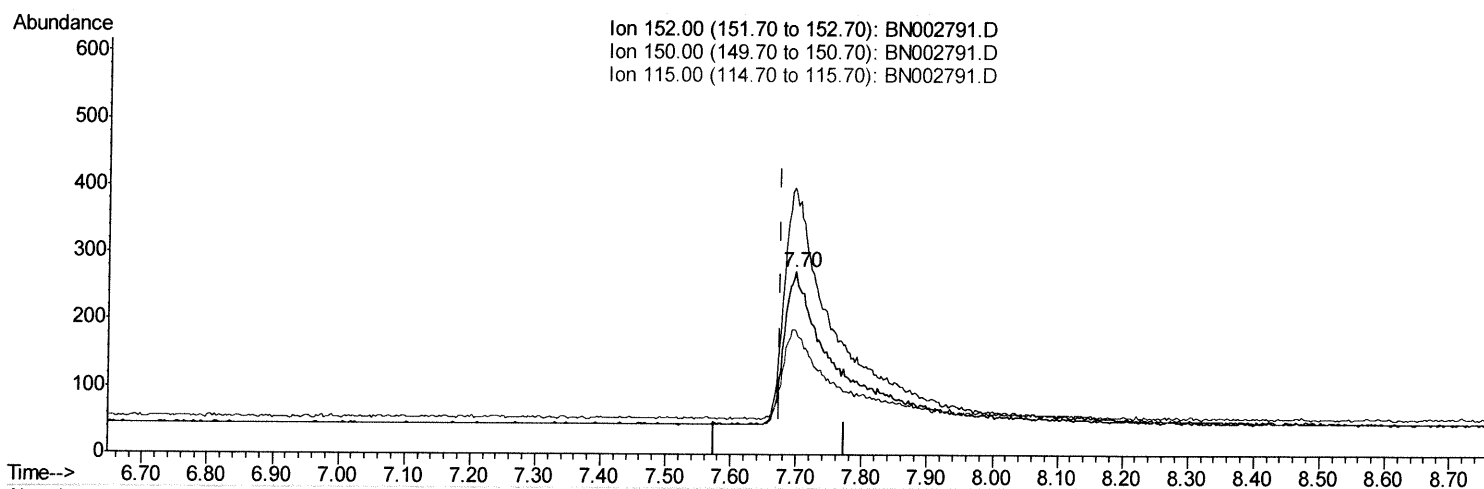

(1) 1,4-Dichlorobenzene-d4 (I)

7.698min (+0.023) 0.40ng/ul

response 800

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	143.59
115.00	64.90	68.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
 Data File : BN002791.D
 Acq On : 20 Sep 2018 17:58
 Operator : JU/SJ
 Sample : PB112991BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK91

Manual Integrations
 APPROVED

Sohil
 9/21/2018 2:06:04 PM

Quant Time: Sep 21 04:00:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 04:00:39 2018
 Response via : Initial Calibration

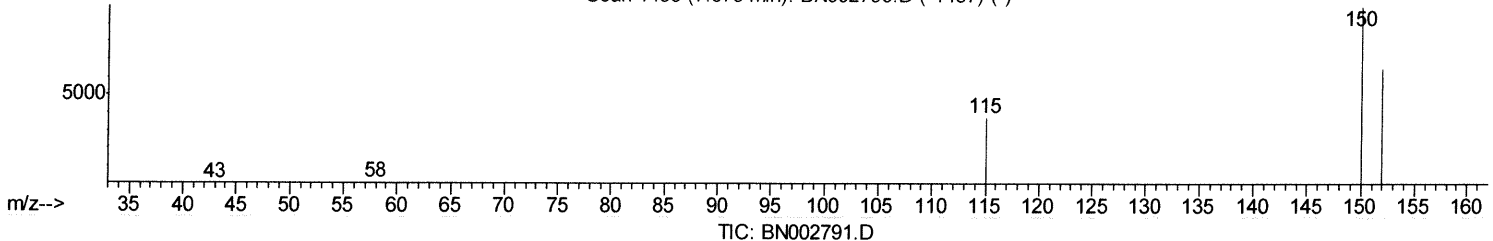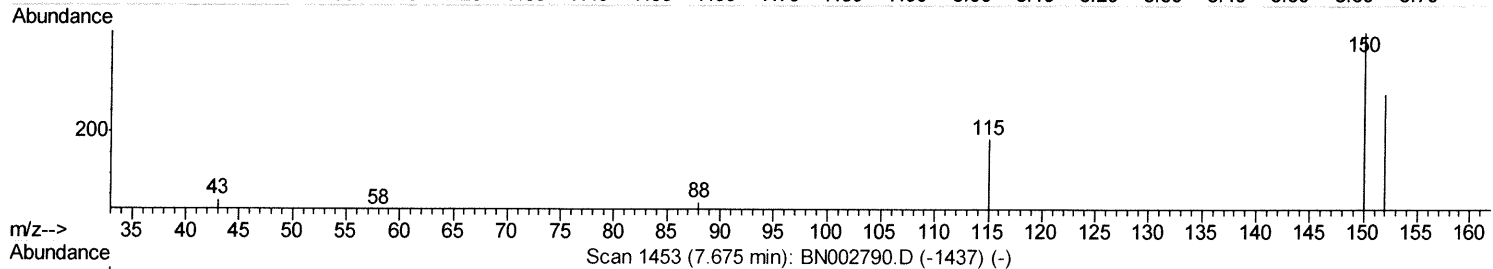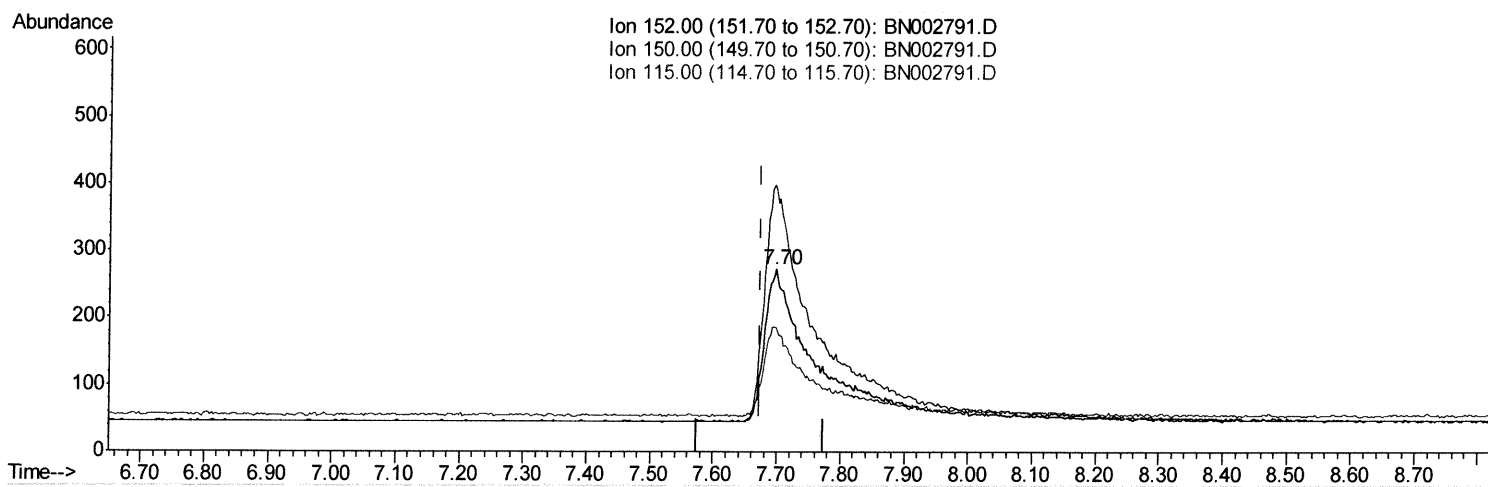

(1) 1,4-Dichlorobenzene-d4 (I)

7.698min (+0.023) 0.40ng/ul m *519/24/18*

response 1042

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	143.59
115.00	64.90	68.13
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
Data File : BN002791.D
Acq On : 20 Sep 2018 17:58
Operator : JU/SJ
Sample : PB112991BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK91

Manual Integrations
APPROVED

Sohil
9/21/2018 2:06:04 PM

Quant Time: Sep 21 04:14:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 04:00:39 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	1042m	0.40	ng/ul	0.02
2) Naphthalene-d8	10.49	136	4506	0.40	ng/ul	0.05
6) Acenaphthene-d10	14.32	164	2419	0.40	ng/ul	0.02
10) Phenanthrene-d10	17.09	188	4709	0.40	ng/ul	0.03
16) Chrysene-d12	21.27	240	4606	0.40	ng/ul	0.01
20) Perylene-d12	23.48	264	4683	0.40	ng/ul	0.00

5/9/24/18

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.09	152	2275	0.35	ng/ul	0.05
14) Fluoranthene-d10	19.10	212	4712	0.39	ng/ul	0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed