


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
Data File : BN002792.D
Acq On : 20 Sep 2018 18:33
Operator : JU/SJ
Sample : PB113006BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Manual Integrations
APPROVED

Sohil
9/21/2018 2:06:05 PM

Quant Time: Sep 21 04:16:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 04:00:39 2018
Response via : Initial Calibration

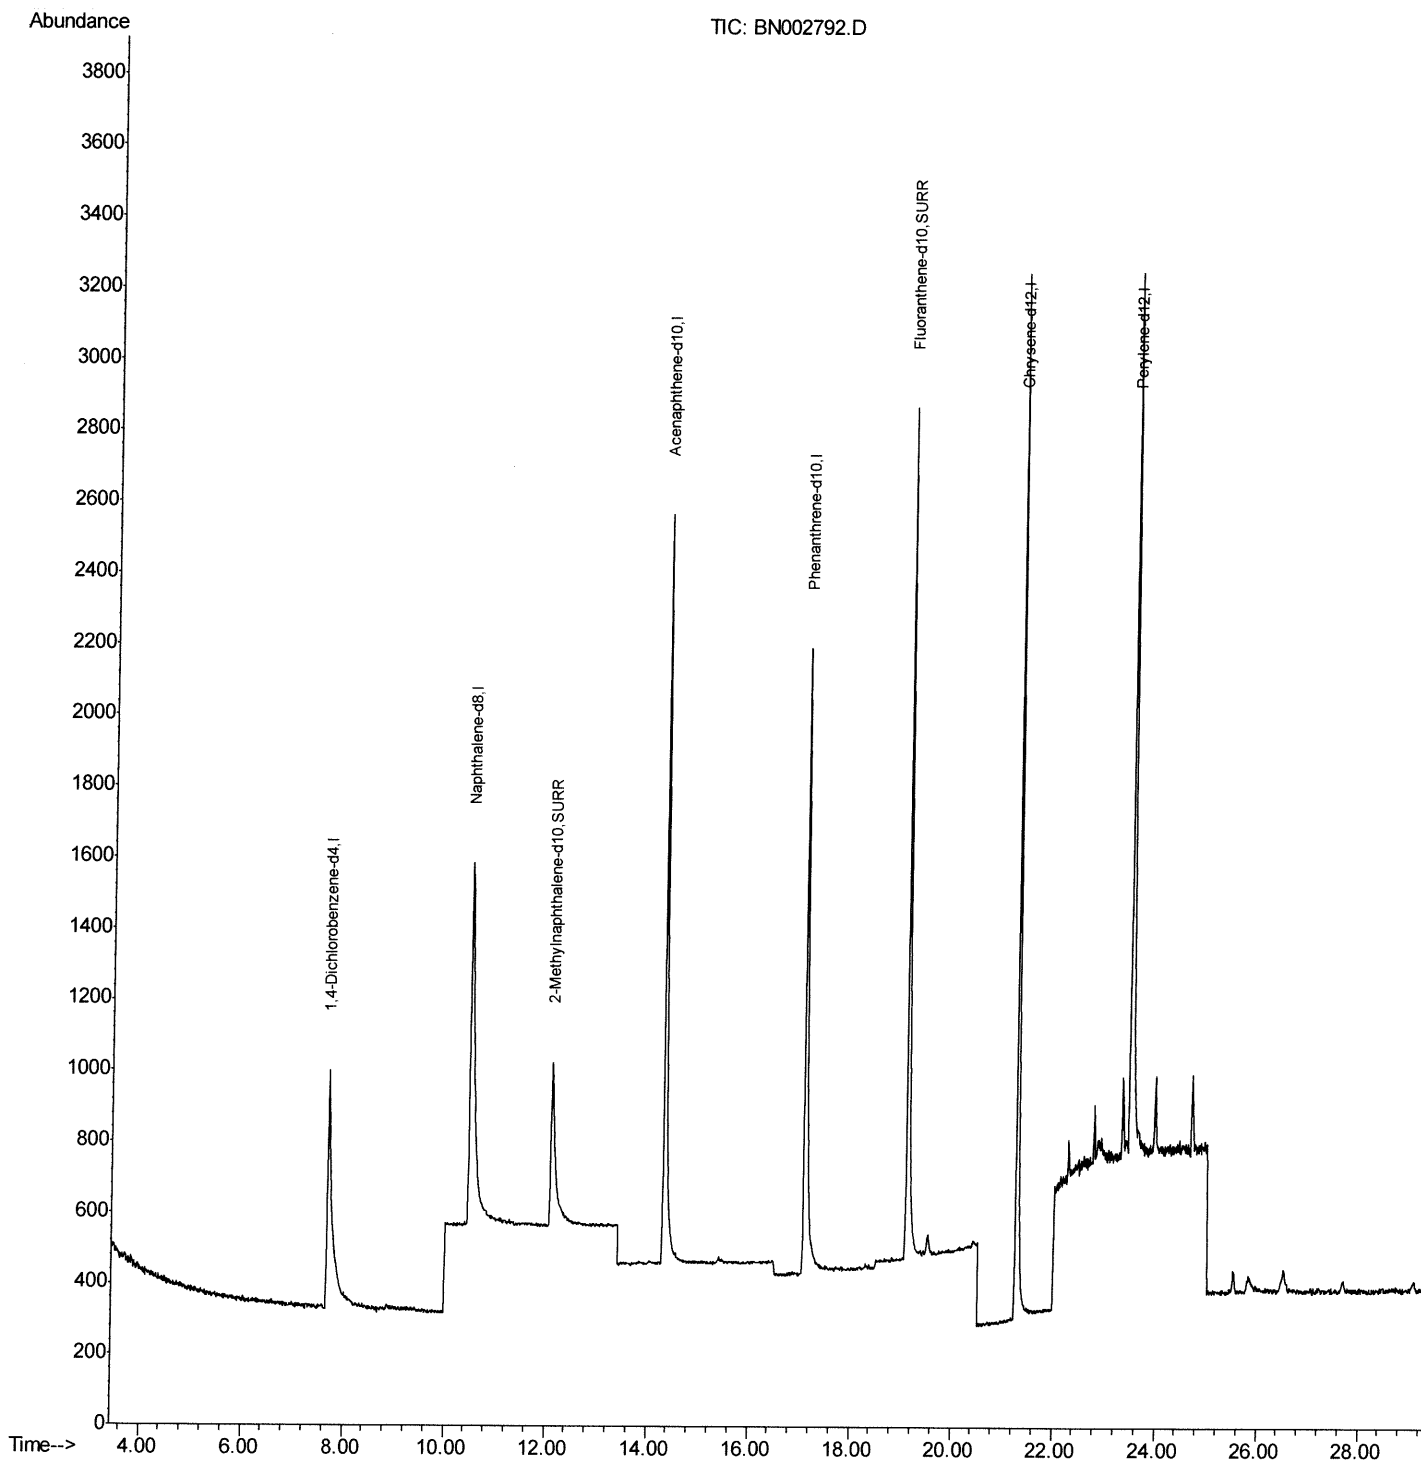

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
Data File : BN002792.D
Acq On : 20 Sep 2018 18:33
Operator : JU/SJ
Sample : PB113006BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Manual Integrations
APPROVED

Sohil
9/21/2018 2:06:05 PM

Quant Time: Sep 21 04:01:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 04:00:39 2018
Response via : Initial Calibration

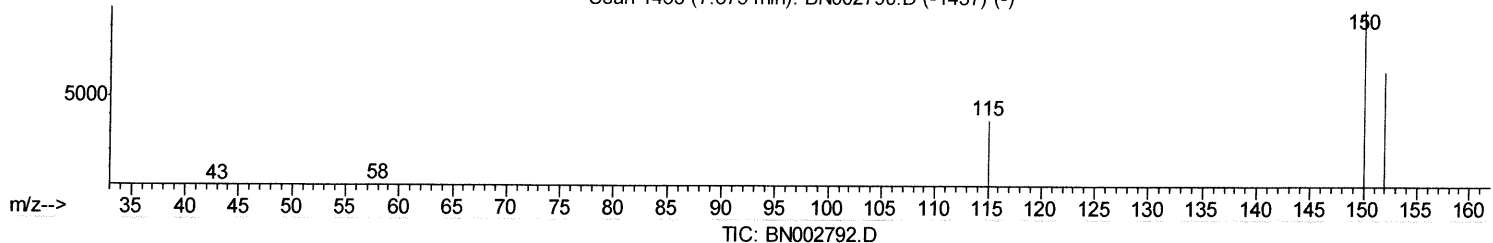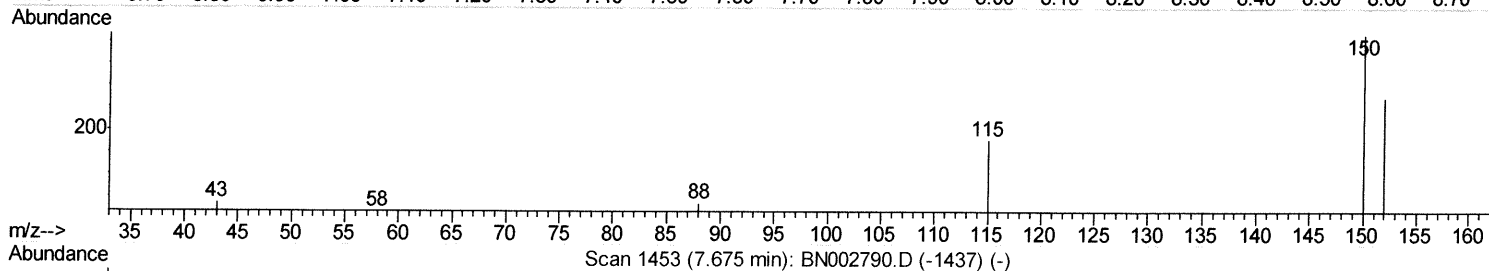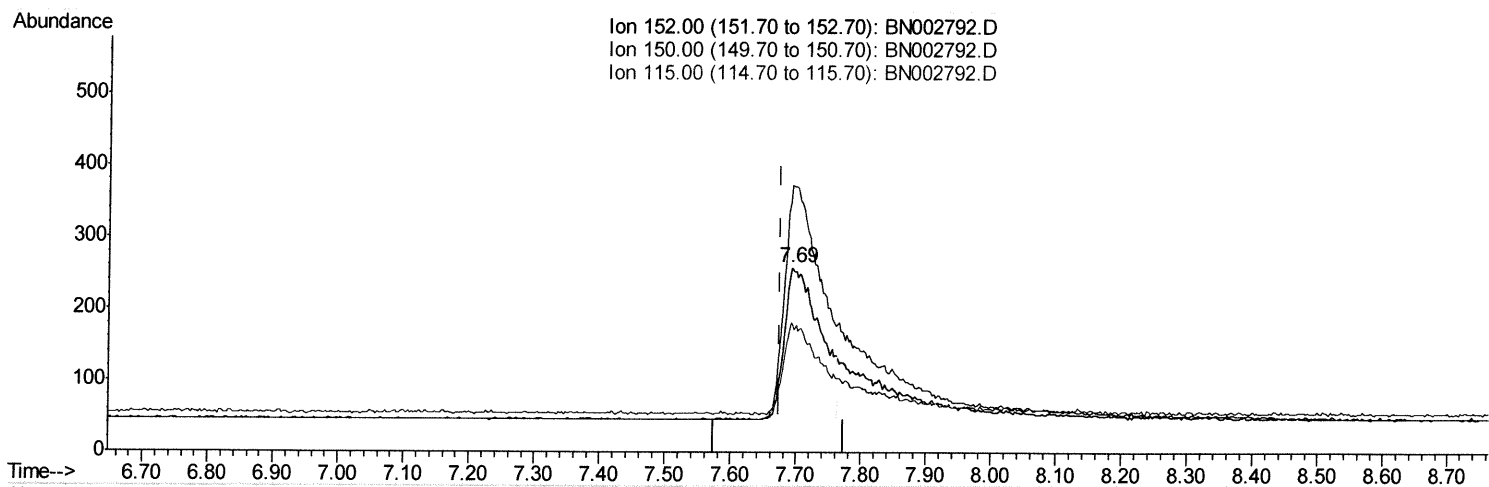

(1) 1,4-Dichlorobenzene-d4 (I)

7.693min (+0.018) 0.40ng/ul

response 801

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	144.19
115.00	64.90	70.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
 Data File : BN002792.D
 Acq On : 20 Sep 2018 18:33
 Operator : JU/SJ
 Sample : PB113006BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK06

Manual Integrations
 APPROVED

Sohil
 9/21/2018 2:06:05 PM

Quant Time: Sep 21 04:01:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 04:00:39 2018
 Response via : Initial Calibration

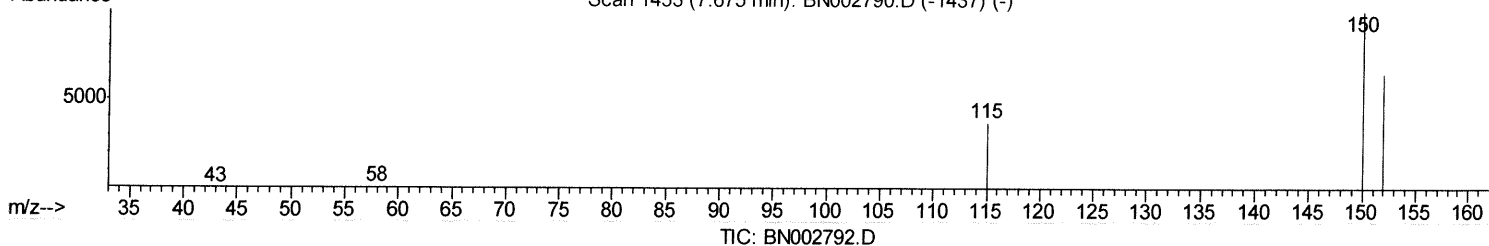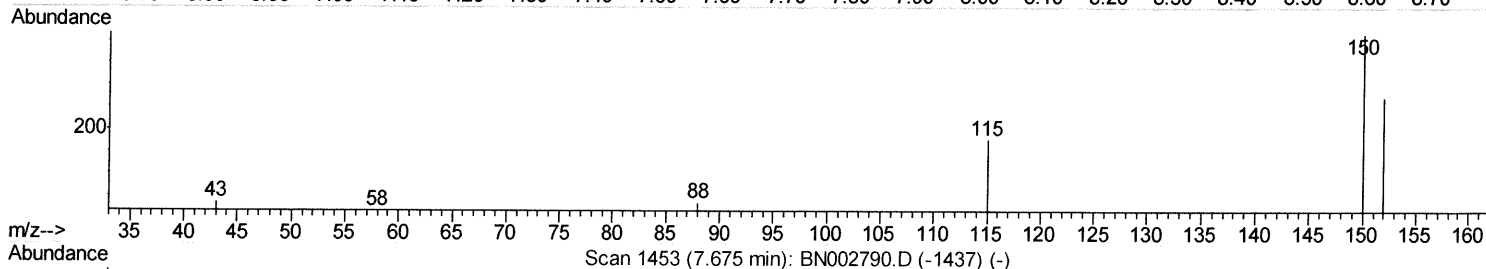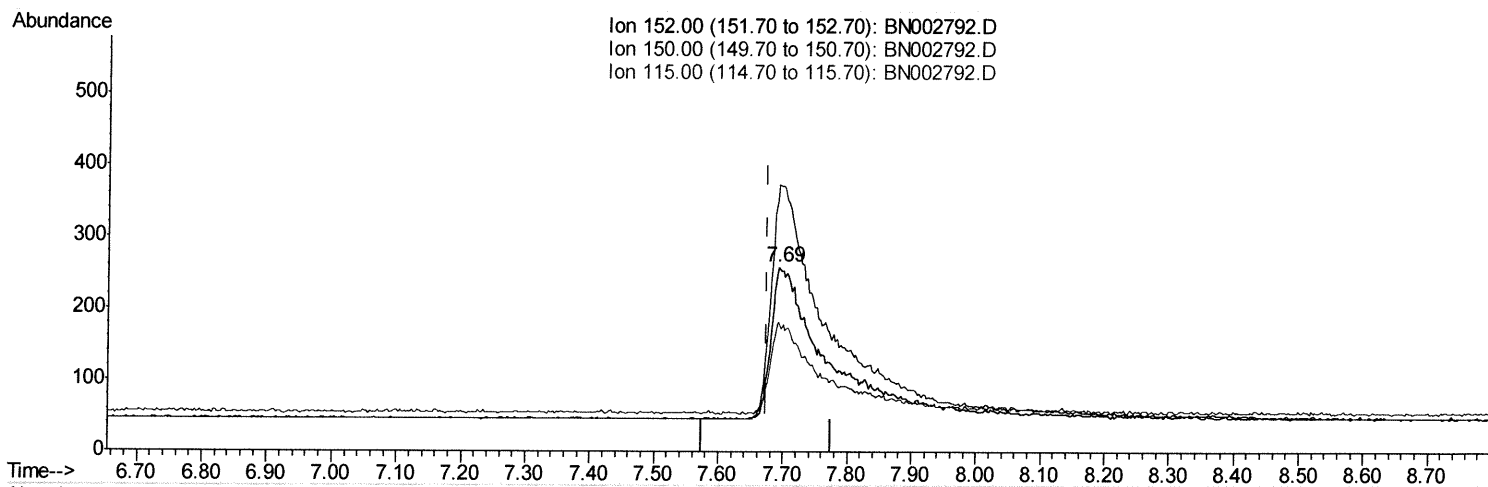

(1) 1,4-Dichlorobenzene-d4 (I)

7.693min (+0.018) 0.40ng/ul m

SS 9/24/18

response 973

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	144.19
115.00	64.90	70.16
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092118\
Data File : BN002792.D
Acq On : 20 Sep 2018 18:33
Operator : JU/SJ
Sample : PB113006BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Manual Integrations
APPROVED

Sohil
9/21/2018 2:06:05 PM

Quant Time: Sep 21 04:16:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 04:00:39 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	973m	0.40	ng/ul	0.02
2) Naphthalene-d8	10.49	136	4401	0.40	ng/ul	0.06
6) Acenaphthene-d10	14.32	164	2458	0.40	ng/ul	0.02
10) Phenanthrene-d10	17.09	188	4881	0.40	ng/ul	0.03
16) Chrysene-d12	21.27	240	4730	0.40	ng/ul	0.01
20) Perylene-d12	23.49	264	4831	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.11	152	2004	0.32	ng/ul	0.06
14) Fluoranthene-d10	19.10	212	4851	0.39	ng/ul	0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SS 9/24/18