

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092118\
 Data File : BN002800.D
 Acq On : 20 Sep 2018 23:13
 Operator : JU/SJ
 Sample : J4900-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3ZE7

Manual Integrations
 APPROVED

Sohil
 9/21/2018 2:06:12 PM

Quant Time: Sep 21 04:53:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 21 04:00:39 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	1695	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.42	136	6255	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	3236	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	6522m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.24	240	5855m	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	5473m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	3111	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	6717m	0.40	ng/ul	-0.01
Target Compounds						
13) Anthracene	17.17	178	388m	0.025	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092118\
Data File : BN002800.D
Acq On : 20 Sep 2018 23:13
Operator : JU/SJ
Sample : J4900-04
Misc :
ALS Vial : 16 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A3ZE7

Manual Integrations
APPROVED

Sohil
9/21/2018 2:06:12 PM

Quant Time: Sep 21 04:53:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 21 04:00:39 2018
Response via : Initial Calibration

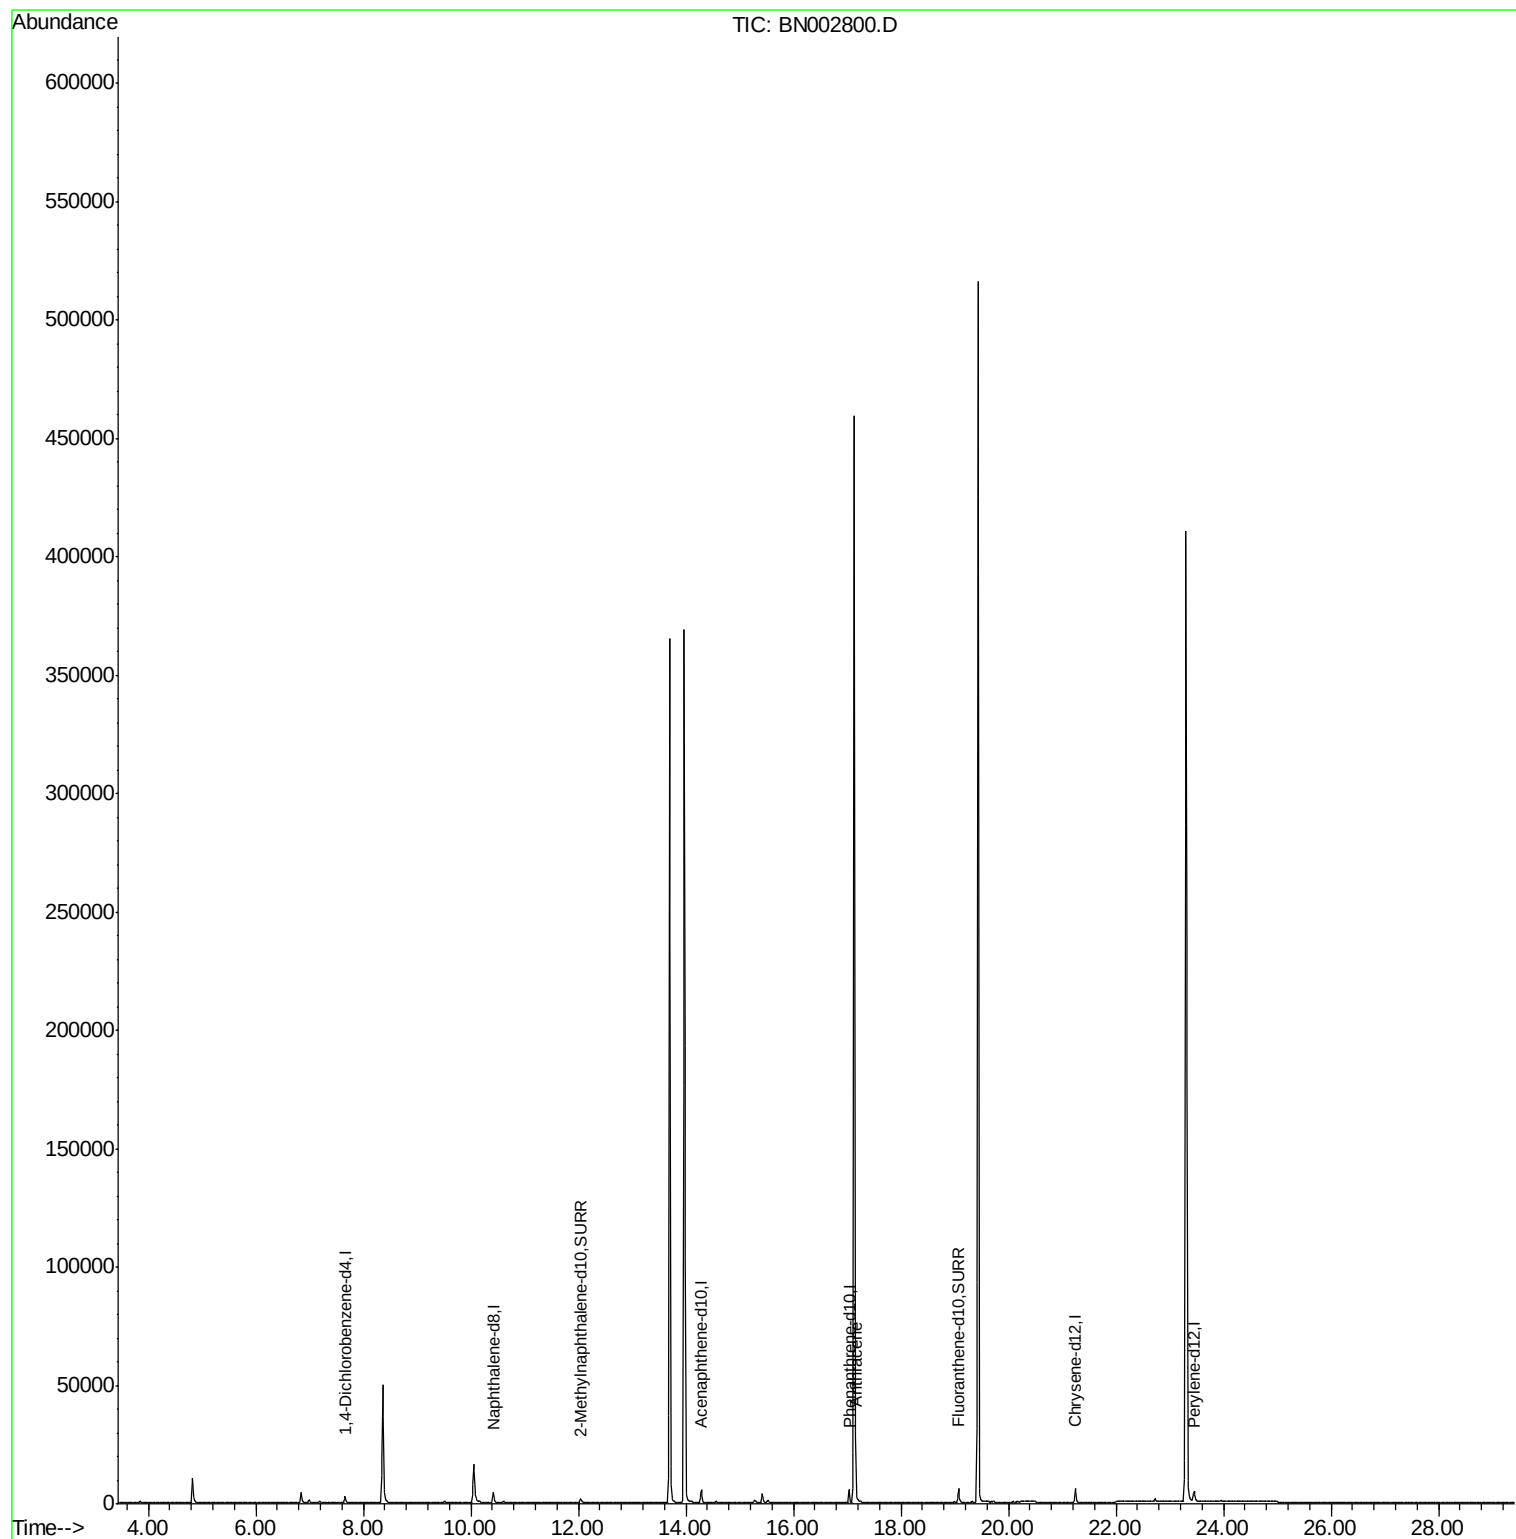

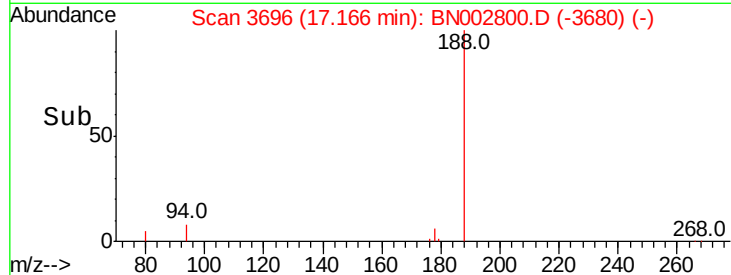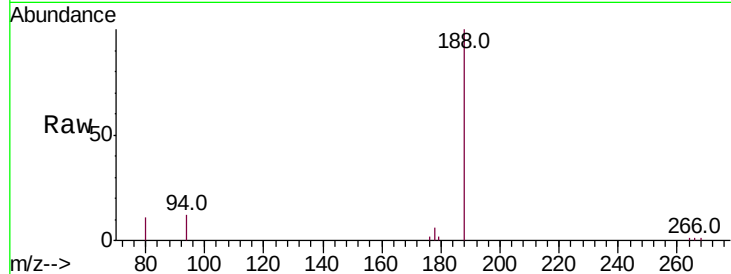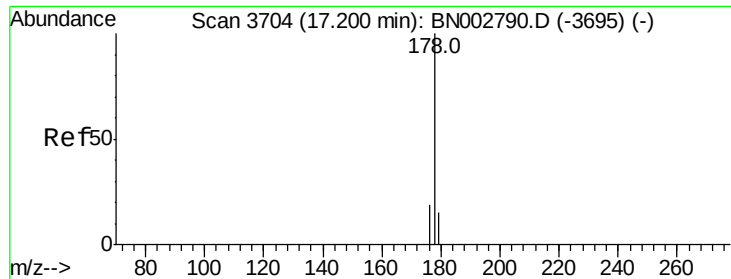

#13

Anthracene

Concen: 0.025 ng/ul m

RT: 17.17 min Scan# 3696

Delta R.T. -0.03 min

Lab File: BN002800.D

Acq: 20 Sep 2018 23:13

Instrument :

BNA_N

ClientSampleId :

A3ZE7

Tot Ion:178 Resp: 388

Ion Ratio Lower Upper

178 100

179 38.4 18.1 27.1#

176 35.9 14.7 22.1#

Manual Integrations

APPROVED

Sohil

9/21/2018 2:06:12 PM

