
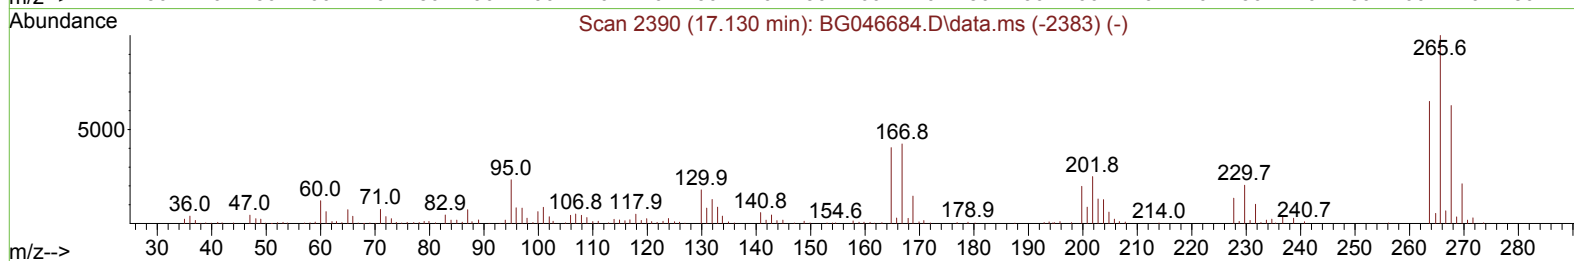
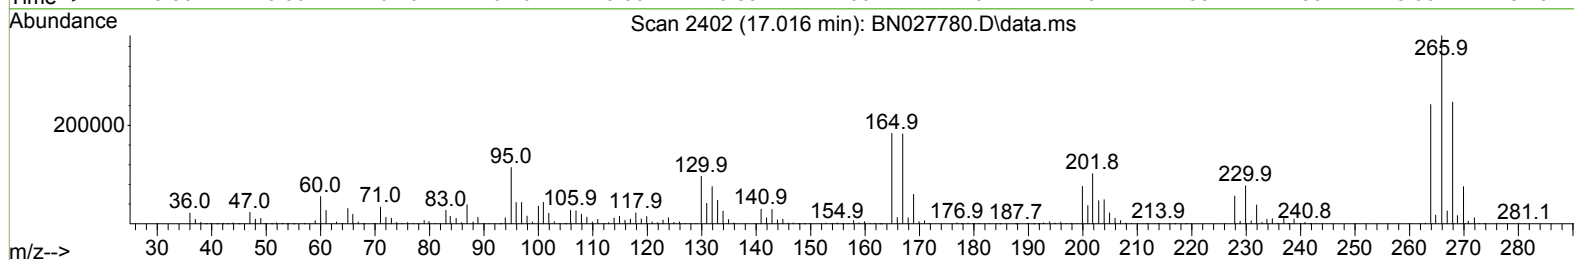


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092123\
Data File : BN027780.D
Acq On : 21 Sep 2023 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 03:03:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:03:16 2023
Response via : Initial Calibration

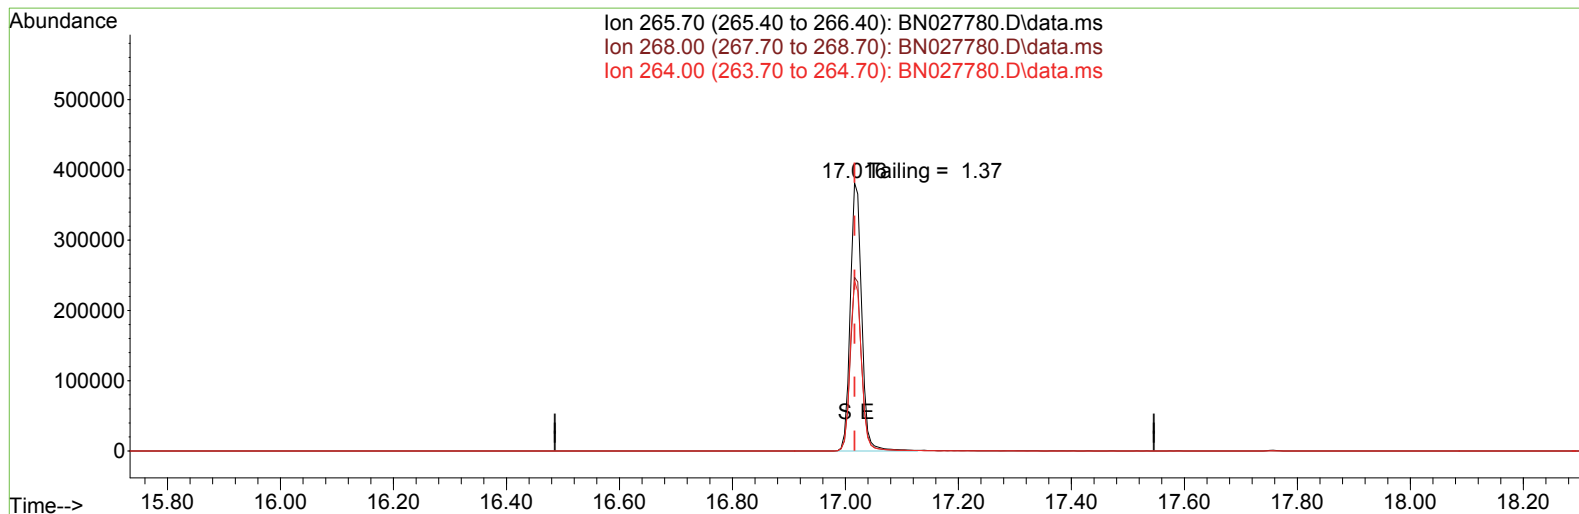

TIC: BN027780.D\data.ms

(70) Pentachlorophenol (C)




17.016min (0.000) 24669.21 ng

response 537621

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.72
264.00	61.60	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092123\
Data File : BN027780.D
Acq On : 21 Sep 2023 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 03:03:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:03:16 2023
Response via : Initial Calibration

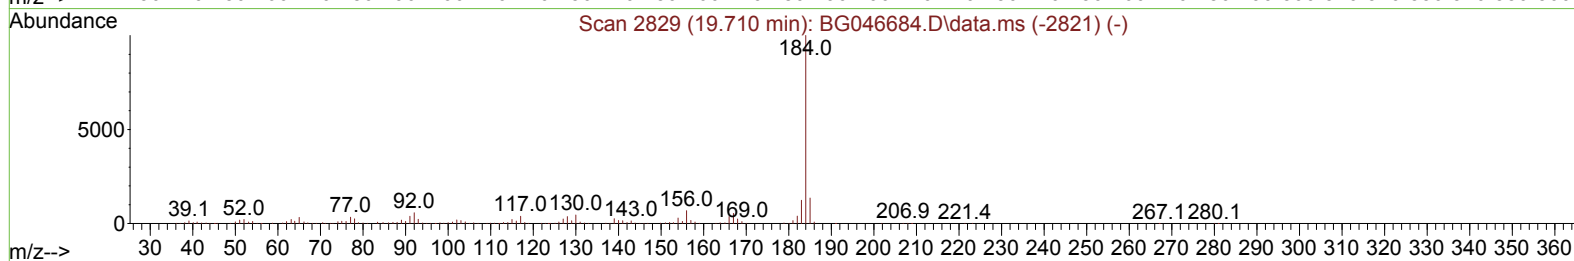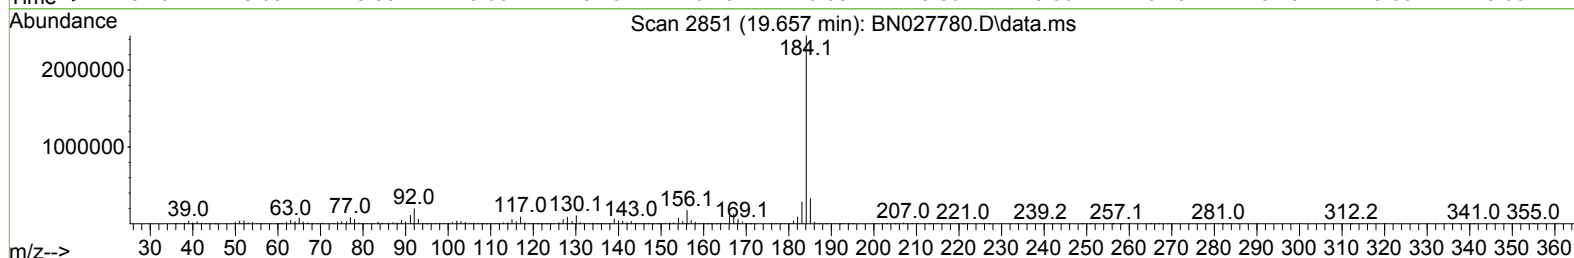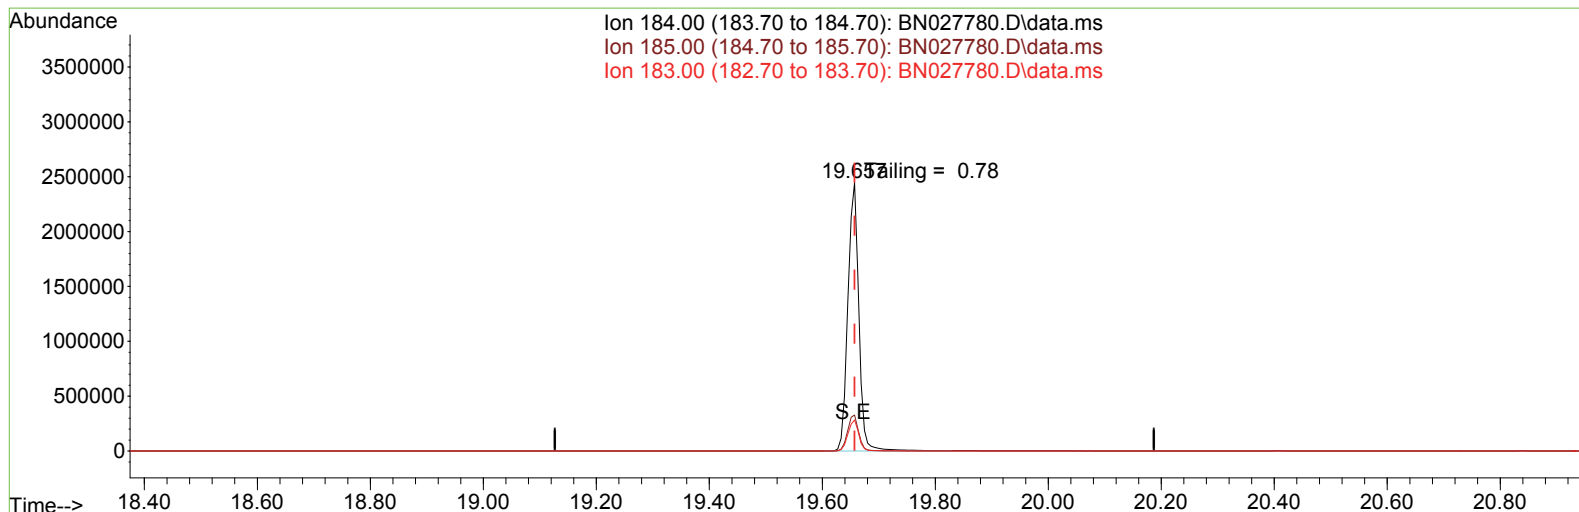

TIC: BN027780.D\data.ms

(77) Benzidine

19.657min (0.000) 0.00 ng

response 3321808

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.44
183.00	13.20	11.58
0.00	0.00	0.00