
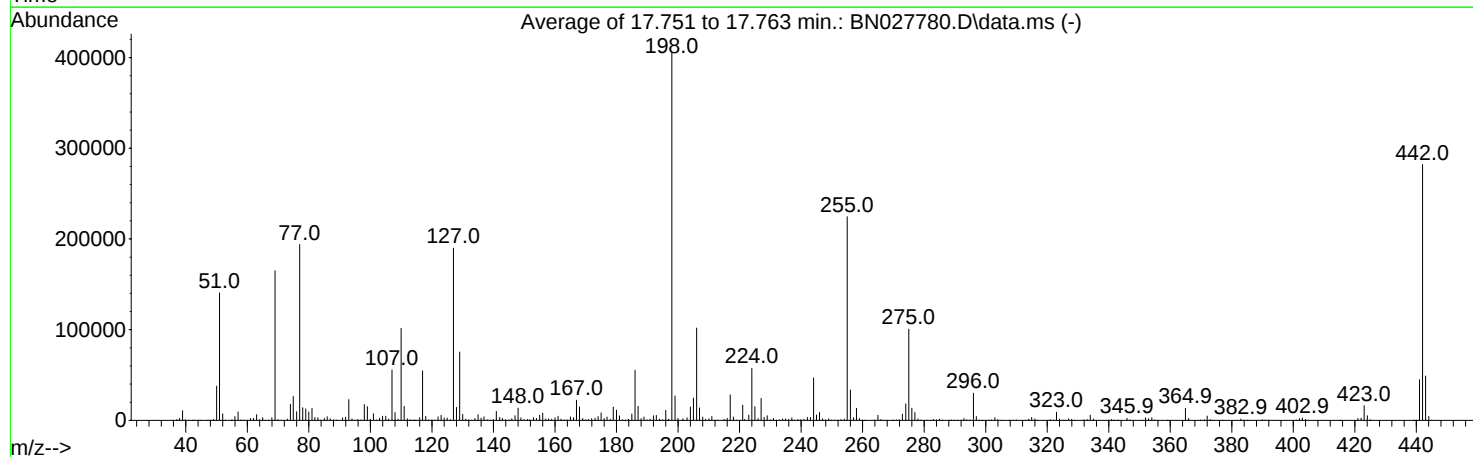


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092123\
Data File : BN027780.D
Acq On : 21 Sep 2023 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 20 13:45:42 2023

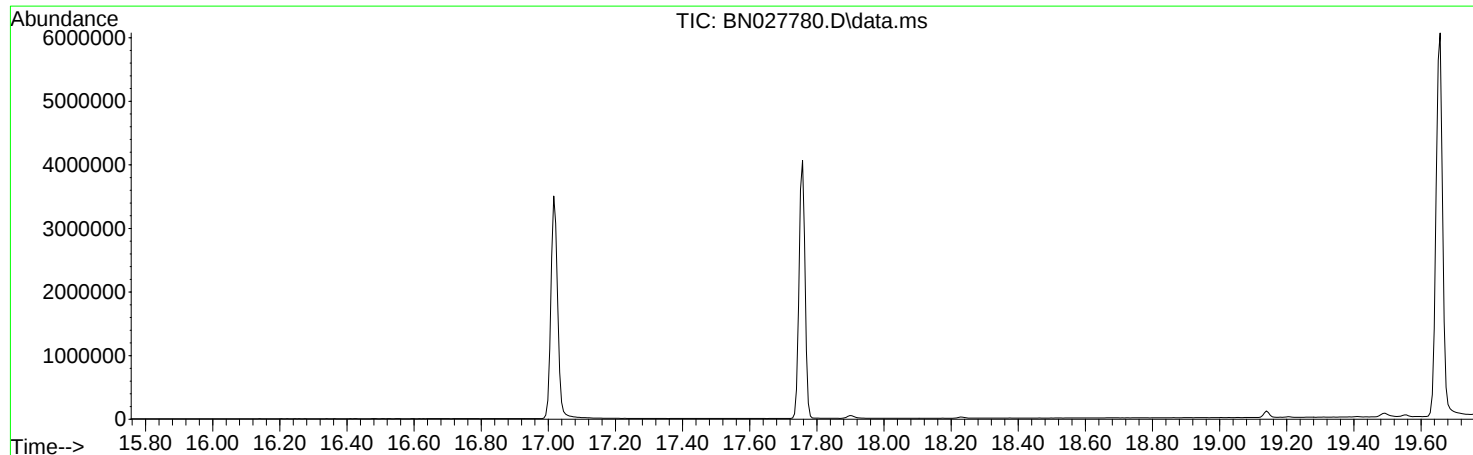




AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	140672	PASS
68	69	0.00	2	1.7	2767	PASS
69	198	0.00	100	40.7	164971	PASS
70	69	0.00	2	0.5	889	PASS
127	198	10	80	46.8	189909	PASS
197	198	0.00	2	0.3	1259	PASS
198	198	100	100	100.0	405589	PASS
199	198	5	9	6.7	27045	PASS
275	198	10	60	24.8	100520	PASS
365	198	1	100	3.3	13297	PASS
441	198	0.01	100	11.1	44888	PASS
442	442	50	100	100.0	282005	PASS
443	442	15	24	17.3	48880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092123\
Data File : BN027780.D
Acq On : 21 Sep 2023 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 22 03:03:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:03:16 2023
Response via : Initial Calibration

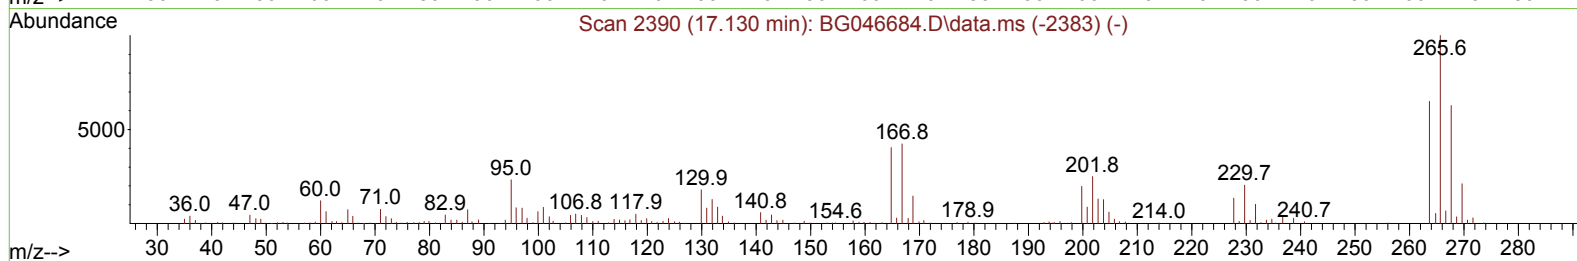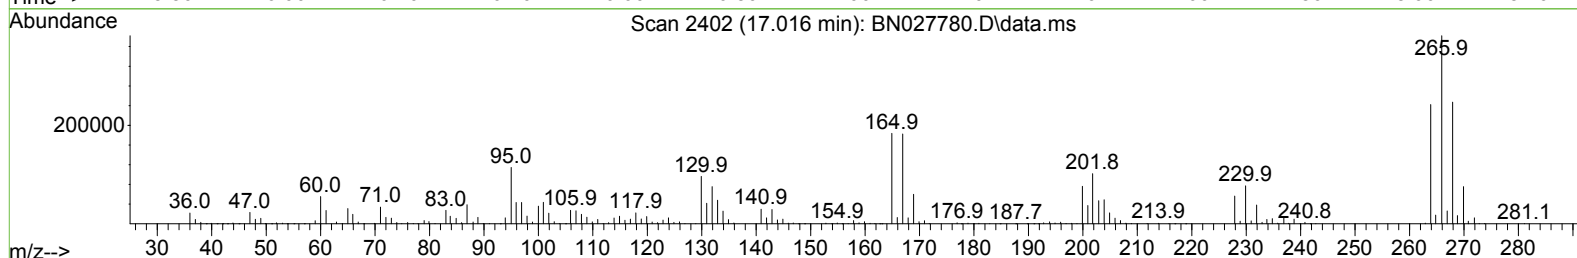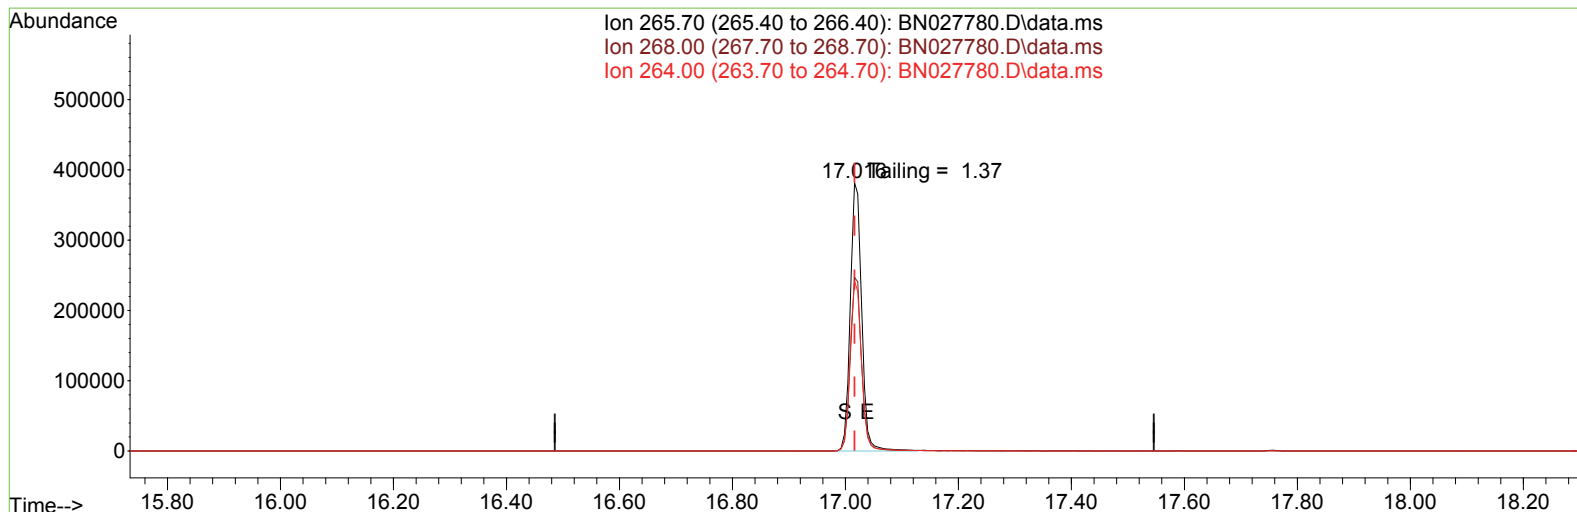

TIC: BN027780.D\data.ms

(70) Pentachlorophenol (C)

17.016min (0.000) 24669.21 ng




response 537621

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.72
264.00	61.60	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092123\
Data File : BN027780.D
Acq On : 21 Sep 2023 08:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 22 03:03:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:03:16 2023
Response via : Initial Calibration

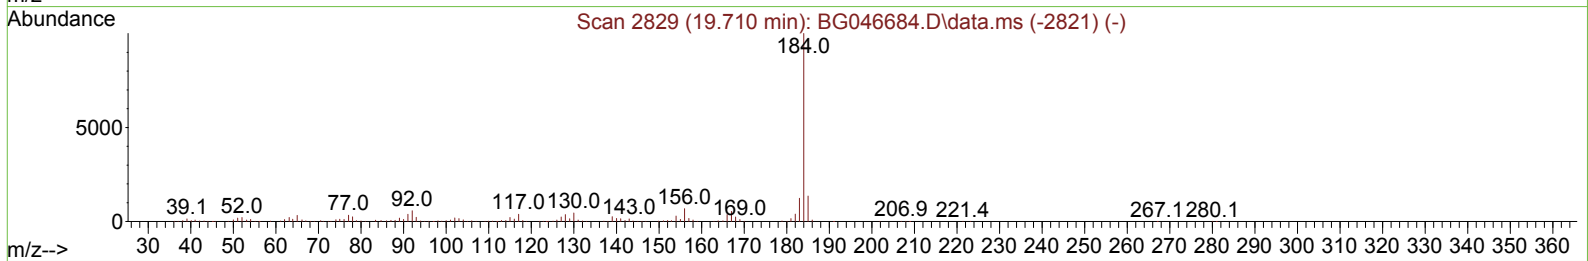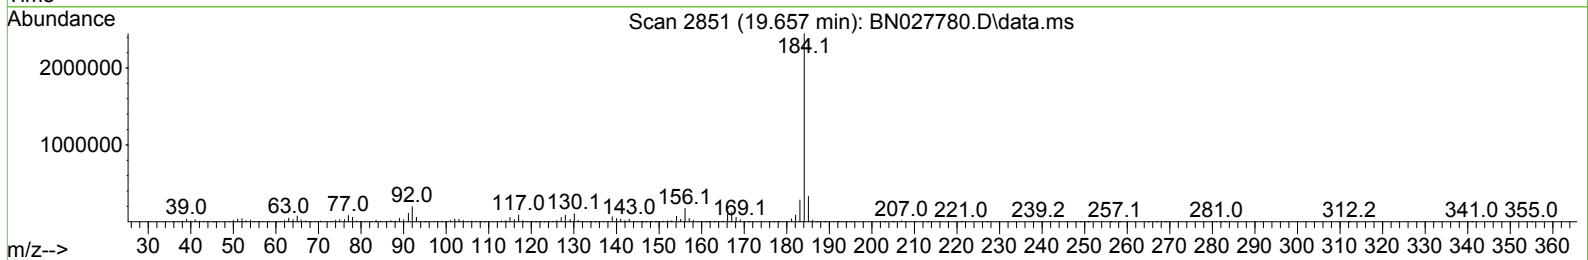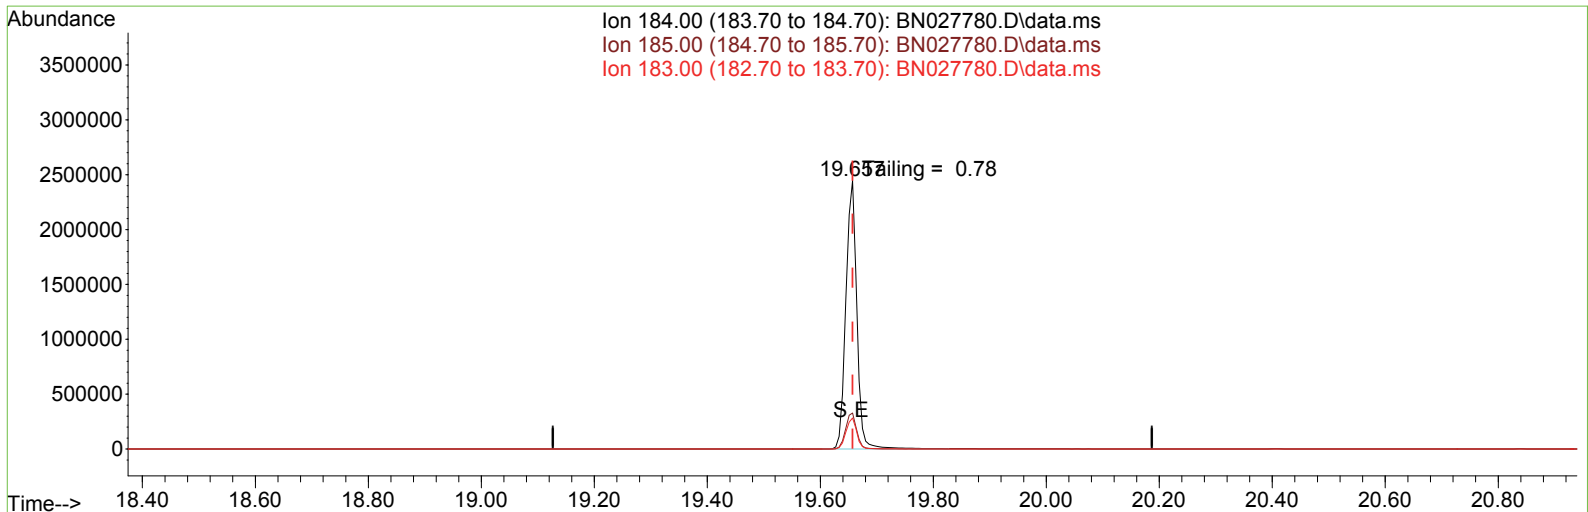

TIC: BN027780.D\data.ms

(77) Benzidine

19.657min (0.000) 0.00 ng

response 3321808

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.44
183.00	13.20	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/21/2023	BNA_N	<u>BN027780.D</u>
Compound Name	Response	Retention Time
DDT	391079	20.839
DDD	782838	20.404
DDE	1208	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
784046	1175125	66.72

Instrument :
BNA_N
ClientSampleId :
DFTPP