

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
 Data File : BN034126.D
 Acq On : 21 Sep 2024 16:03
 Operator : JU/RC
 Sample : P4116-16
 Misc :
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE131D1-20240917

Quant Time: Sep 22 23:59:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 16:09:28 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.431	152	5522	0.400	ng	0.00
7) Naphthalene-d8	10.180	136	15246	0.400	ng	#-0.02
13) Acenaphthene-d10	14.069	164	8928	0.400	ng	-0.01
19) Phenanthrene-d10	16.828	188	18987	0.400	ng	#-0.01
29) Chrysene-d12	21.051	240	13317	0.400	ng	0.00
35) Perylene-d12	23.172	264	10098	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.069	112	3238	0.207	ng	0.00
5) Phenol-d6	6.629	99	2084	0.114	ng	0.00
8) Nitrobenzene-d5	8.568	82	3807	0.326	ng	0.00
11) 2-Methylnaphthalene-d10	11.784	152	7966	0.354	ng	0.00
14) 2,4,6-Tribromophenol	15.574	330	1106	0.273	ng	-0.01
15) 2-Fluorobiphenyl	12.690	172	13065	0.360	ng	-0.01
27) Fluoranthene-d10	18.874	212	19612	0.409	ng	-0.01
31) Terphenyl-d14	19.496	244	12995	0.489	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.068	88	54315	7.868	ng	# 88
20) 4,6-Dinitro-2-methylph...	15.234	198	2	0.138	ng	# 1
34) Bis(2-ethylhexyl)phtha...	21.006	149	1412	0.080	ng	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034126.D
Acq On : 21 Sep 2024 16:03
Operator : JU/RC
Sample : P4116-16
Misc :
ALS Vial : 90 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE131D1-20240917


Quant Time: Sep 22 23:59:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 16:09:28 2024
Response via : Initial Calibration

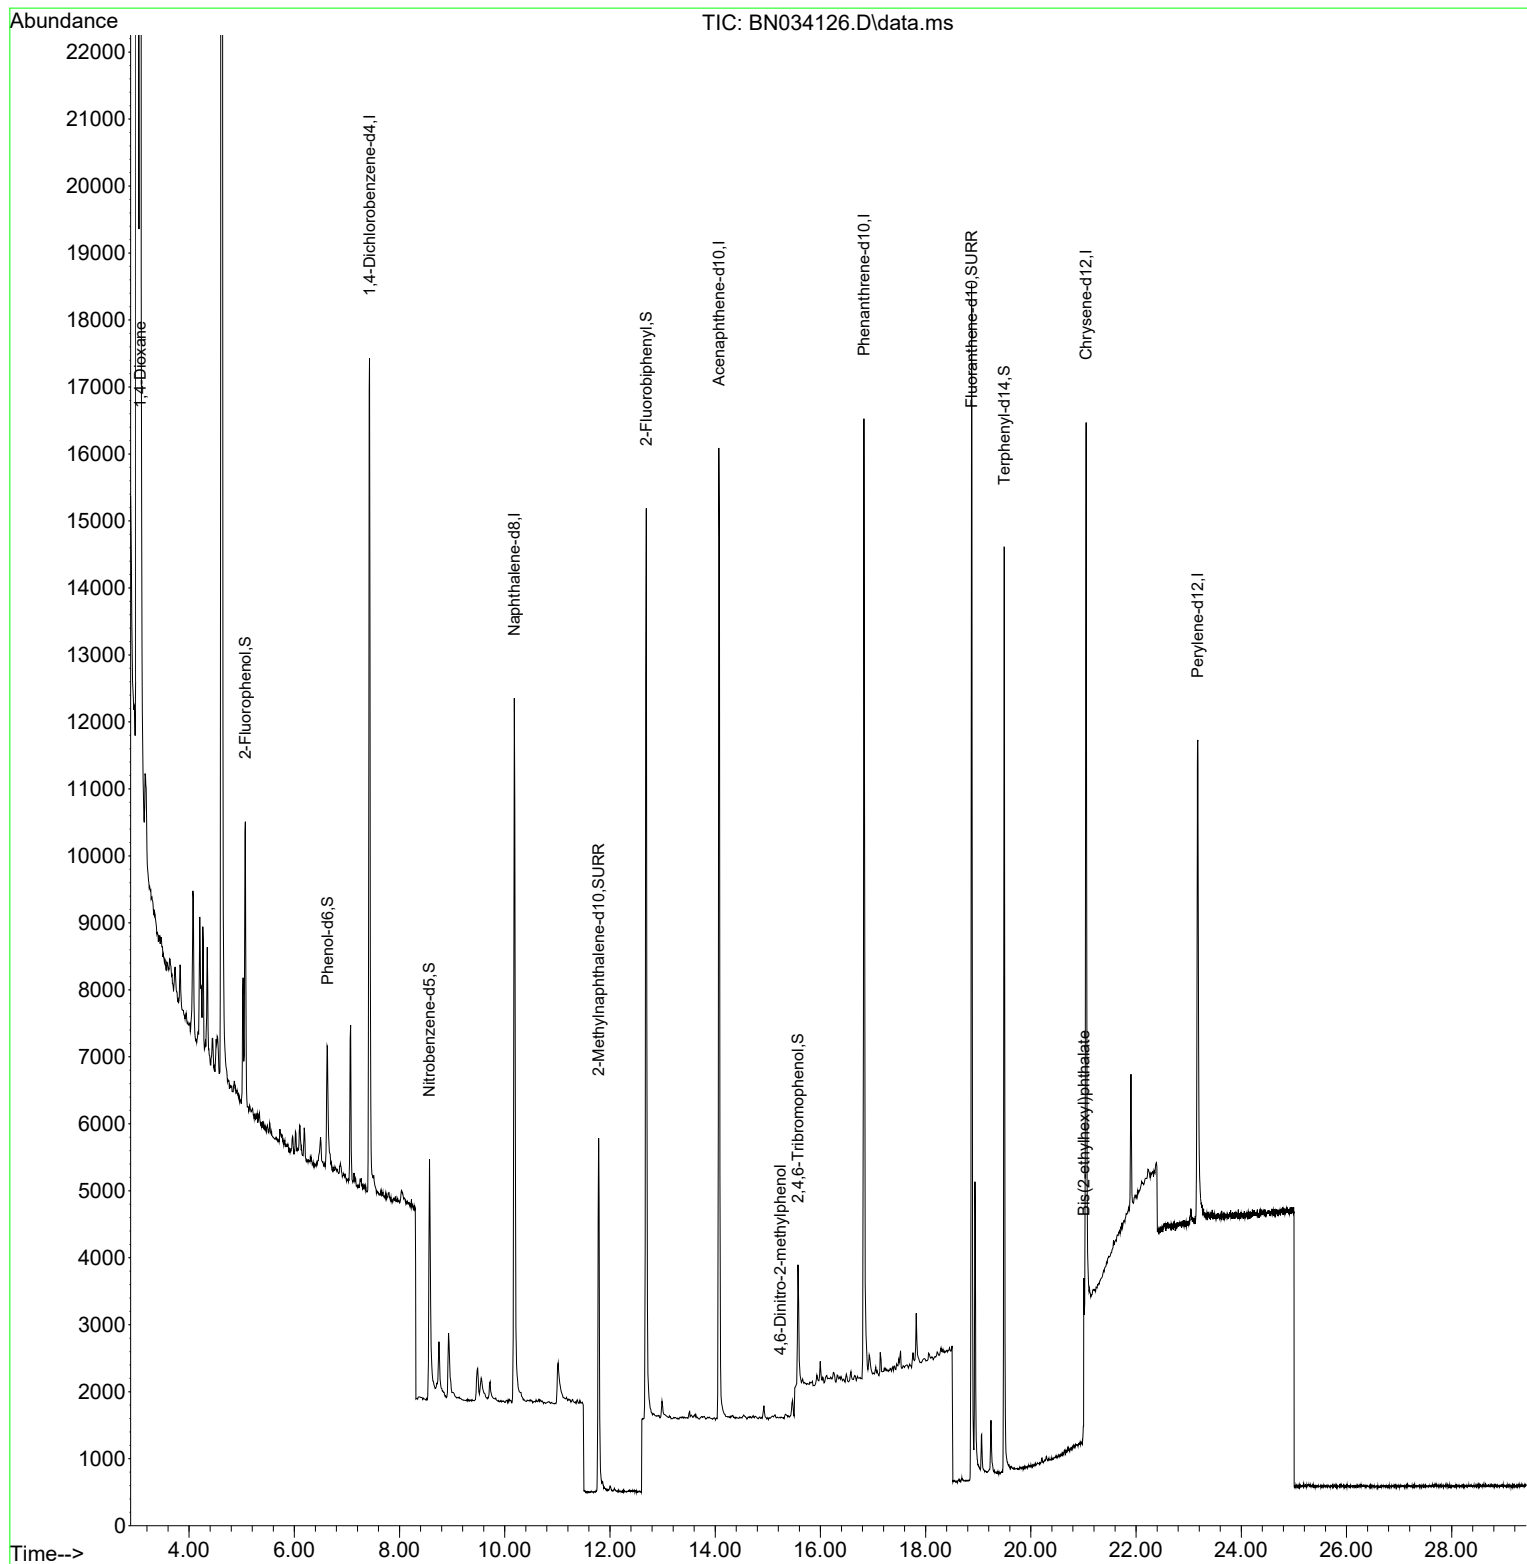



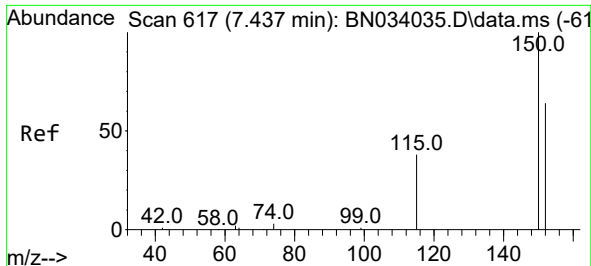


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.431 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BN034126.D
 Acq: 21 Sep 2024 16:03


Instrument :
 BNA_N
 ClientSampleId :
 RE131D1-20240917

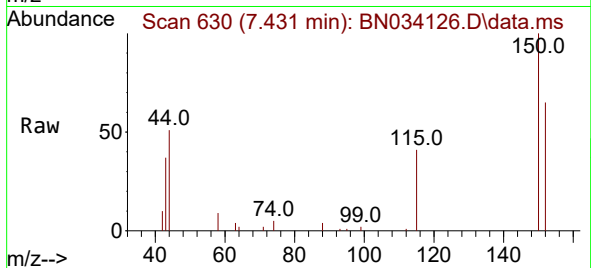



Tgt Ion:152 Resp: 5522
 Ion Ratio Lower Upper
 152 100
 150 152.7 124.6 187.0
 115 62.9 50.0 75.0

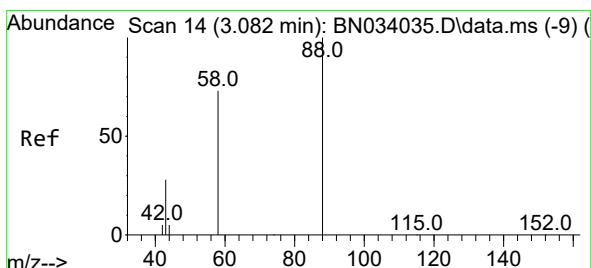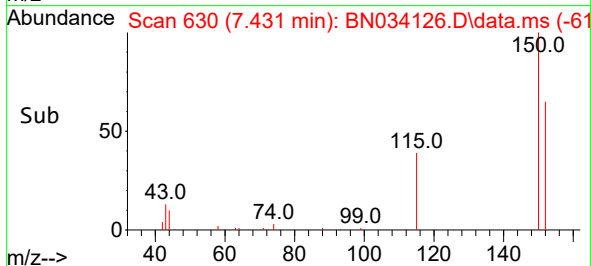


#2
 1,4-Dioxane
 Concen: 7.868 ng
 RT: 3.068 min Scan# 26
 Delta R.T. -0.013 min
 Lab File: BN034126.D
 Acq: 21 Sep 2024 16:03

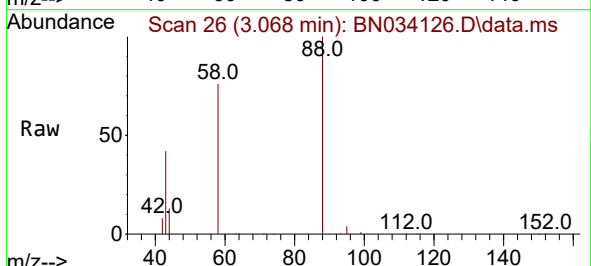

Tgt Ion: 88 Resp: 54315
 Ion Ratio Lower Upper
 88 100
 43 39.7 25.8 38.8#
 58 83.0 58.8 88.2




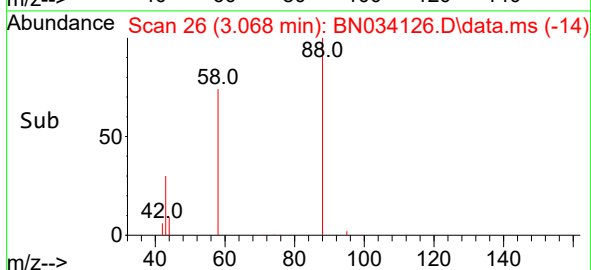


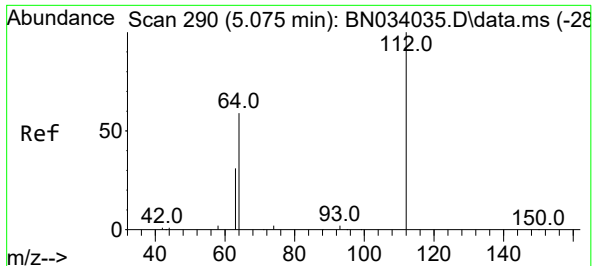

#4
2-Fluorophenol
Concen: 0.207 ng
RT: 5.069 min Scan# 303
Delta R.T. -0.006 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03




Instrument :
BNA_N
ClientSampleId :
RE131D1-20240917


Tgt Ion:112 Resp: 3238
Ion Ratio Lower Upper
112 100
64 64.2 48.6 72.8
63 34.6 25.6 38.4

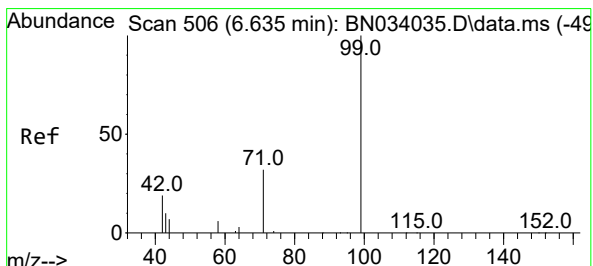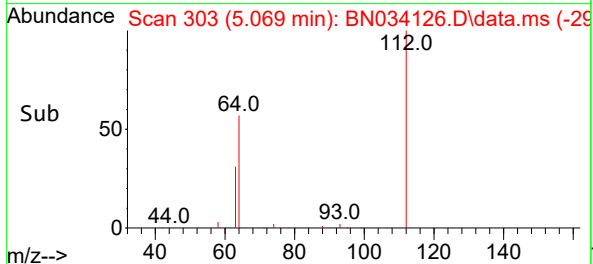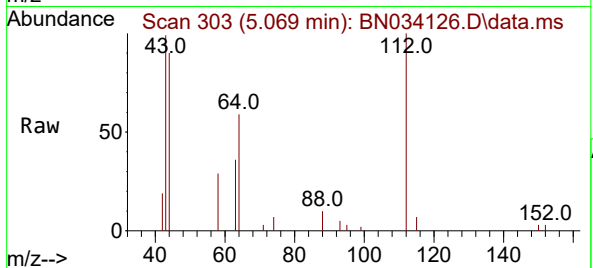

#5
Phenol-d6
Concen: 0.114 ng
RT: 6.629 min Scan# 519
Delta R.T. -0.006 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03

Tgt Ion: 99 Resp: 2084
Ion Ratio Lower Upper
99 100
42 25.8 17.8 26.8
71 40.4 26.2 39.2#


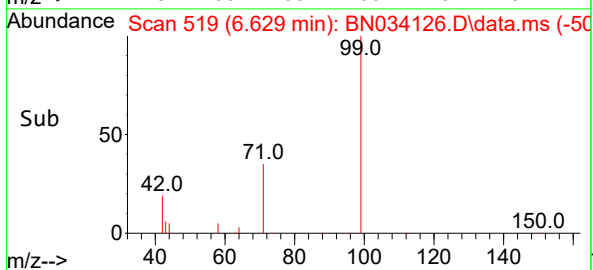

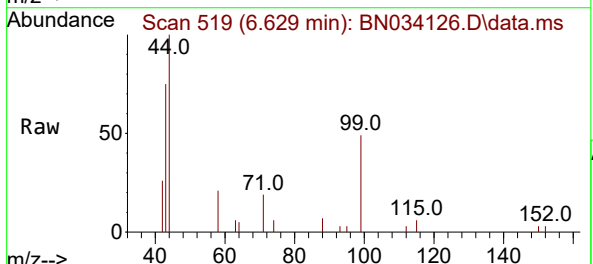


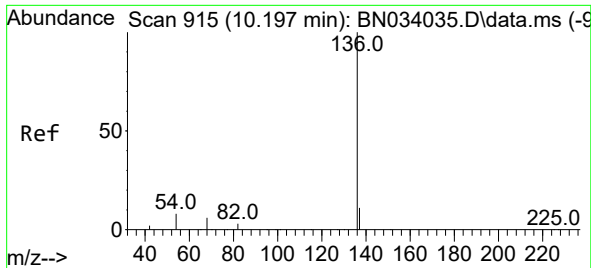

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.180 min Scan# 915
Delta R.T. -0.017 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03




Instrument :
BNA_N
ClientSampleId :
RE131D1-20240917


Tgt Ion:	136	Resp:	15246
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.0	13.6
54	11.9	6.8	10.2#
68	7.7	5.0	7.6#

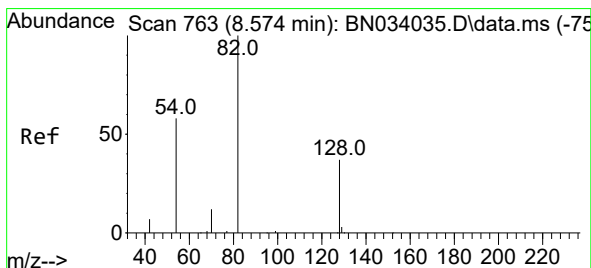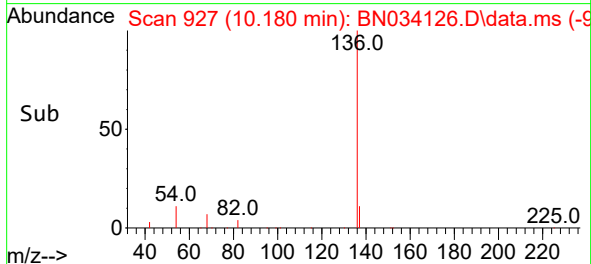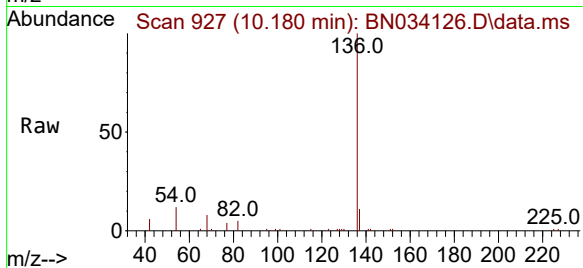

#8
Nitrobenzene-d5
Concen: 0.326 ng
RT: 8.568 min Scan# 776
Delta R.T. -0.006 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03

Tgt Ion:	82	Resp:	3807
Ion Ratio	Lower	Upper	
82	100		
128	39.6	31.4	47.2
54	62.0	47.4	71.0


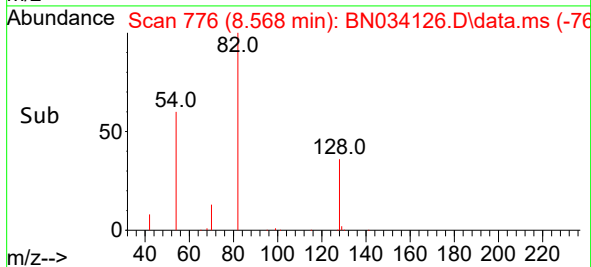

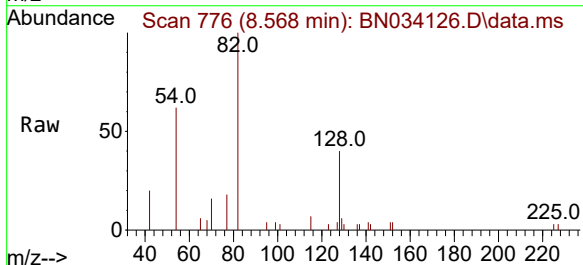


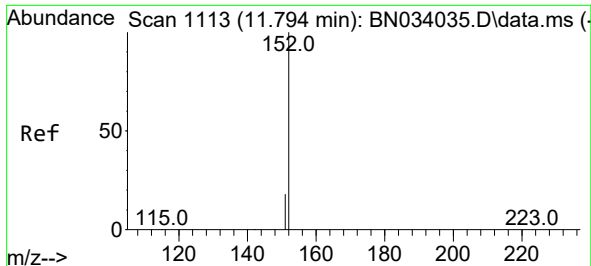

#11
2-Methylnaphthalene-d10
Concen: 0.354 ng
RT: 11.784 min Scan# 1113
Delta R.T. -0.010 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03




Instrument :
BNA_N
ClientSampleId :
RE131D1-20240917


Tgt Ion:152 Resp: 7966
Ion Ratio Lower Upper
152 100
151 21.6 16.8 25.2

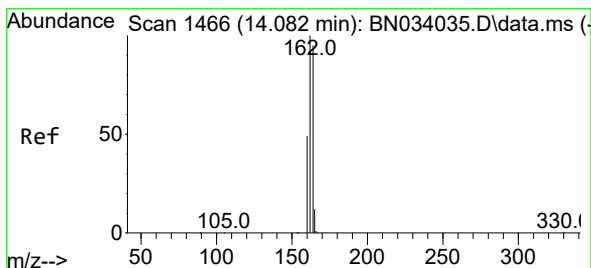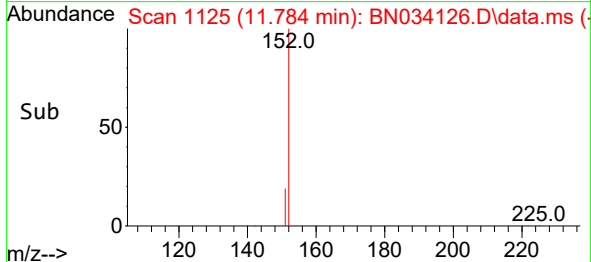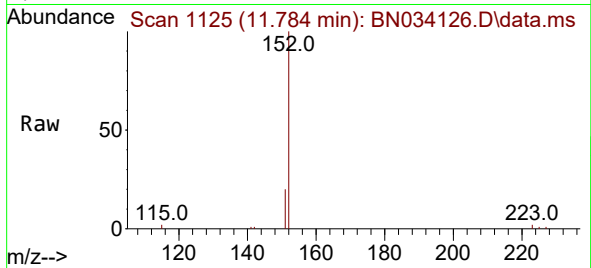

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.069 min Scan# 1479
Delta R.T. -0.013 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03


Tgt Ion:164 Resp: 8928
Ion Ratio Lower Upper
164 100
162 107.8 84.2 126.2
160 54.4 41.7 62.5

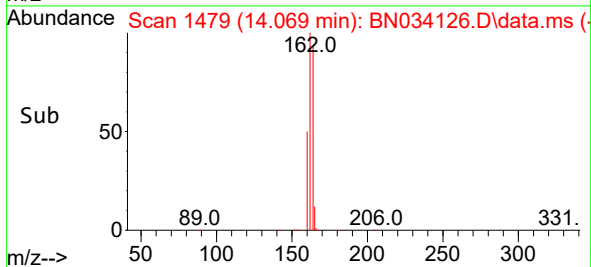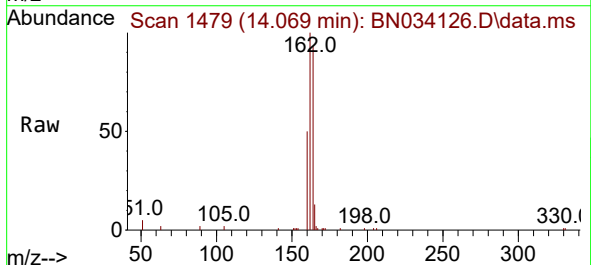



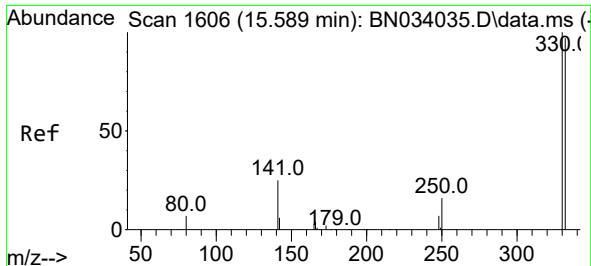


#14
2,4,6-Tribromophenol
Concen: 0.273 ng
RT: 15.574 min Scan# 1
Delta R.T. -0.015 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03

Instrument :
BNA_N
ClientSampleId :
RE131D1-20240917



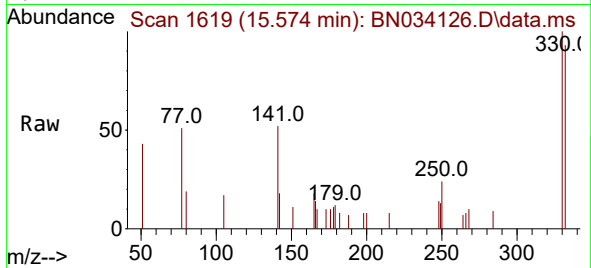



Tgt Ion:330 Resp: 1106
Ion Ratio Lower Upper
330 100
332 138.5 77.4 116.0#
141 49.0 35.9 53.9

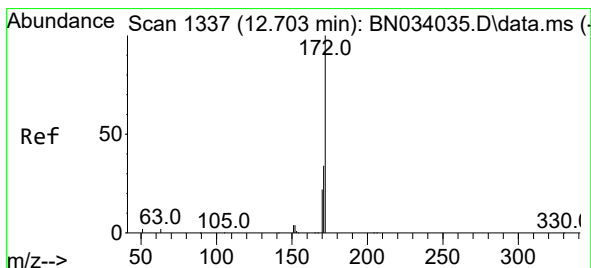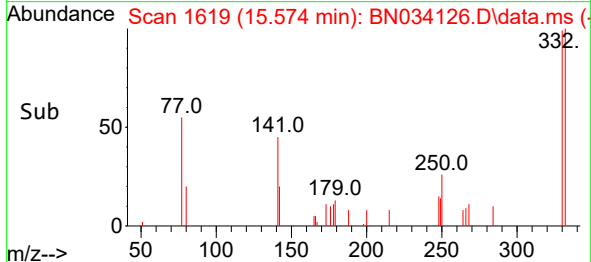

#15
2-Fluorobiphenyl
Concen: 0.360 ng
RT: 12.690 min Scan# 1350
Delta R.T. -0.013 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03

Tgt Ion:172 Resp: 13065
Ion Ratio Lower Upper
172 100
171 34.6 27.3 40.9
170 23.5 18.1 27.1


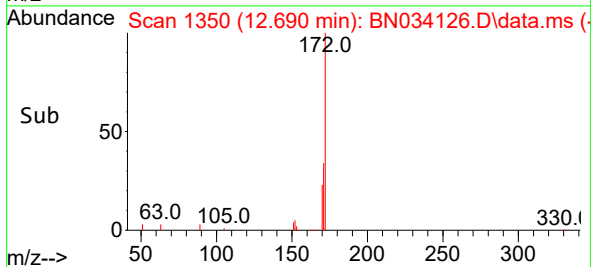

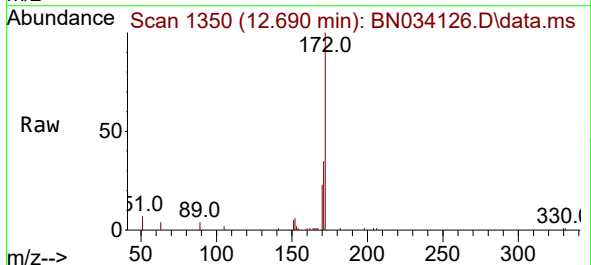


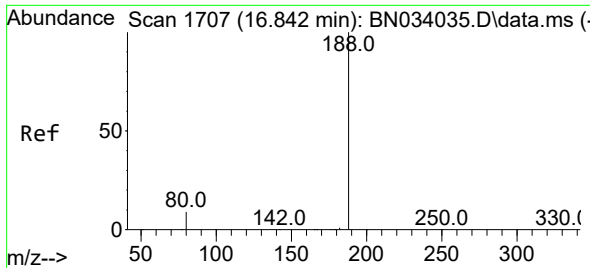

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.828 min Scan# 11
Delta R.T. -0.015 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03




Instrument :
BNA_N
ClientSampleId :
RE131D1-20240917


Tgt Ion:188 Resp: 18987
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.4 7.4 11.0#

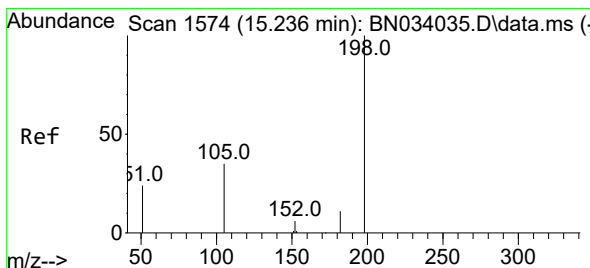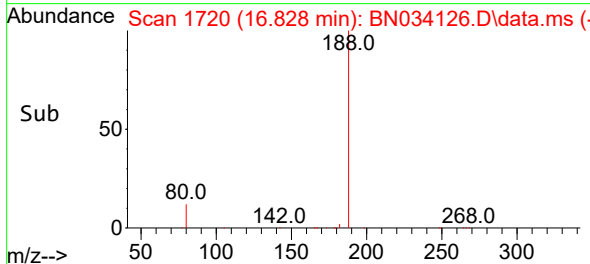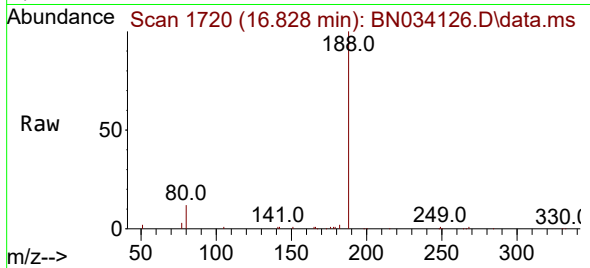

#20
4,6-Dinitro-2-methylphenol
Concen: 0.138 ng
RT: 15.234 min Scan# 1588
Delta R.T. -0.002 min
Lab File: BN034126.D
Acq: 21 Sep 2024 16:03

Tgt Ion:198 Resp: 2
Ion Ratio Lower Upper
198 100
51 563.8 106.4 159.6#
105 187.2 38.5 57.7#

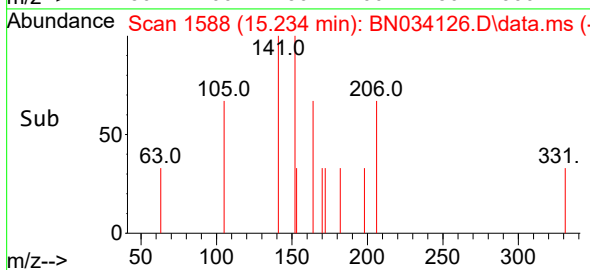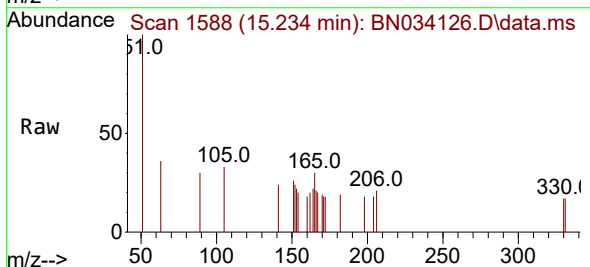

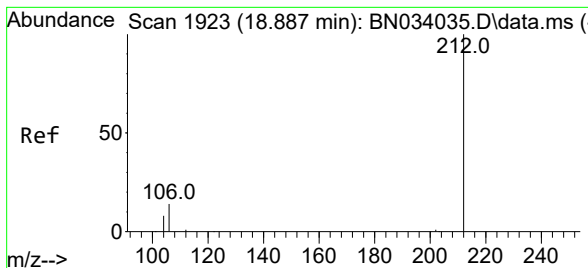

#27

Fluoranthene-d10

Concen: 0.409 ng

RT: 18.874 min Scan# 1933

Delta R.T. -0.013 min

Lab File: BN034126.D

Acq: 21 Sep 2024 16:03

Instrument :

BNA_N

ClientSampleId :

RE131D1-20240917





Tgt Ion:212 Resp: 19612

Ion Ratio Lower Upper

212 100

106 15.9 13.4 20.2

104 9.3 7.8 11.6

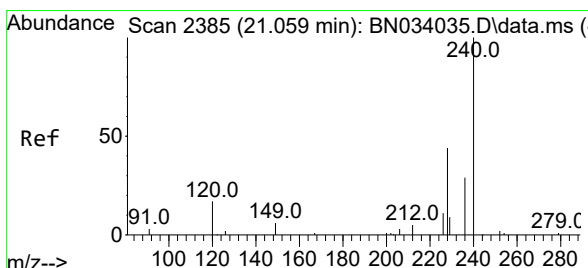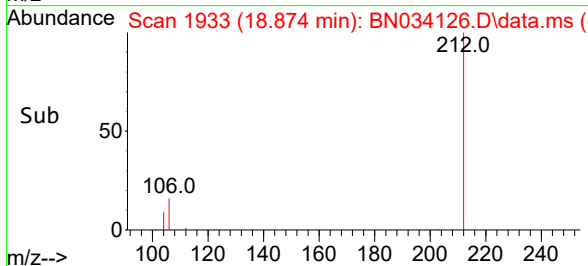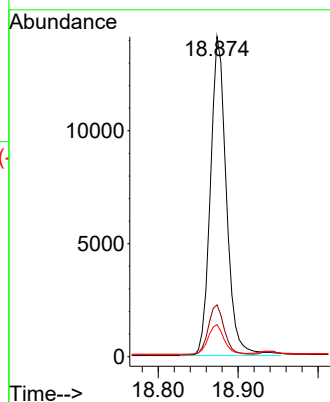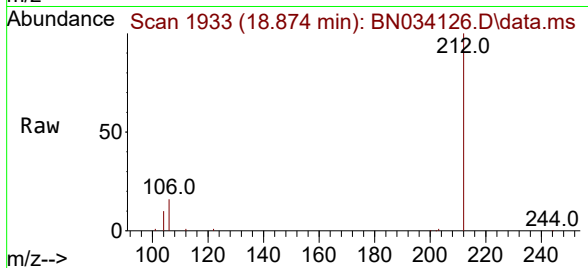

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.051 min Scan# 2397

Delta R.T. -0.008 min

Lab File: BN034126.D

Acq: 21 Sep 2024 16:03




Tgt Ion:240 Resp: 13317


Ion Ratio Lower Upper

240 100

120 14.5 13.5 20.3

236 28.7 23.4 35.0


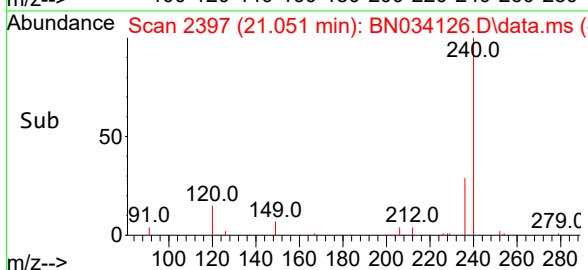
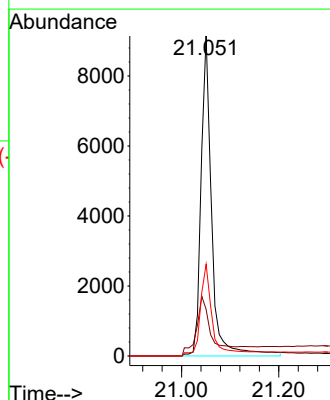
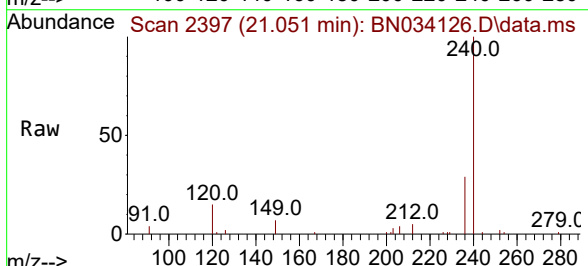


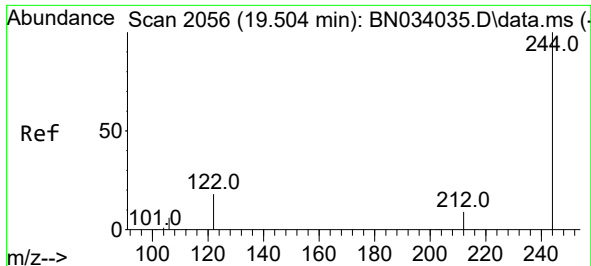

#31
 Terphenyl-d14
 Concen: 0.489 ng
 RT: 19.496 min Scan# 2056
 Delta R.T. -0.008 min
 Lab File: BN034126.D
 Acq: 21 Sep 2024 16:03




Instrument :
 BNA_N
 ClientSampleId :
 RE131D1-20240917


Tgt Ion:244 Resp: 12995
 Ion Ratio Lower Upper
 244 100
 212 10.4 7.8 11.6
 122 17.4 14.8 22.2

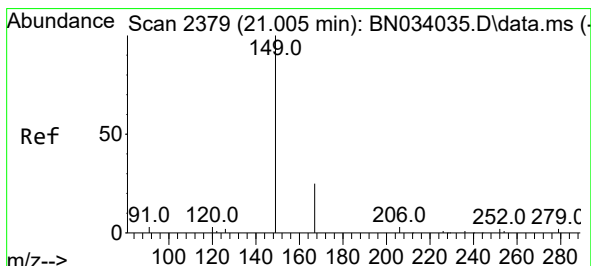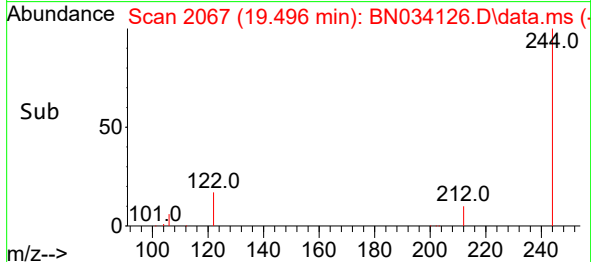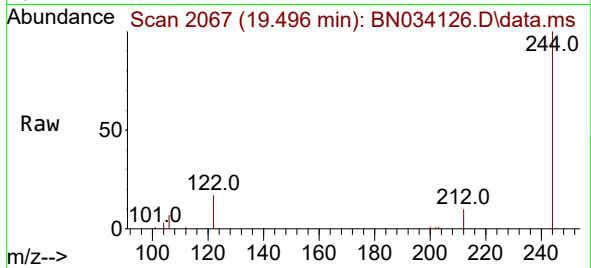

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.080 ng
 RT: 21.006 min Scan# 2392
 Delta R.T. 0.001 min
 Lab File: BN034126.D
 Acq: 21 Sep 2024 16:03


Tgt Ion:149 Resp: 1412
 Ion Ratio Lower Upper
 149 100
 167 14.7 19.9 29.9#
 279 16.9 4.6 6.8#

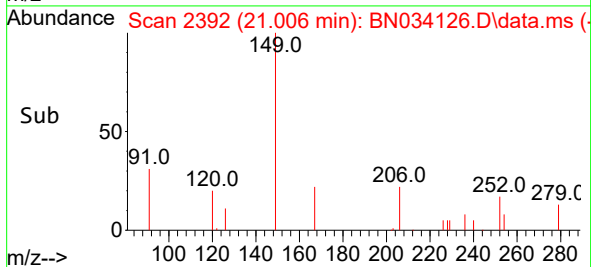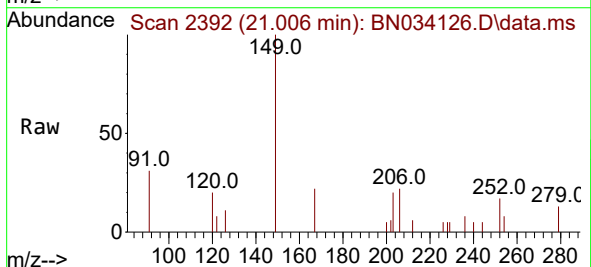

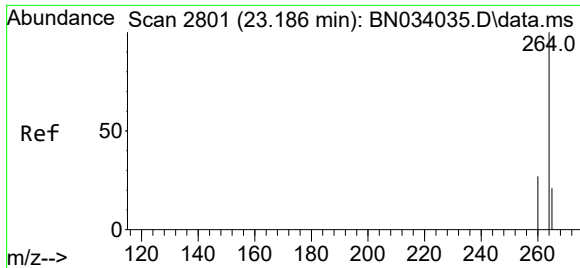

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.172 min Scan# 21
 Delta R.T. -0.014 min
 Lab File: BN034126.D
 Acq: 21 Sep 2024 16:03

Instrument :
 BNA_N
 ClientSampleId :
 RE131D1-20240917

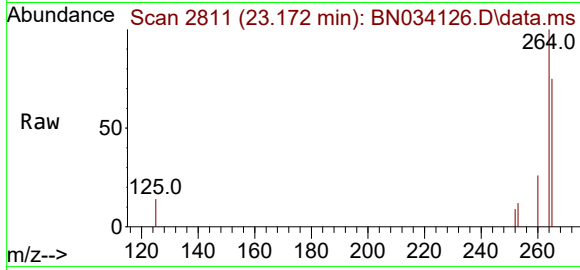

Tgt Ion:264 Resp: 10098

Ion	Ratio	Lower	Upper
264	100		
260	25.9	21.7	32.5
265	75.2	52.1	78.1

