
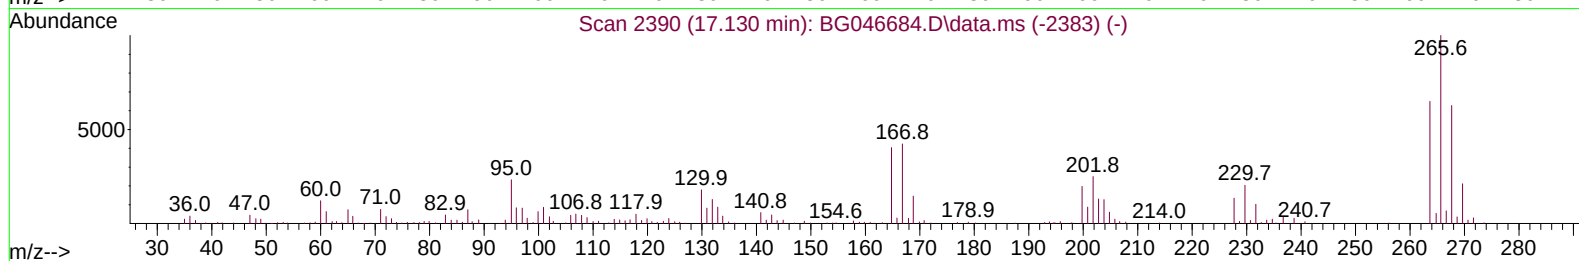
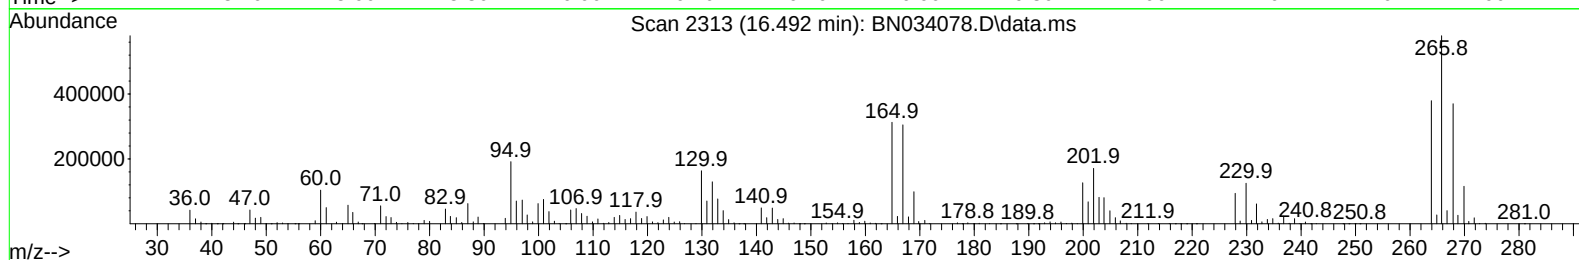


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034078.D
Acq On : 20 Sep 2024 09:36
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Sep 21 02:10:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:06:58 2024
Response via : Initial Calibration

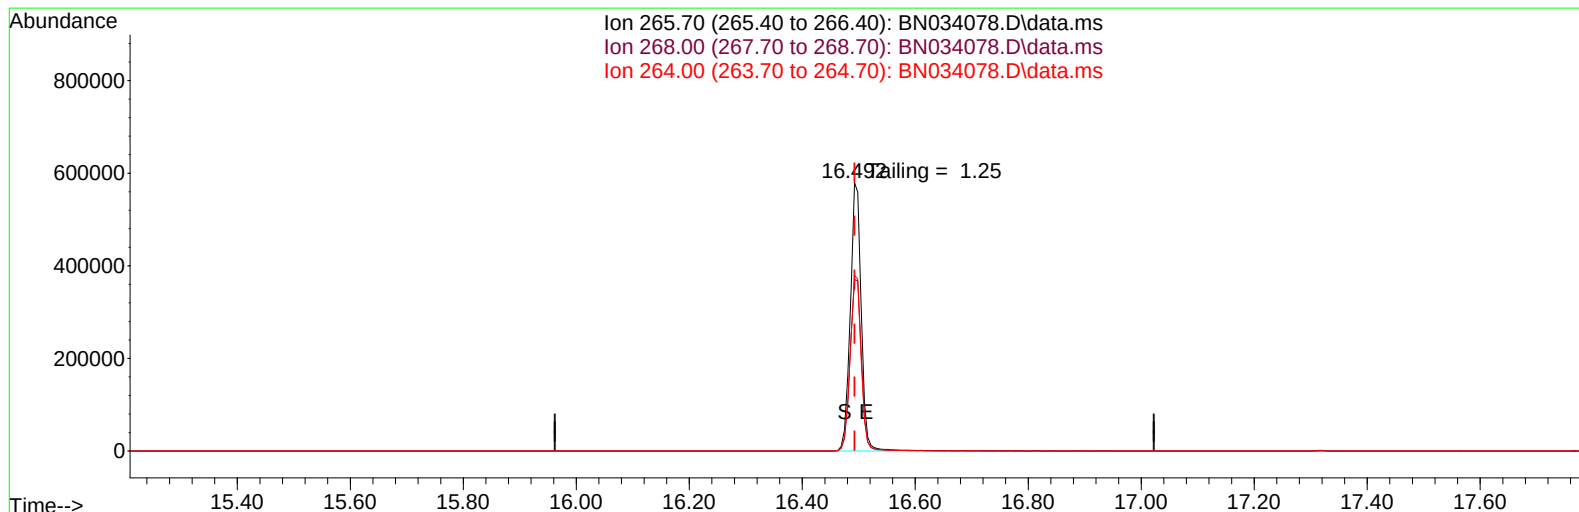

TIC: BN034078.D\data.ms

(70) Pentachlorophenol (C)




16.492min (-0.000) 24564.55 ng

response 783829

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.85
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034078.D
Acq On : 20 Sep 2024 09:36
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Sep 21 02:10:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:06:58 2024
Response via : Initial Calibration

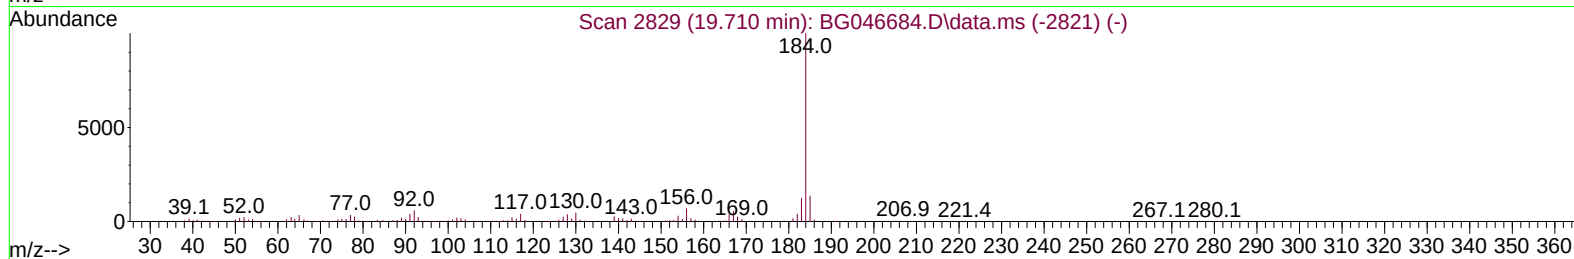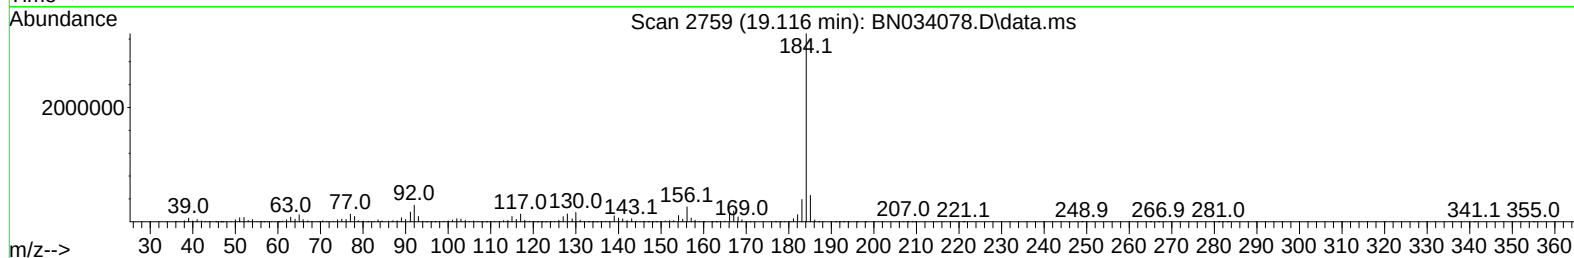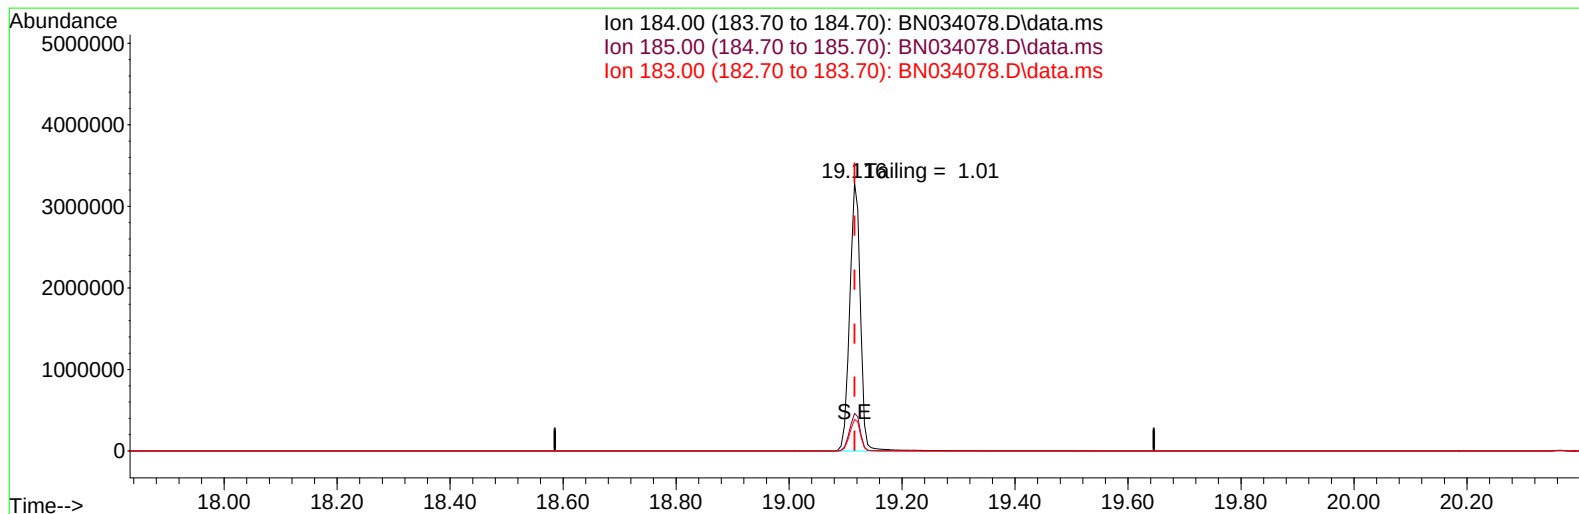

TIC: BN034078.D\data.ms

(77) Benzidine

19.116min (-0.000) 0.00 ng

response 4330600

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	11.84
0.00	0.00	0.00