
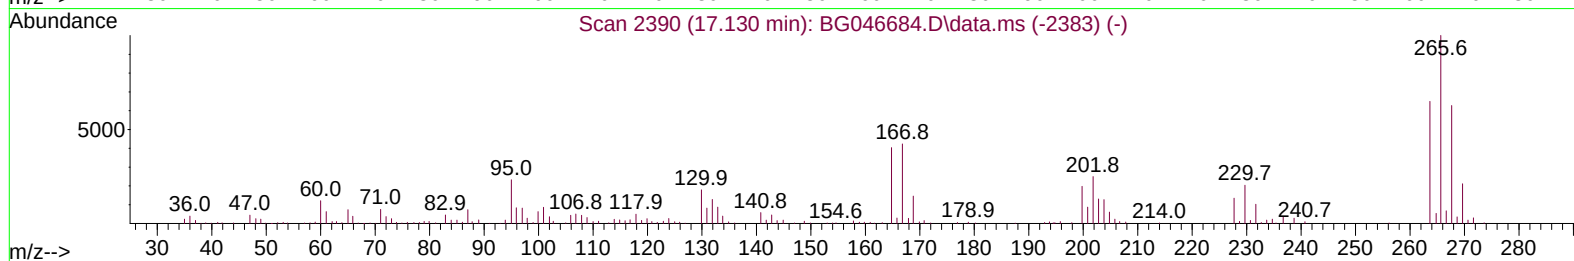
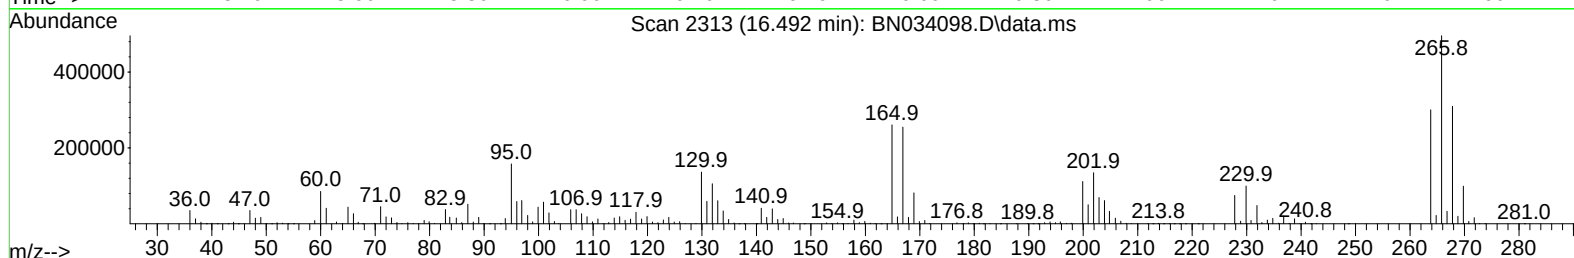


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034098.D
Acq On : 20 Sep 2024 22:24
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Quant Time: Sep 21 02:07:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:06:58 2024
Response via : Initial Calibration

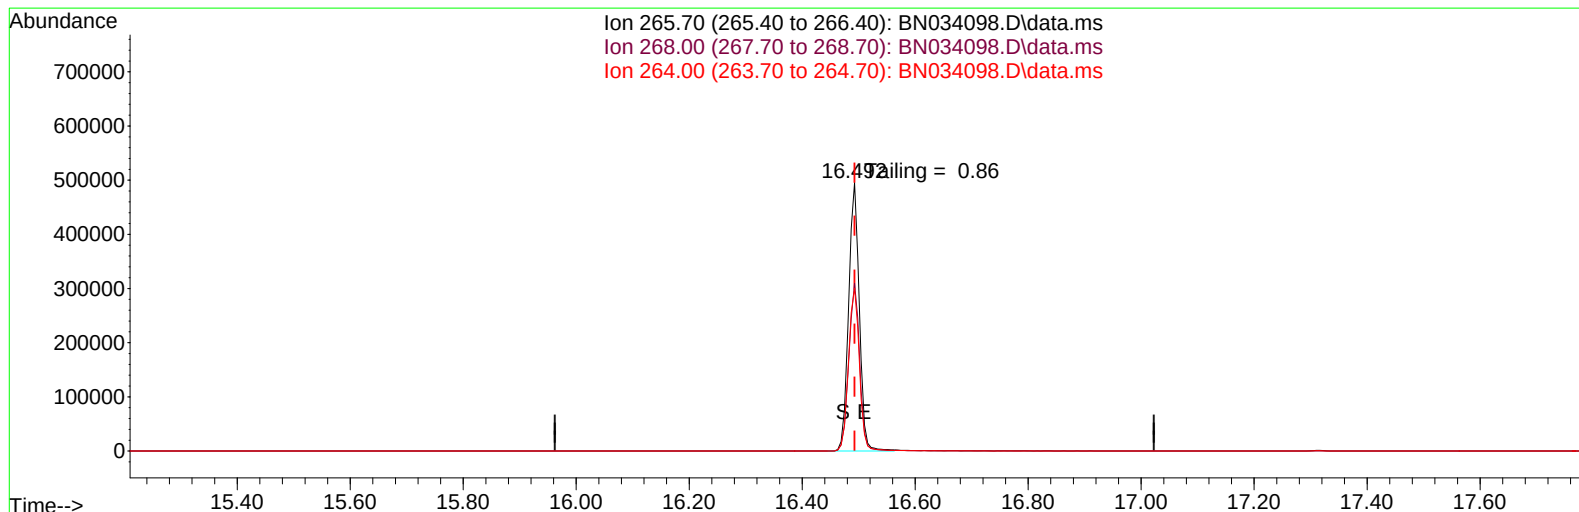

TIC: BN034098.D\data.ms

(70) Pentachlorophenol (C)




16.492min (0.000) 23726.54 ng

response 655610

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.52
264.00	61.60	60.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034098.D
Acq On : 20 Sep 2024 22:24
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 61 Sample Multiplier: 1

Quant Time: Sep 21 02:07:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:06:58 2024
Response via : Initial Calibration

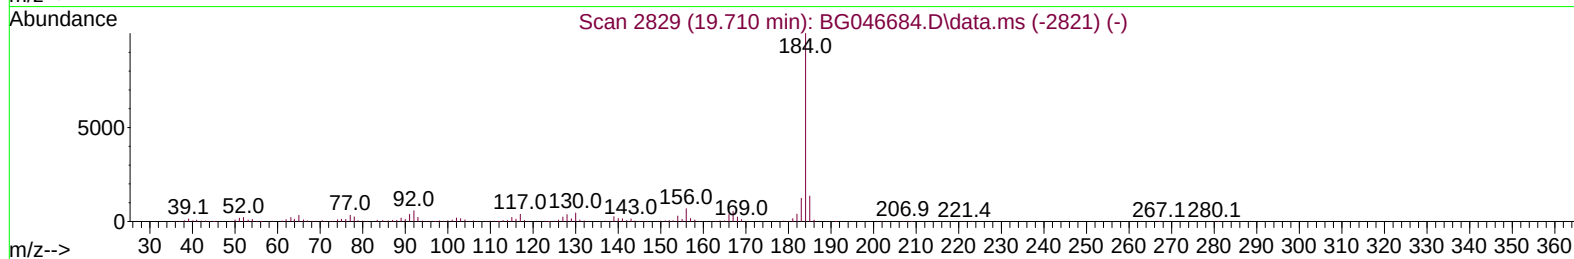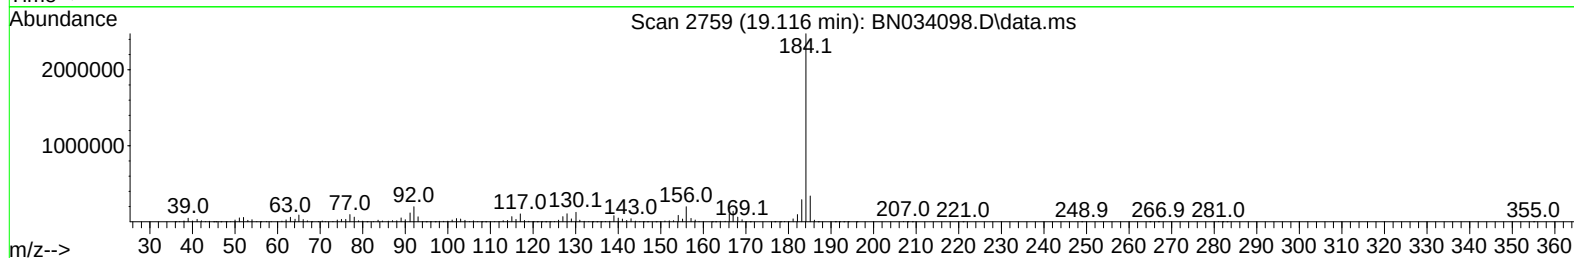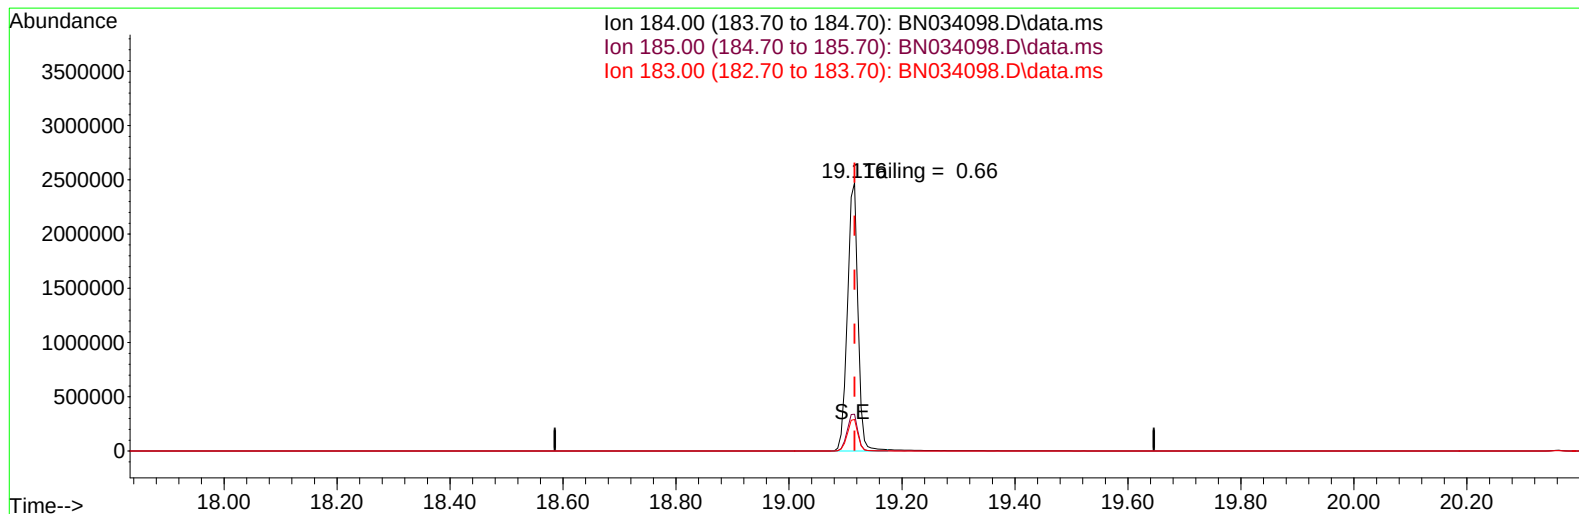

TIC: BN034098.D\data.ms

(77) Benzidine

19.116min (0.000) 0.00 ng

response 3222864

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.74
183.00	13.20	11.73
0.00	0.00	0.00