
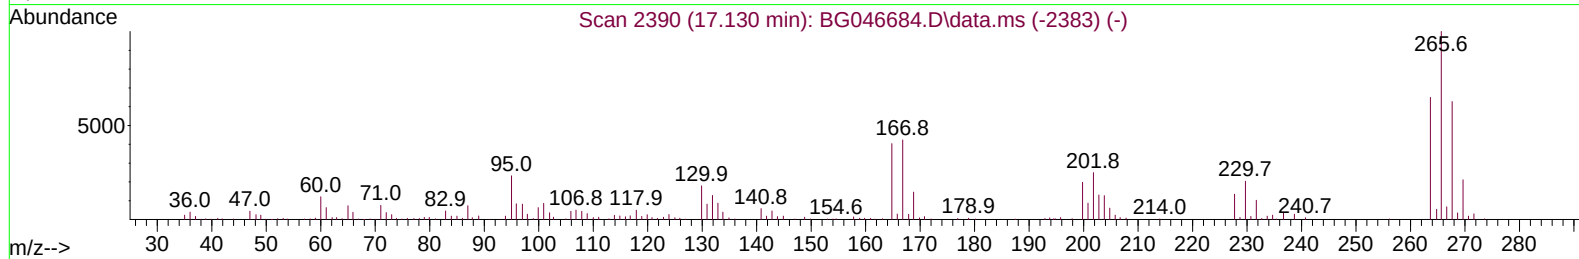
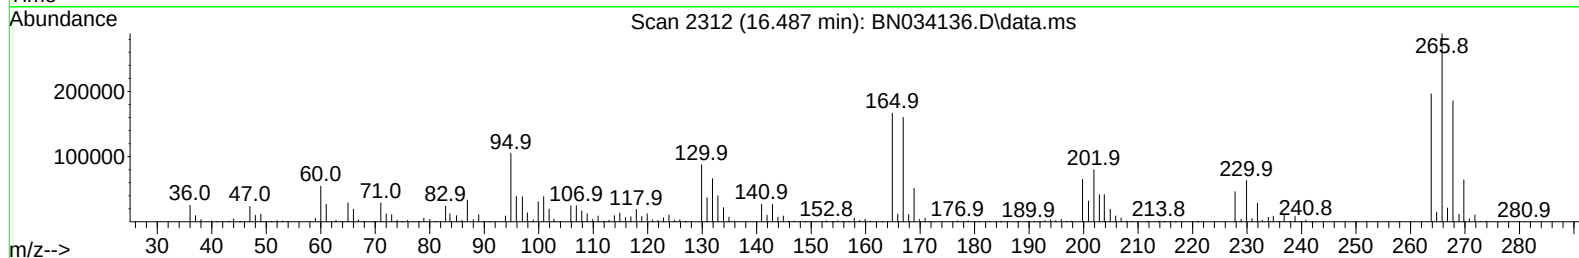


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034136.D
Acq On : 21 Sep 2024 22:43
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 101 Sample Multiplier: 1

Quant Time: Sep 23 01:15:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

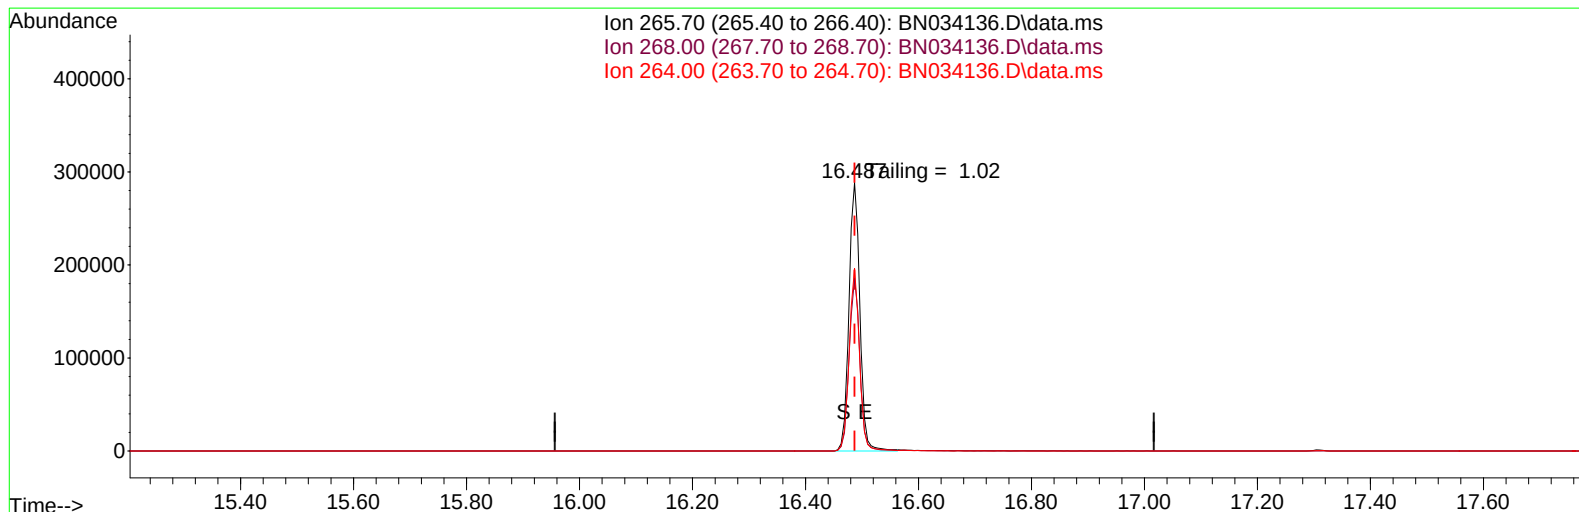

TIC: BN034136.D\data.ms

(70) Pentachlorophenol (C)




16.487min (+ 0.000) 18362.98 ng

response 389524

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.31
264.00	61.60	68.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034136.D
Acq On : 21 Sep 2024 22:43
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 101 Sample Multiplier: 1

Quant Time: Sep 23 01:15:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 01:13:26 2024
Response via : Initial Calibration

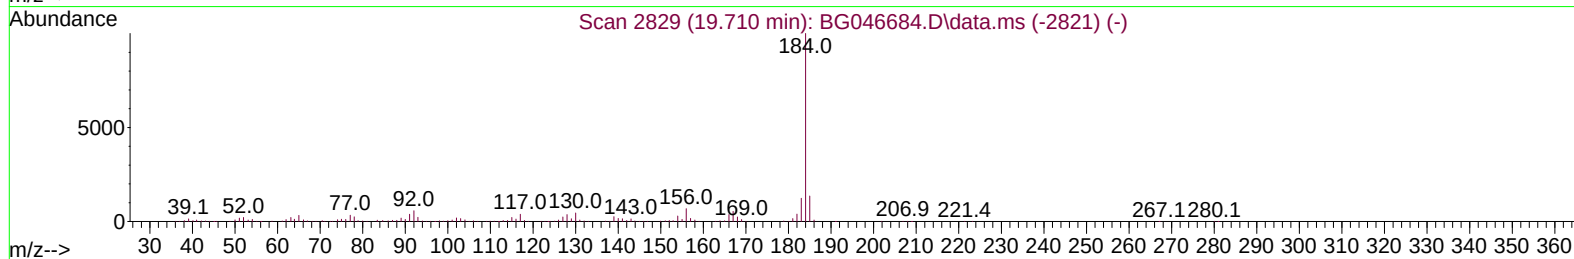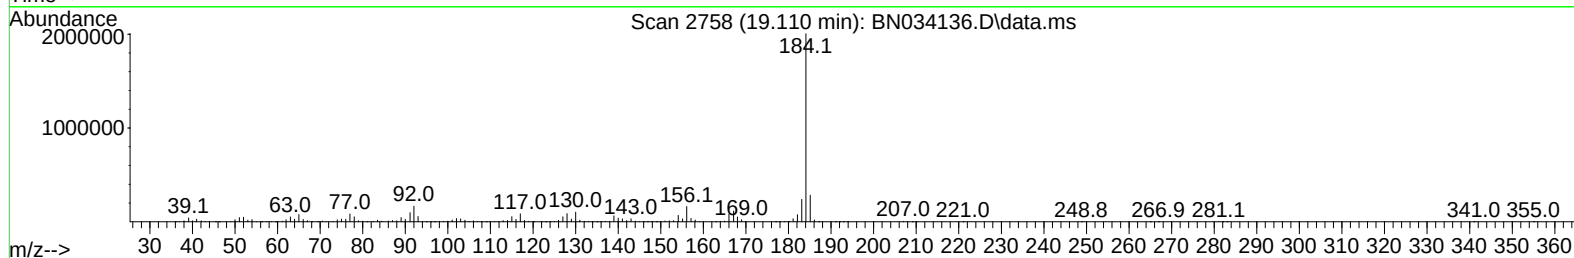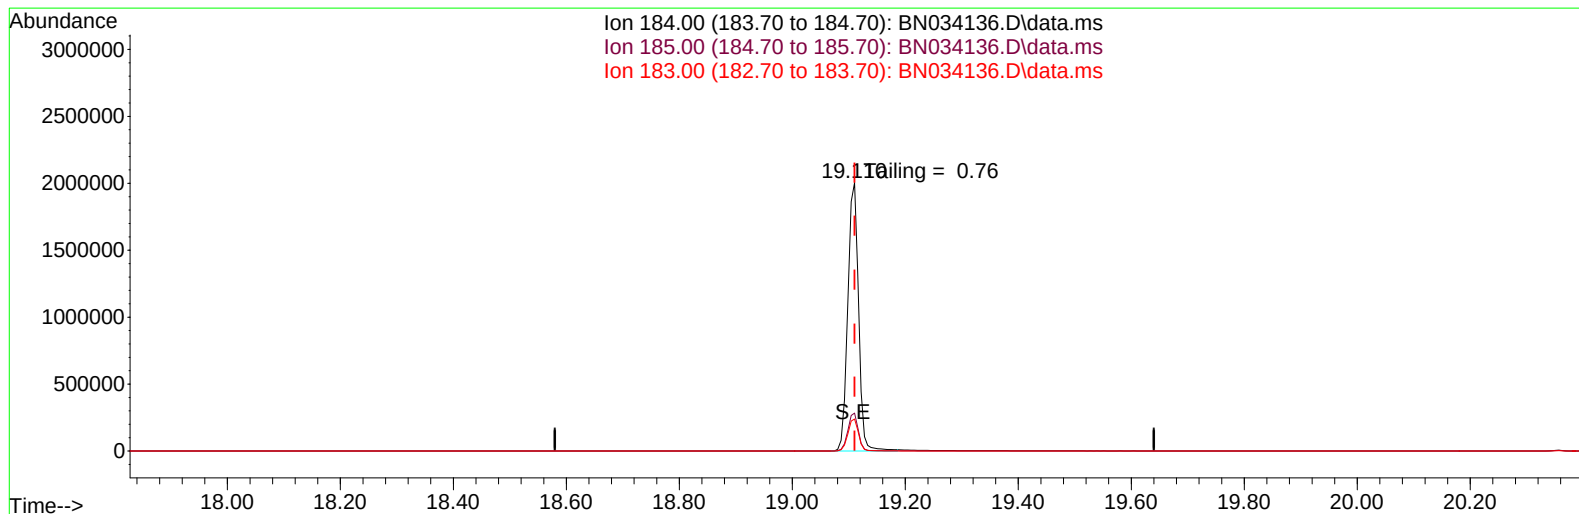

TIC: BN034136.D\data.ms

(77) Benzidine**19.110min (+ 0.000) 0.00 ng****response 2674968**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	11.94
0.00	0.00	0.00