

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
 Data File : BN034146.D
 Acq On : 22 Sep 2024 04:47
 Operator : JU/RC
 Sample : P4111-04
 Misc :
 ALS Vial : 111 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RW7-SP303-20240918

Quant Time: Sep 23 00:03:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 16:09:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.423	152	5454	0.400	ng	-0.01
7) Naphthalene-d8	10.180	136	14644	0.400	ng	#-0.02
13) Acenaphthene-d10	14.069	164	8075	0.400	ng	-0.01
19) Phenanthrene-d10	16.828	188	15340	0.400	ng	#-0.01
29) Chrysene-d12	21.051	240	10264	0.400	ng	# 0.00
35) Perylene-d12	23.169	264	9401	0.400	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.069	112	1970	0.127	ng	0.00
5) Phenol-d6	6.622	99	1222	0.068	ng	-0.01
8) Nitrobenzene-d5	8.568	82	3312	0.296	ng	0.00
11) 2-Methylnaphthalene-d10	11.784	152	6606	0.305	ng	0.00
14) 2,4,6-Tribromophenol	15.574	330	766	0.209	ng	-0.01
15) 2-Fluorobiphenyl	12.690	172	10186	0.310	ng	-0.01
27) Fluoranthene-d10	18.874	212	13674	0.353	ng	-0.01
31) Terphenyl-d14	19.491	244	8903	0.434	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.076	88	505	0.074	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034146.D
Acq On : 22 Sep 2024 04:47
Operator : JU/RC
Sample : P4111-04
Misc :
ALS Vial : 111 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RW7-SP303-20240918


Quant Time: Sep 23 00:03:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 16:09:28 2024
Response via : Initial Calibration

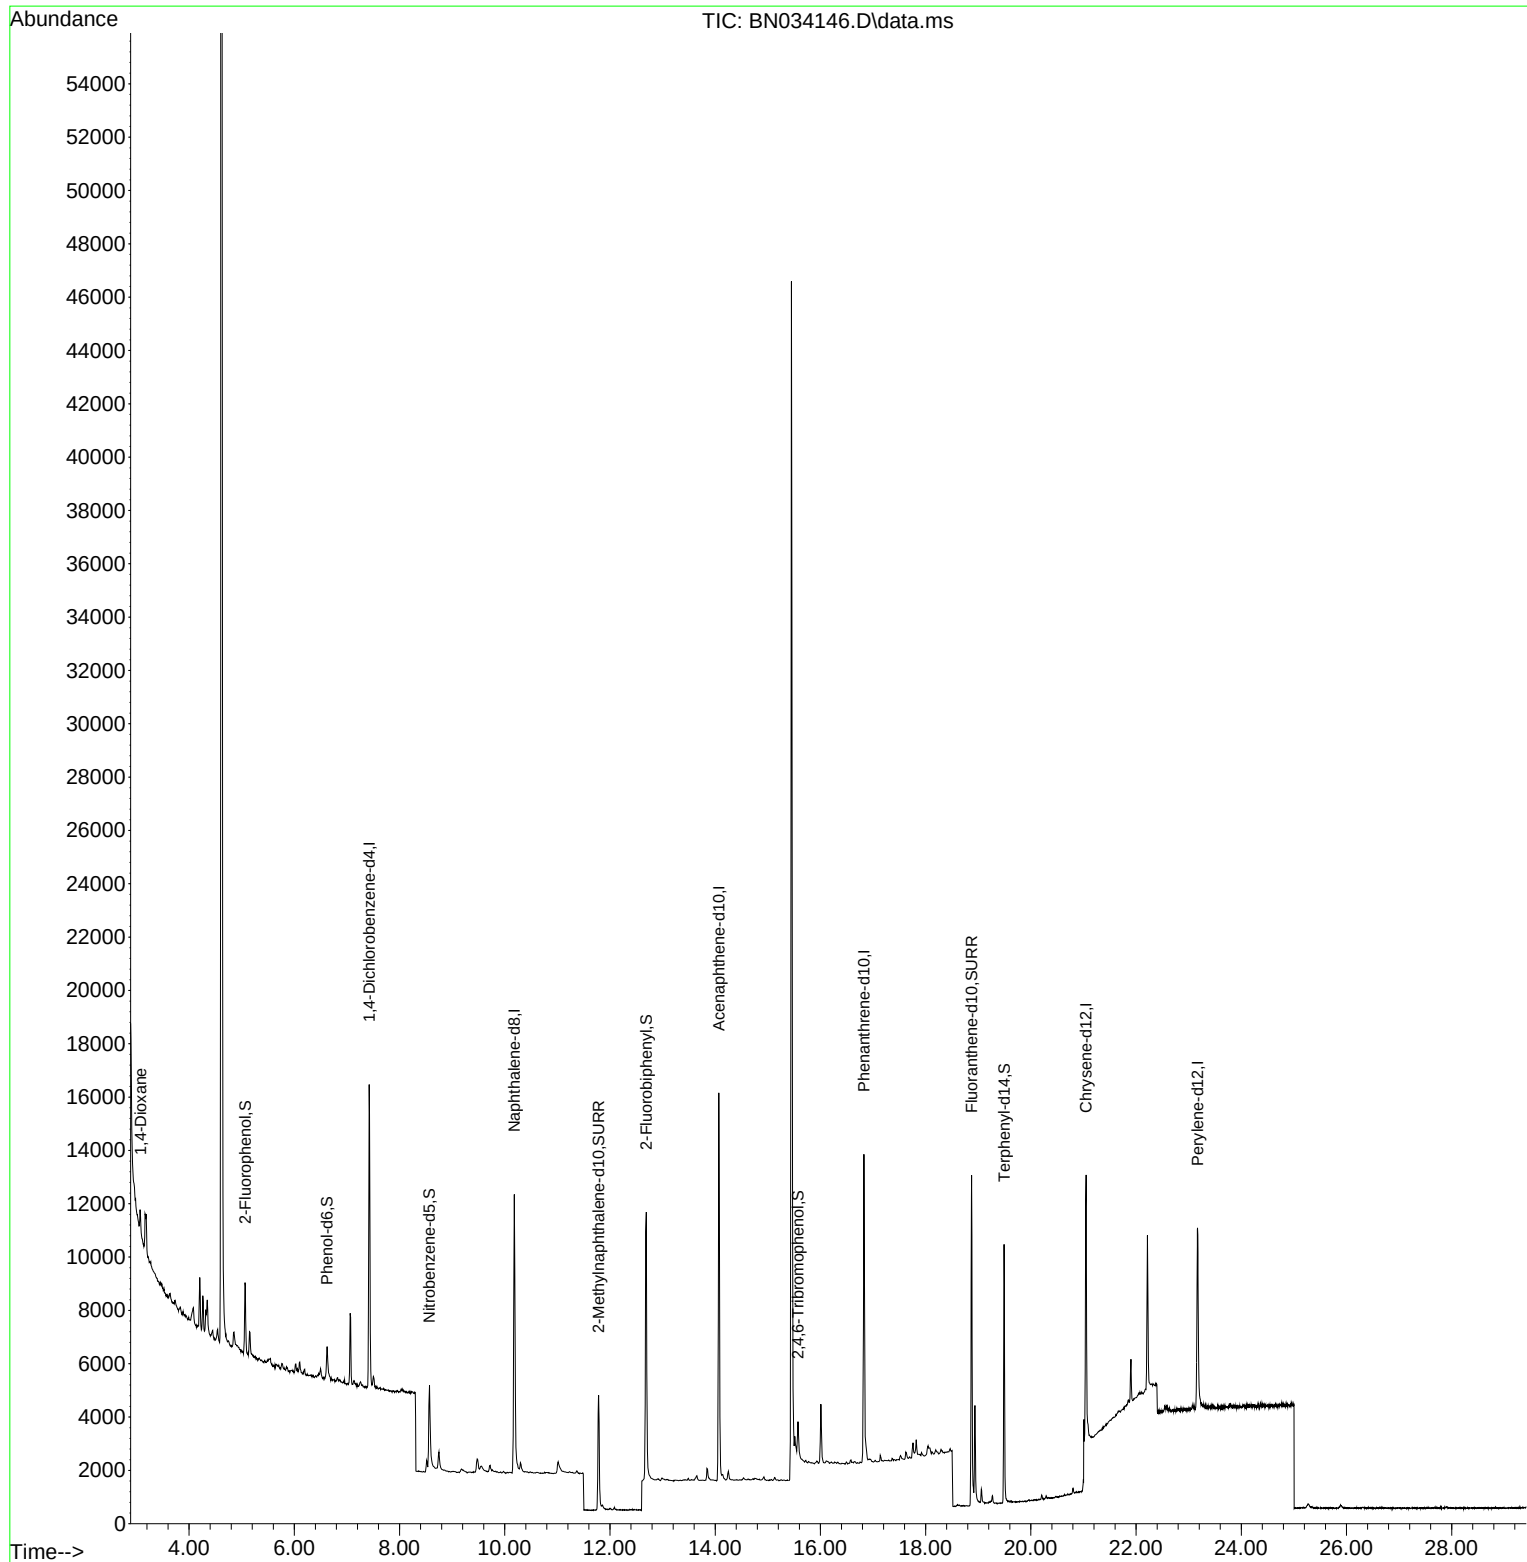



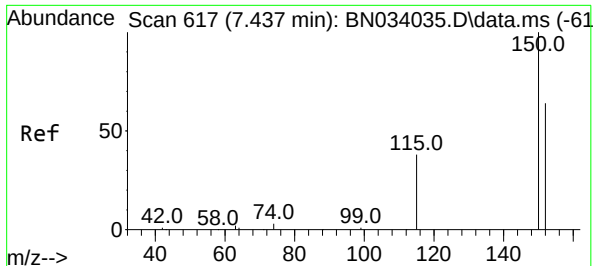


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.423 min Scan# 61
 Delta R.T. -0.014 min
 Lab File: BN034146.D
 Acq: 22 Sep 2024 04:47


Instrument :
 BNA_N
 ClientSampleId :
 RW7-SP303-20240918

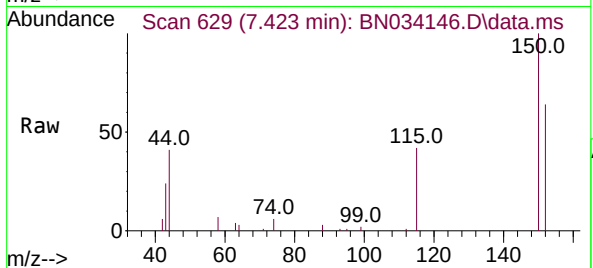



Tgt Ion:152 Resp: 5454
 Ion Ratio Lower Upper
 152 100
 150 156.6 124.6 187.0
 115 65.5 50.0 75.0

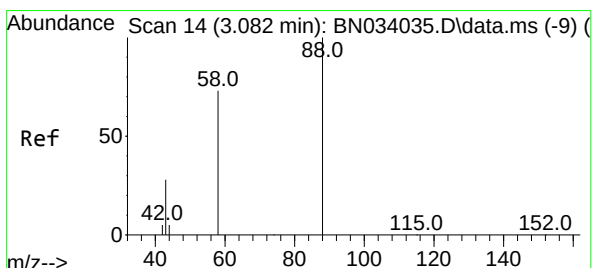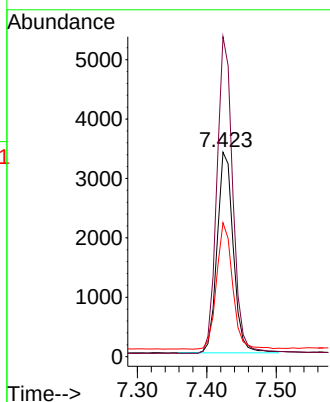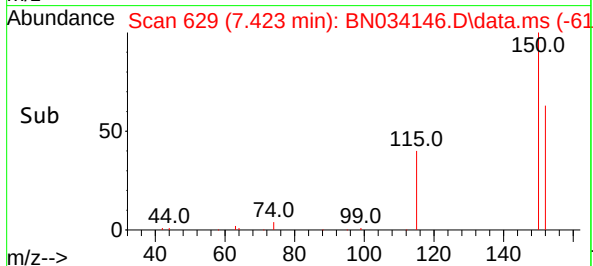


#2
 1,4-Dioxane
 Concen: 0.074 ng
 RT: 3.076 min Scan# 27
 Delta R.T. -0.006 min
 Lab File: BN034146.D
 Acq: 22 Sep 2024 04:47

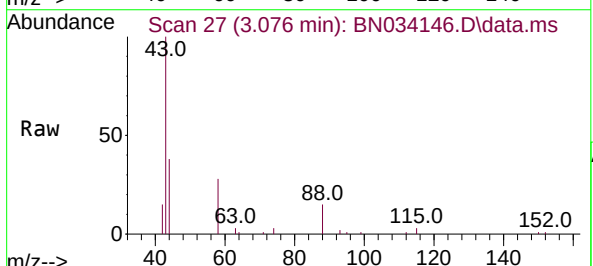

Tgt Ion: 88 Resp: 505
 Ion Ratio Lower Upper
 88 100
 43 243.2 25.8 38.8#
 58 89.1 58.8 88.2#



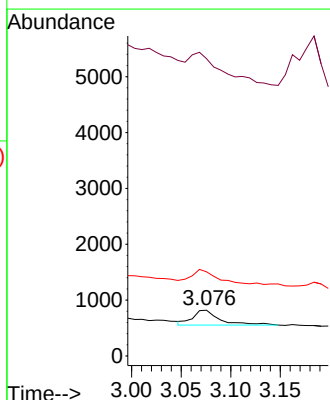
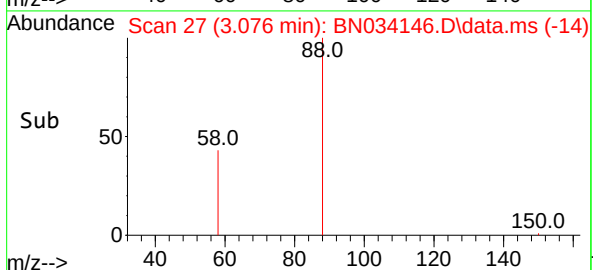


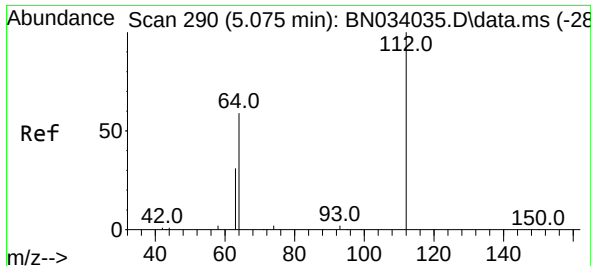

#4
2-Fluorophenol
Concen: 0.127 ng
RT: 5.069 min Scan# 30
Delta R.T. -0.006 min
Lab File: BN034146.D
Acq: 22 Sep 2024 04:47




Instrument :
BNA_N
ClientSampleId :
RW7-SP303-20240918


Tgt Ion:112 Resp: 1970
Ion Ratio Lower Upper
112 100
64 64.4 48.6 72.8
63 36.6 25.6 38.4

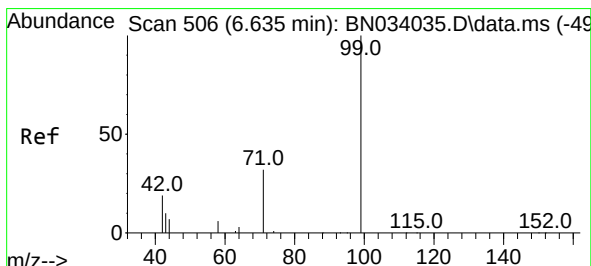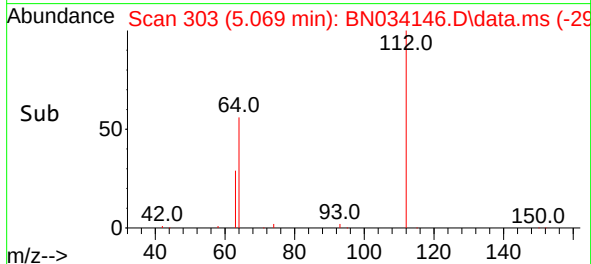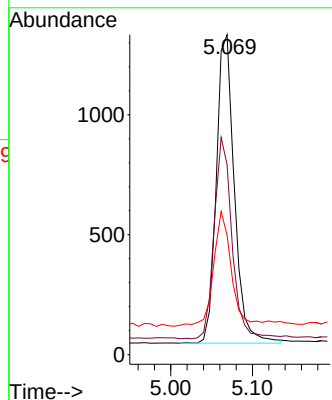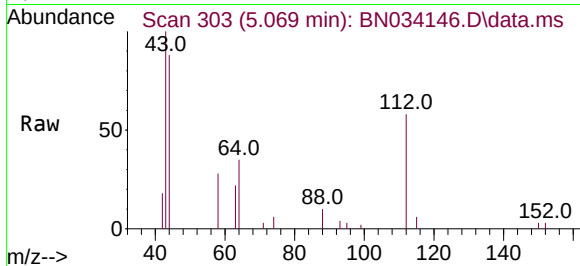

#5
Phenol-d6
Concen: 0.068 ng
RT: 6.622 min Scan# 518
Delta R.T. -0.013 min
Lab File: BN034146.D
Acq: 22 Sep 2024 04:47

Tgt Ion: 99 Resp: 1222
Ion Ratio Lower Upper
99 100
42 32.5 17.8 26.8#
71 43.9 26.2 39.2#

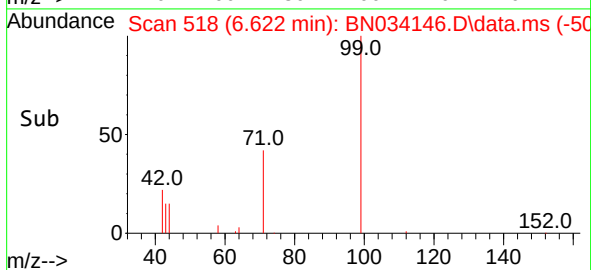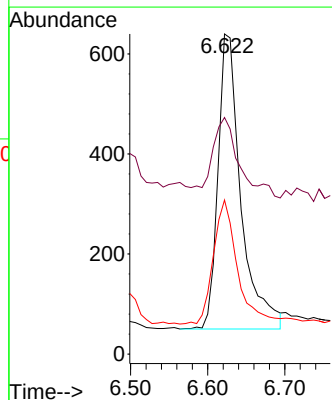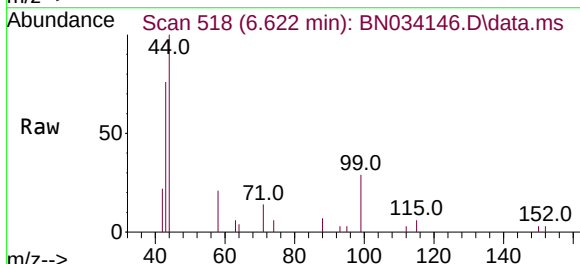

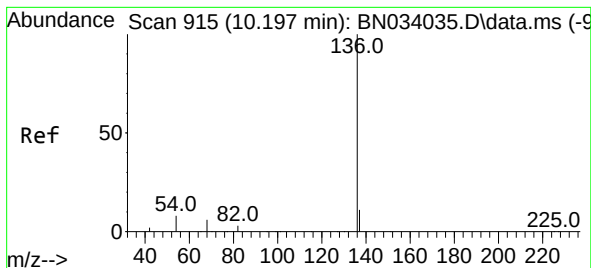

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.180 min Scan# 915

Delta R.T. -0.017 min

Lab File: BN034146.D

Acq: 22 Sep 2024 04:47

Instrument :

BNA_N

ClientSampleId :

RW7-SP303-20240918

Tgt Ion:136 Resp: 14644





Ion Ratio Lower Upper

136 100

137 11.4 9.0 13.6

54 11.2 6.8 10.2#

68 7.0 5.0 7.6

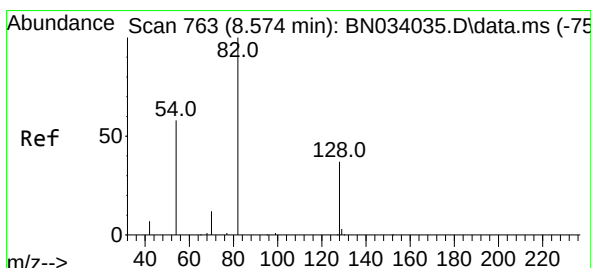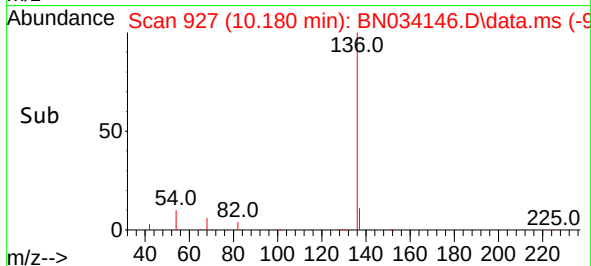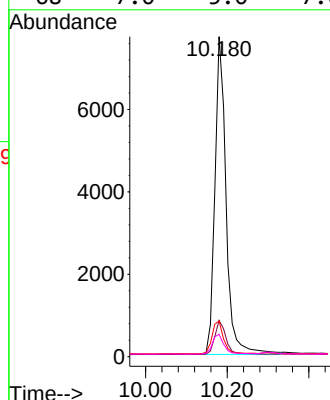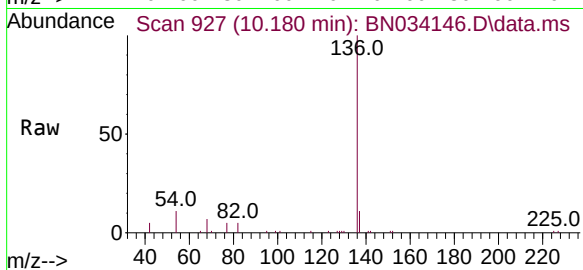

#8

Nitrobenzene-d5

Concen: 0.296 ng

RT: 8.568 min Scan# 776

Delta R.T. -0.006 min

Lab File: BN034146.D

Acq: 22 Sep 2024 04:47




Tgt Ion: 82 Resp: 3312


Ion Ratio Lower Upper

82 100

128 44.2 31.4 47.2

54 60.1 47.4 71.0


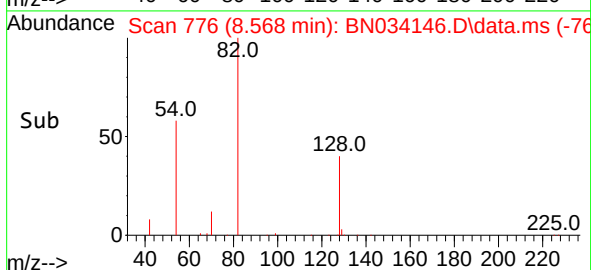
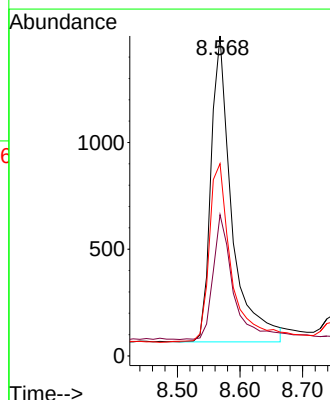
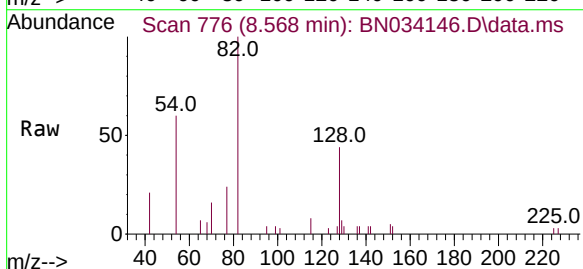


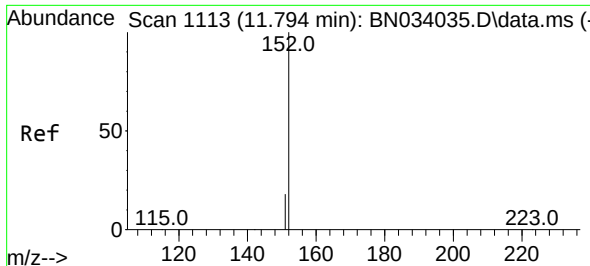

#11
2-Methylnaphthalene-d10
Concen: 0.305 ng
RT: 11.784 min Scan# 1113
Delta R.T. -0.010 min
Lab File: BN034146.D
Acq: 22 Sep 2024 04:47




Instrument :
BNA_N
ClientSampleId :
RW7-SP303-20240918


Tgt Ion:152 Resp: 6606
Ion Ratio Lower Upper
152 100
151 21.5 16.8 25.2

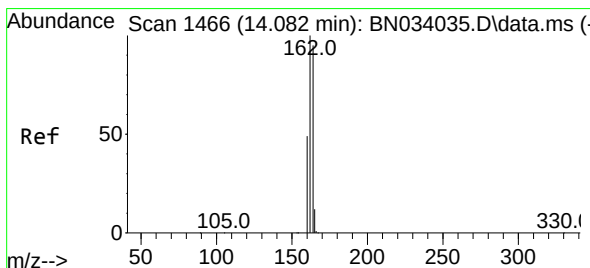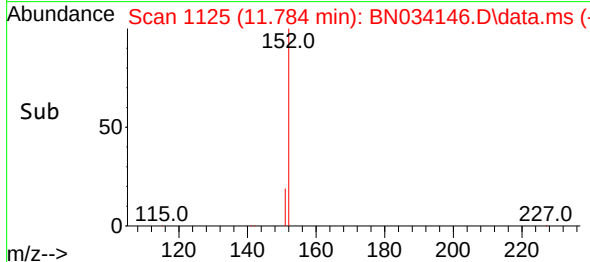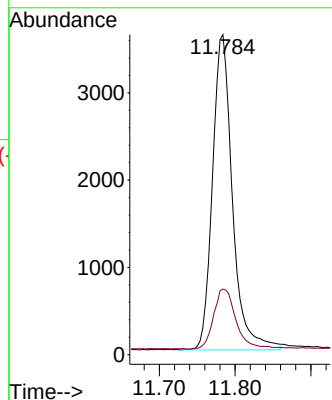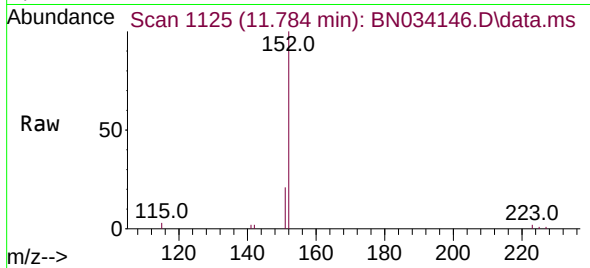

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.069 min Scan# 1479
Delta R.T. -0.013 min
Lab File: BN034146.D
Acq: 22 Sep 2024 04:47


Tgt Ion:164 Resp: 8075
Ion Ratio Lower Upper
164 100
162 106.2 84.2 126.2
160 52.4 41.7 62.5

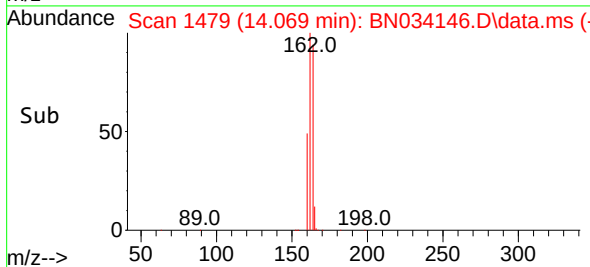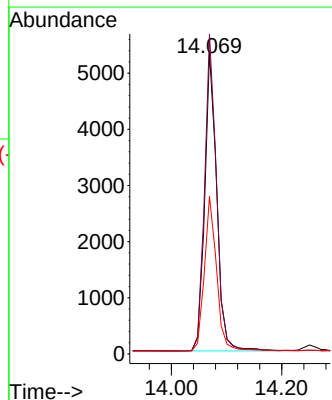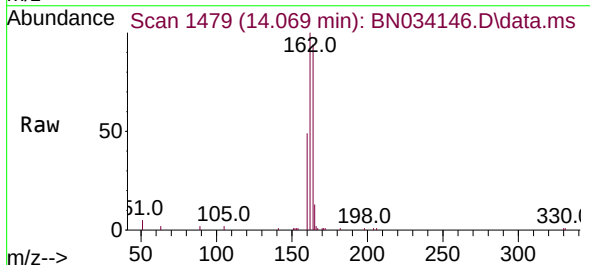



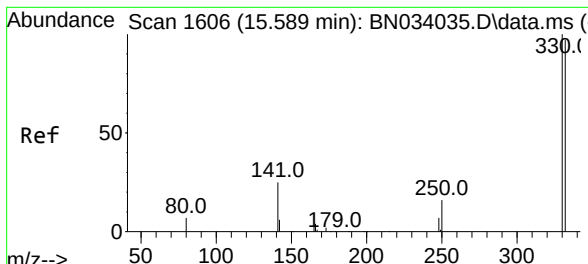


#14
 2,4,6-Tribromophenol
 Concen: 0.209 ng
 RT: 15.574 min Scan# 1
 Delta R.T. -0.015 min
 Lab File: BN034146.D
 Acq: 22 Sep 2024 04:47

Instrument :
 BNA_N
 ClientSampleId :
 RW7-SP303-20240918



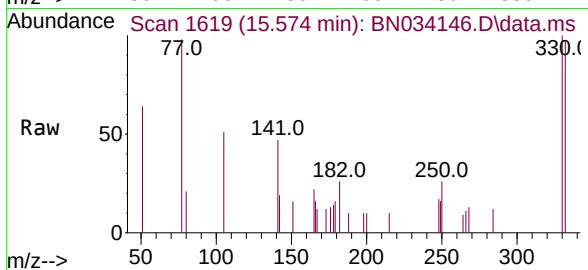



Tgt Ion:330 Resp: 766
 Ion Ratio Lower Upper
 330 100
 332 158.5 77.4 116.0#
 141 45.0 35.9 53.9

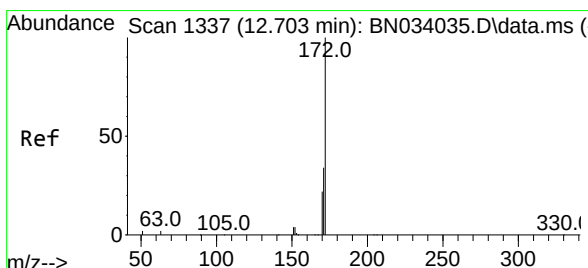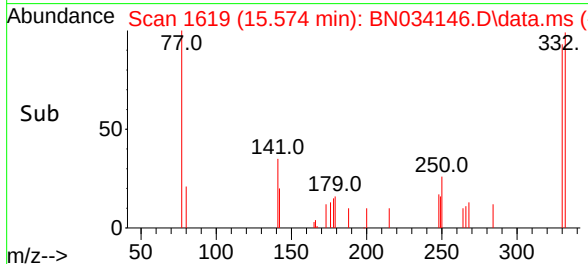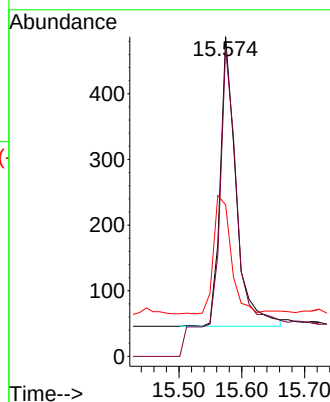

#15
 2-Fluorobiphenyl
 Concen: 0.310 ng
 RT: 12.690 min Scan# 1350
 Delta R.T. -0.013 min
 Lab File: BN034146.D
 Acq: 22 Sep 2024 04:47

Tgt Ion:172 Resp: 10186
 Ion Ratio Lower Upper
 172 100
 171 34.7 27.3 40.9
 170 22.8 18.1 27.1


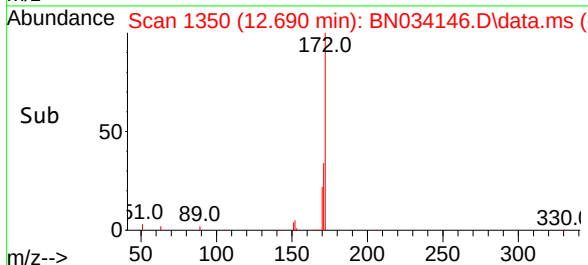
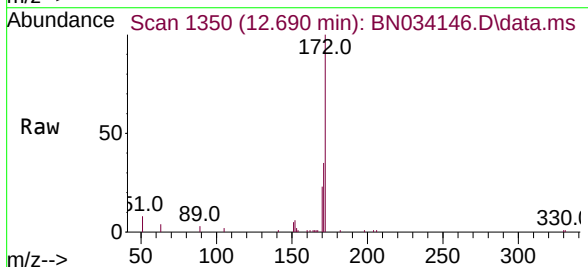
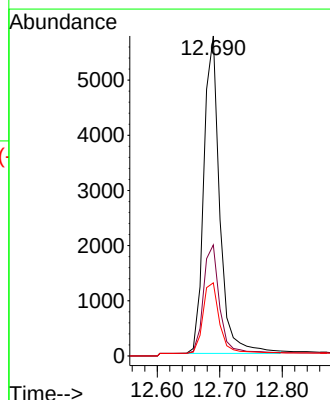


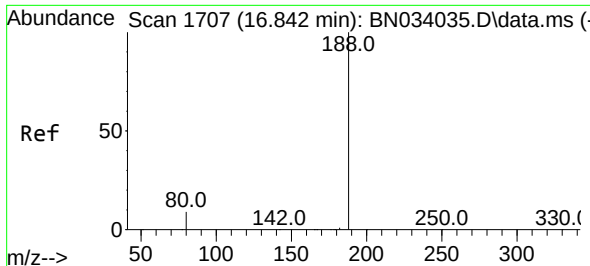

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.828 min Scan# 11
Delta R.T. -0.015 min
Lab File: BN034146.D
Acq: 22 Sep 2024 04:47




Instrument :
BNA_N
ClientSampleId :
RW7-SP303-20240918


Tgt Ion:188 Resp: 15340
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.5 7.4 11.0#

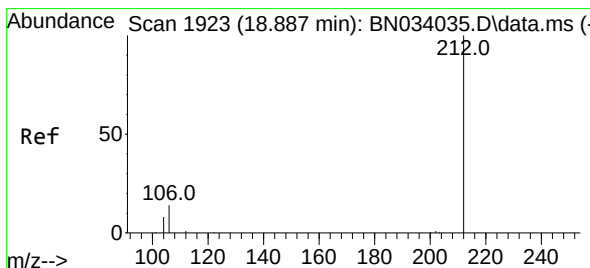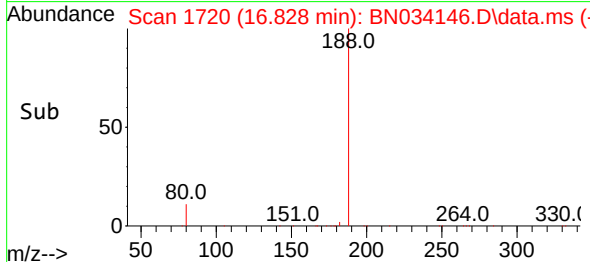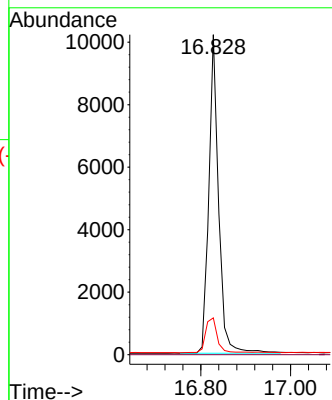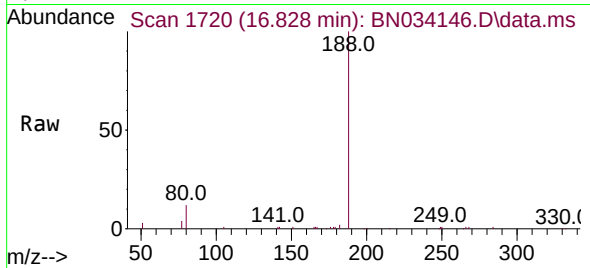

#27
Fluoranthene-d10
Concen: 0.353 ng
RT: 18.874 min Scan# 1933
Delta R.T. -0.013 min
Lab File: BN034146.D
Acq: 22 Sep 2024 04:47

Tgt Ion:212 Resp: 13674
Ion Ratio Lower Upper
212 100
106 16.1 13.4 20.2
104 9.1 7.8 11.6

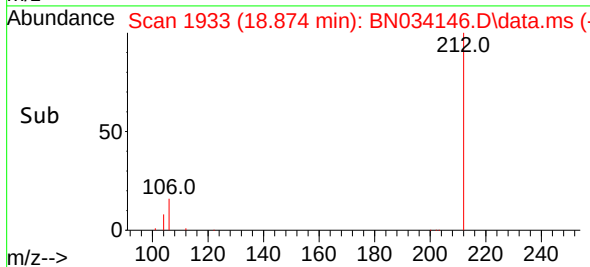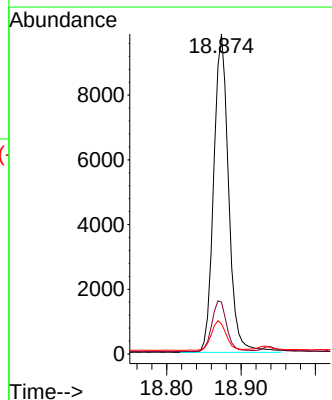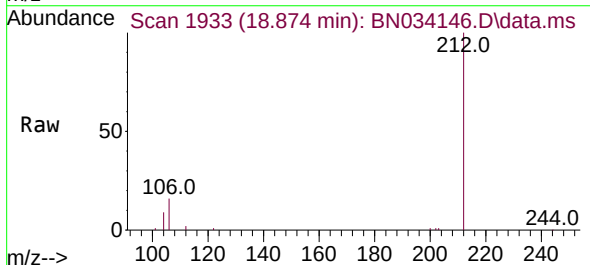

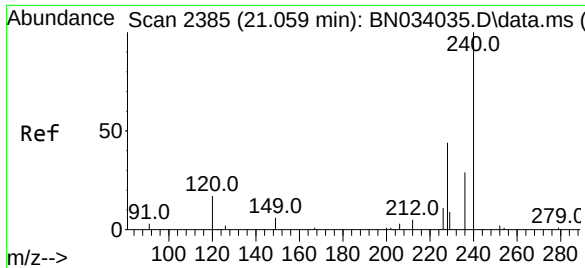

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.051 min Scan# 21

Delta R.T. -0.008 min

Lab File: BN034146.D

Acq: 22 Sep 2024 04:47

Instrument :

BNA_N

ClientSampleId :

RW7-SP303-20240918





Tgt Ion:240 Resp: 10264

Ion Ratio Lower Upper

240 100

120 13.5 13.5 20.3#

236 29.1 23.4 35.0

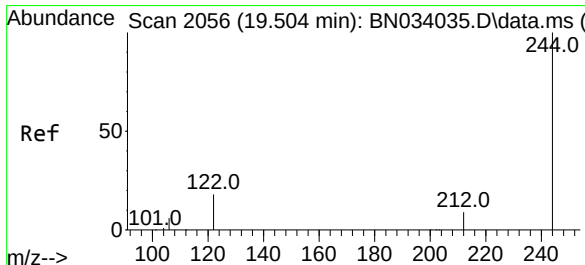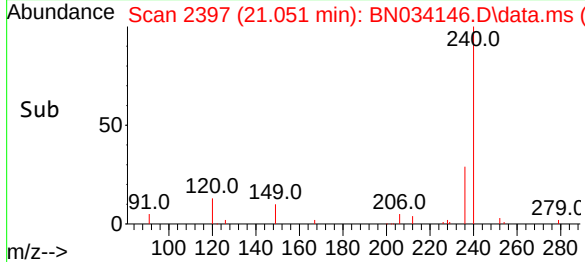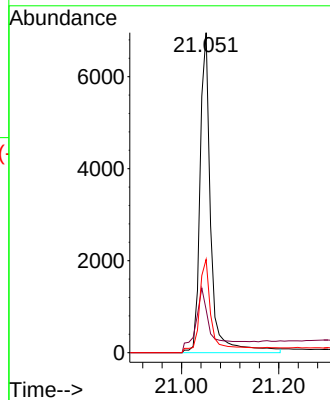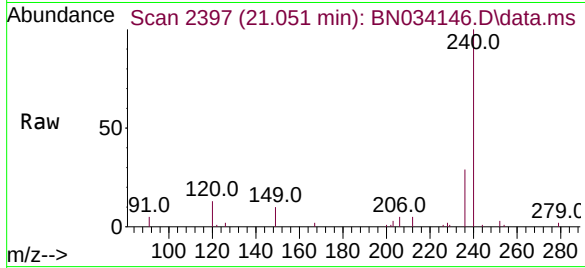

#31

Terphenyl-d14

Concen: 0.434 ng

RT: 19.491 min Scan# 2066

Delta R.T. -0.013 min

Lab File: BN034146.D

Acq: 22 Sep 2024 04:47




Tgt Ion:244 Resp: 8903


Ion Ratio Lower Upper

244 100

212 10.8 7.8 11.6


122 19.6 14.8 22.2

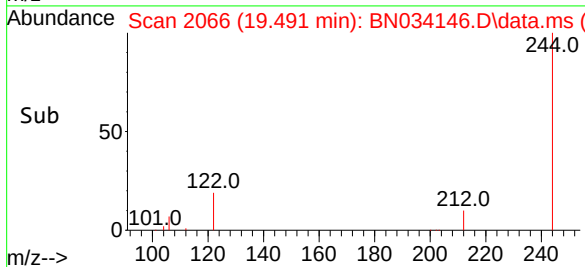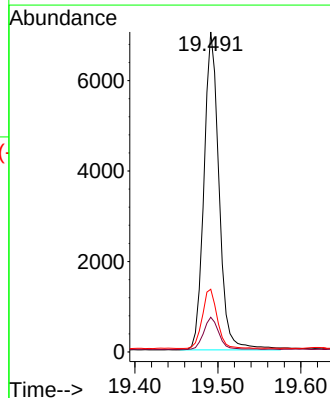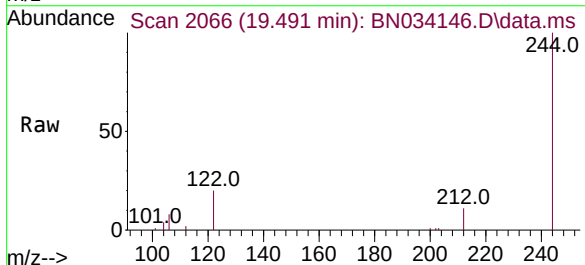

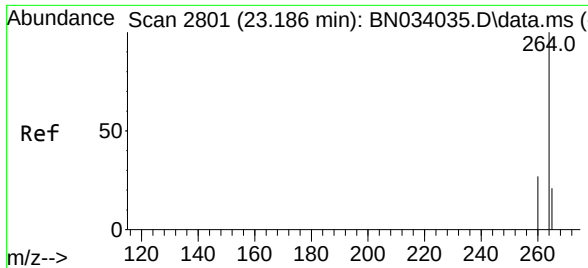

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.169 min Scan# 2810
Delta R.T. -0.017 min
Lab File: BN034146.D
Acq: 22 Sep 2024 04:47

Instrument :
BNA_N
ClientSampleId :
RW7-SP303-20240918

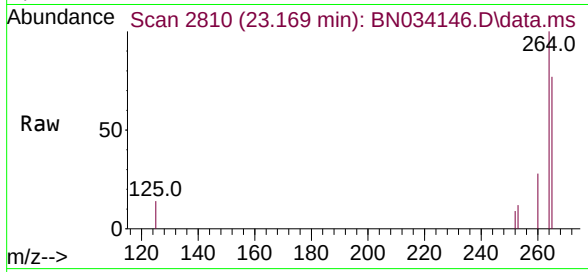

Tgt Ion:264 Resp: 9401
Ion Ratio Lower Upper
264 100
260 27.6 21.7 32.5
265 77.2 52.1 78.1

