
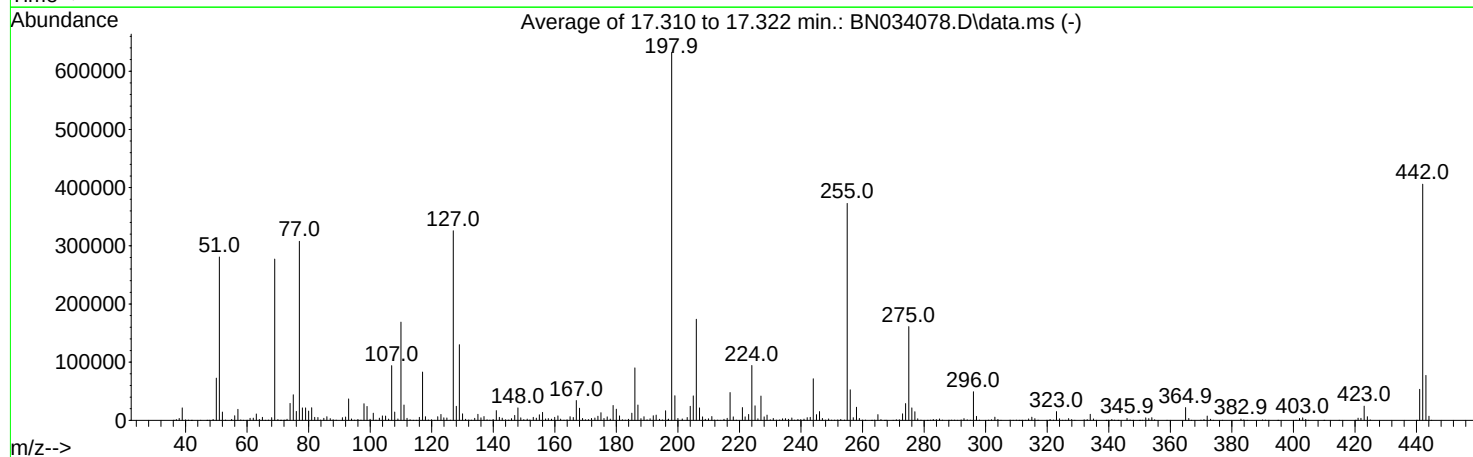


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034078.D
Acq On : 20 Sep 2024 09:36
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 18 16:09:28 2024

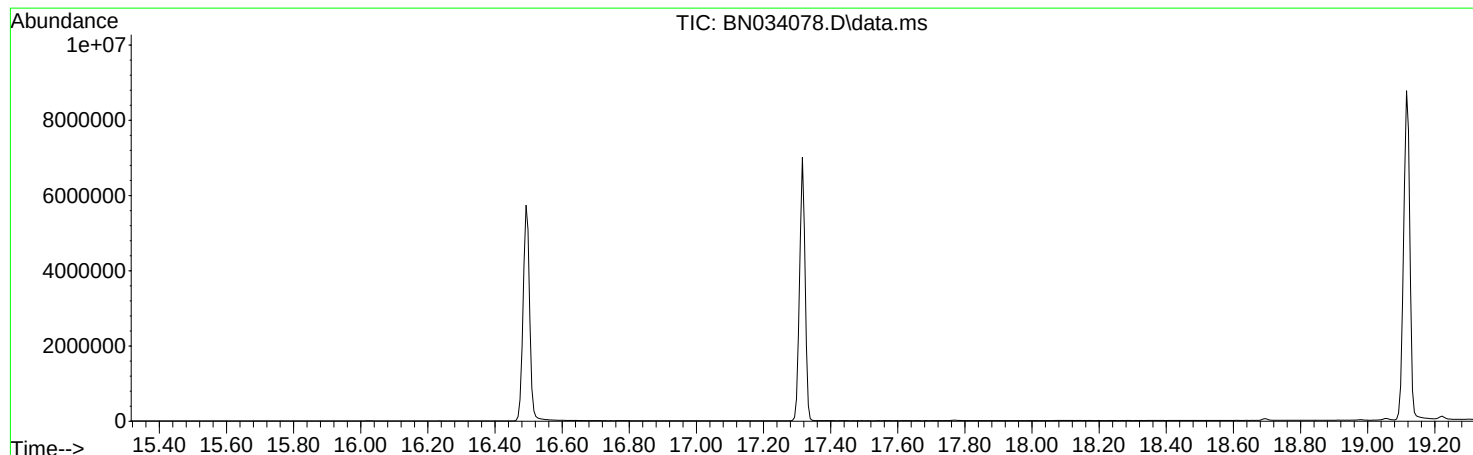

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	280679	PASS
68	69	0.00	2	1.7	4745	PASS
69	198	0.00	100	43.9	277269	PASS
70	69	0.00	2	0.5	1456	PASS
127	198	10	80	51.5	325696	PASS
197	198	0.00	2	0.4	2233	PASS
198	198	100	100	100.0	632149	PASS
199	198	5	9	6.7	42443	PASS
275	198	10	60	25.5	161096	PASS
365	198	1	100	3.5	22097	PASS
441	198	0.01	100	8.4	53325	PASS
442	442	50	100	100.0	405931	PASS
443	442	15	24	19.0	77272	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/21/2024	BNA_N	<u>BN034078.D</u>
Compound Name	Response	Retention Time
DDT	2182004	20.369
DDD	22370	19.969
DDE	248	19.416
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22618	2204622	1.03

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034078.D
Acq On : 20 Sep 2024 09:36
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 21 02:10:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:06:58 2024
Response via : Initial Calibration

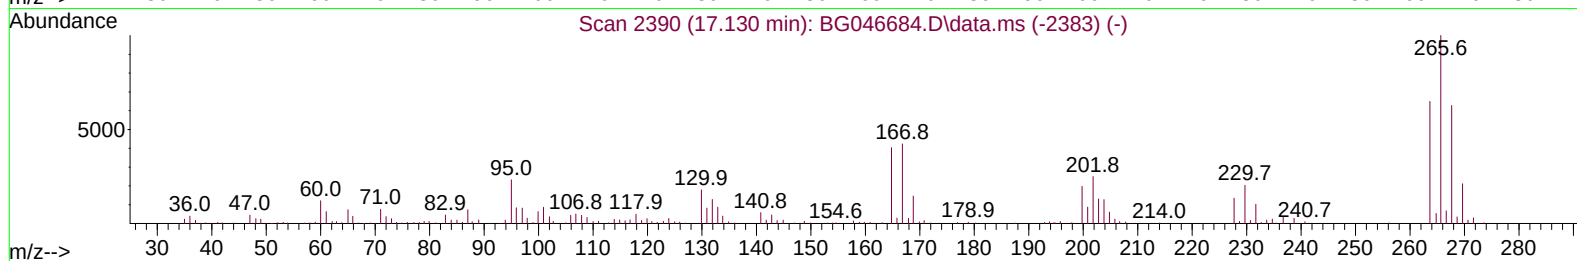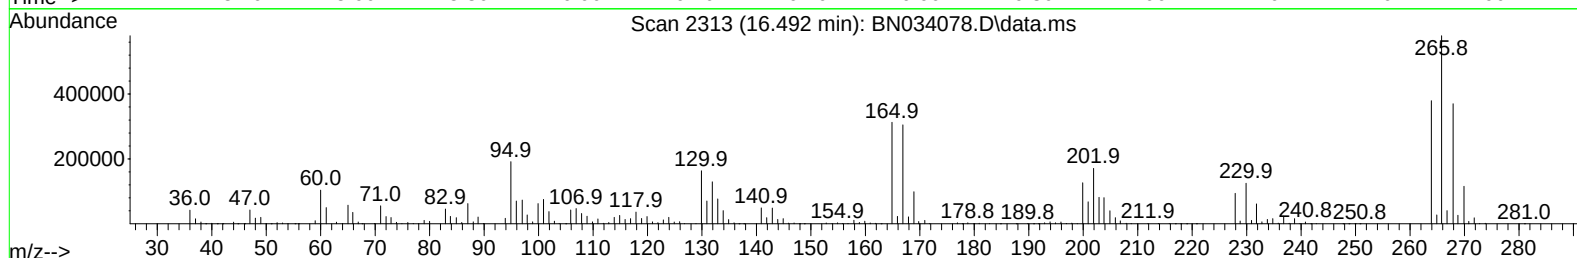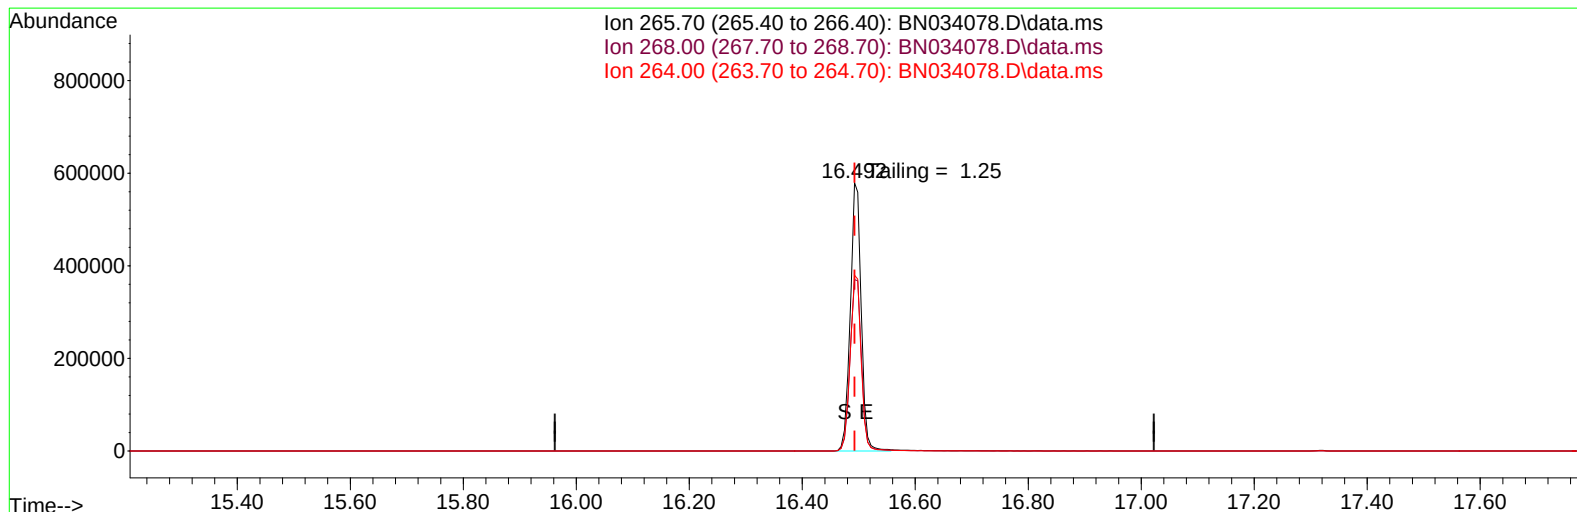

TIC: BN034078.D\data.ms

(70) Pentachlorophenol (C)

16.492min (-0.000) 24564.55 ng




response 783829

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.85
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092124\
Data File : BN034078.D
Acq On : 20 Sep 2024 09:36
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 21 02:10:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:06:58 2024
Response via : Initial Calibration

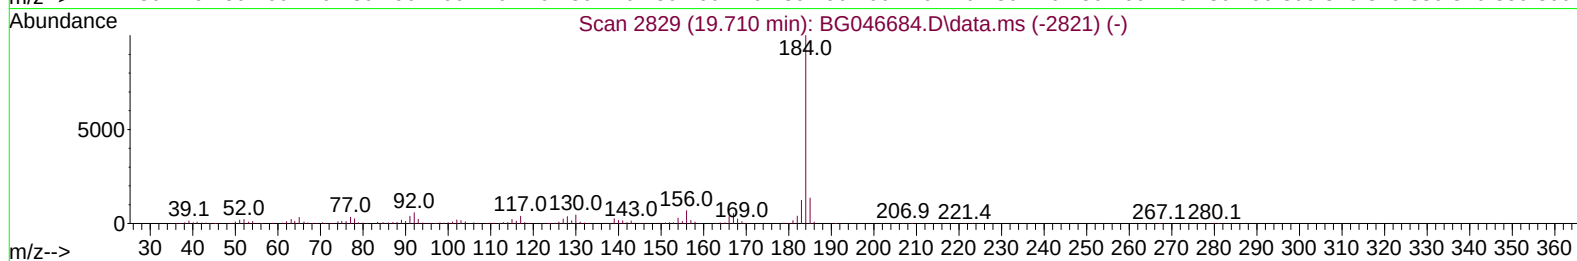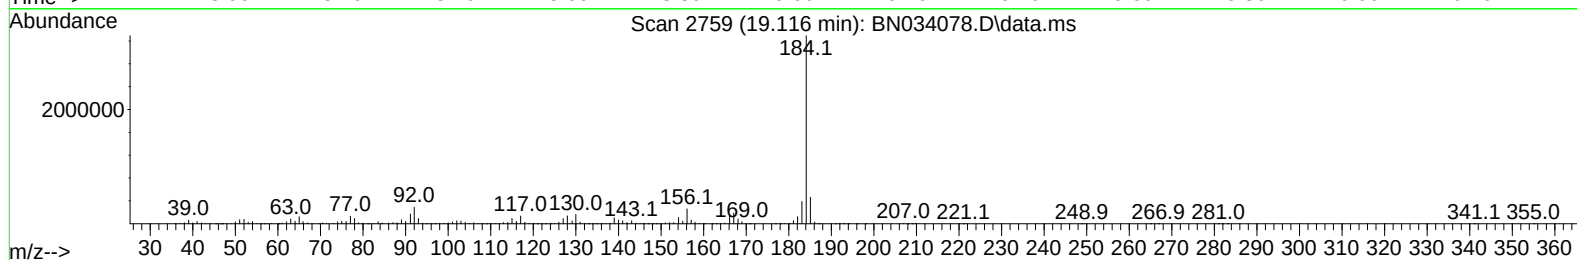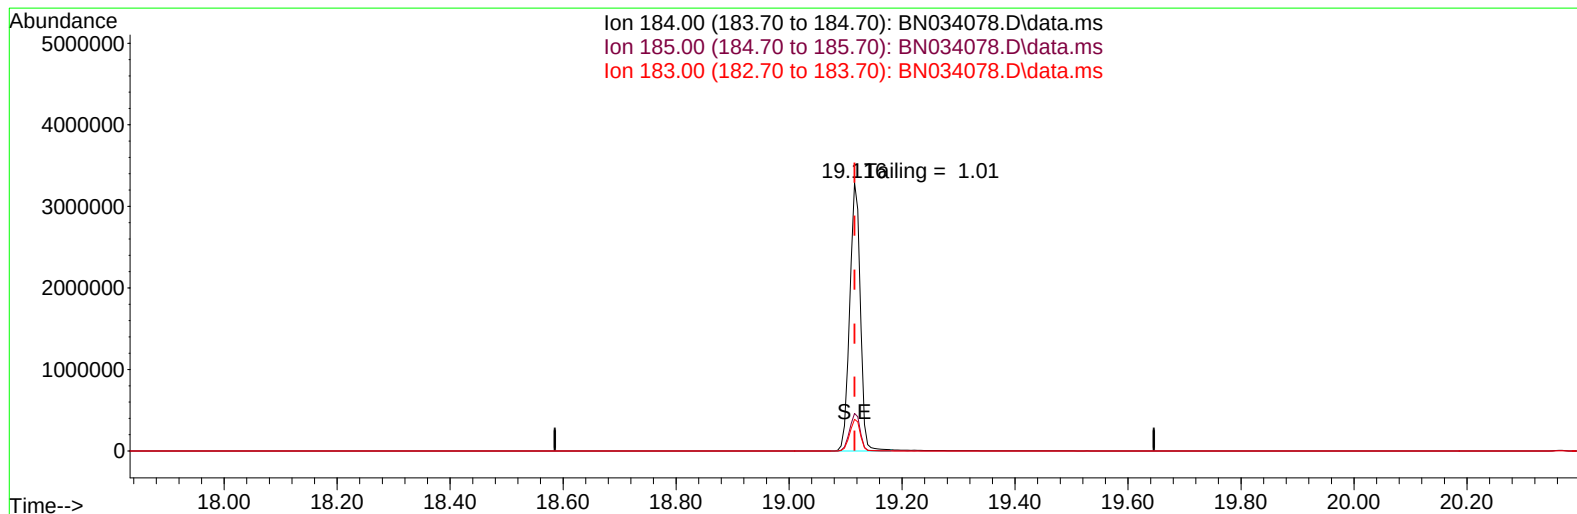

TIC: BN034078.D\data.ms

(77) Benzidine

19.116min (-0.000) 0.00 ng

response 4330600

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	11.84
0.00	0.00	0.00